

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071624\
 Data File : VU059970.D
 Acq On : 16 Jul 2024 13:28
 Operator : MD/SY
 Sample : P3217-22 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YDZJ8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	85	94	108	rBV	53028	68543	17.01%	1.995%
2	1.907	182	192	213	rBV	43002	64190	15.93%	1.868%
3	2.557	383	394	413	rBV	82001	136308	33.82%	3.967%
4	3.039	534	544	554	rBV2	7685	13510	3.35%	0.393%
5	4.624	1024	1037	1069	rBV	58139	151039	37.48%	4.396%
6	5.055	1154	1171	1196	rBV2	79696	179683	44.59%	5.230%
7	5.721	1357	1378	1406	rBV2	154975	403011	100.00%	11.730%
8	6.245	1529	1541	1570	rBV	152091	291027	72.21%	8.470%
9	6.685	1665	1678	1695	rBV	97630	190619	47.30%	5.548%
10	7.563	1939	1951	1974	rBV2	40400	74285	18.43%	2.162%
11	7.894	2039	2054	2072	rBV	164800	294265	73.02%	8.565%
12	8.180	2133	2143	2157	rBV	24715	42289	10.49%	1.231%
13	8.470	2221	2233	2243	rBV3	2495	5017	1.24%	0.146%
14	8.631	2273	2283	2315	rBV	193400	380146	94.33%	11.064%
15	9.415	2515	2527	2554	rBV	226425	386370	95.87%	11.245%
16	10.753	2927	2943	2963	rBV2	82451	135110	33.53%	3.932%
17	10.891	2977	2986	2998	rVB	4025	6179	1.53%	0.180%
18	11.811	3259	3272	3292	rBV	203023	335892	83.35%	9.776%
19	12.190	3378	3390	3412	rBV	157313	270350	67.08%	7.869%
20	14.576	4121	4132	4141	rBV	4953	7991	1.98%	0.233%




Sum of corrected areas: 3435824

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071624\
Data File : VU059970.D
Acq On : 16 Jul 2024 13:28
Operator : MD/SY
Sample : P3217-22 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

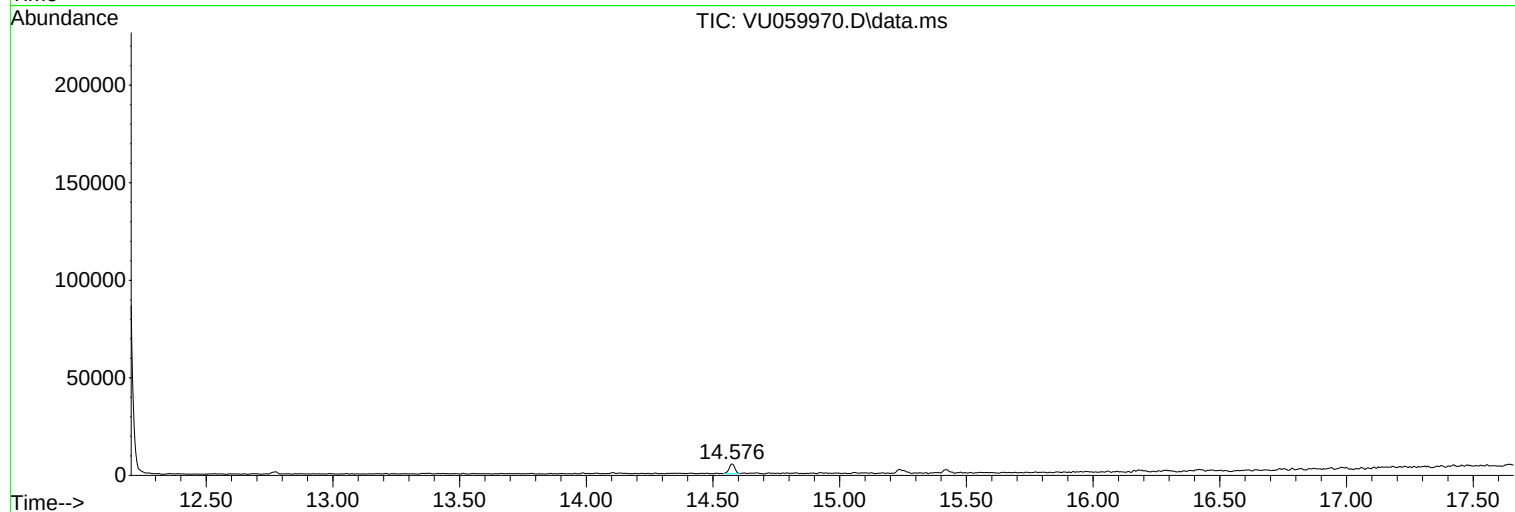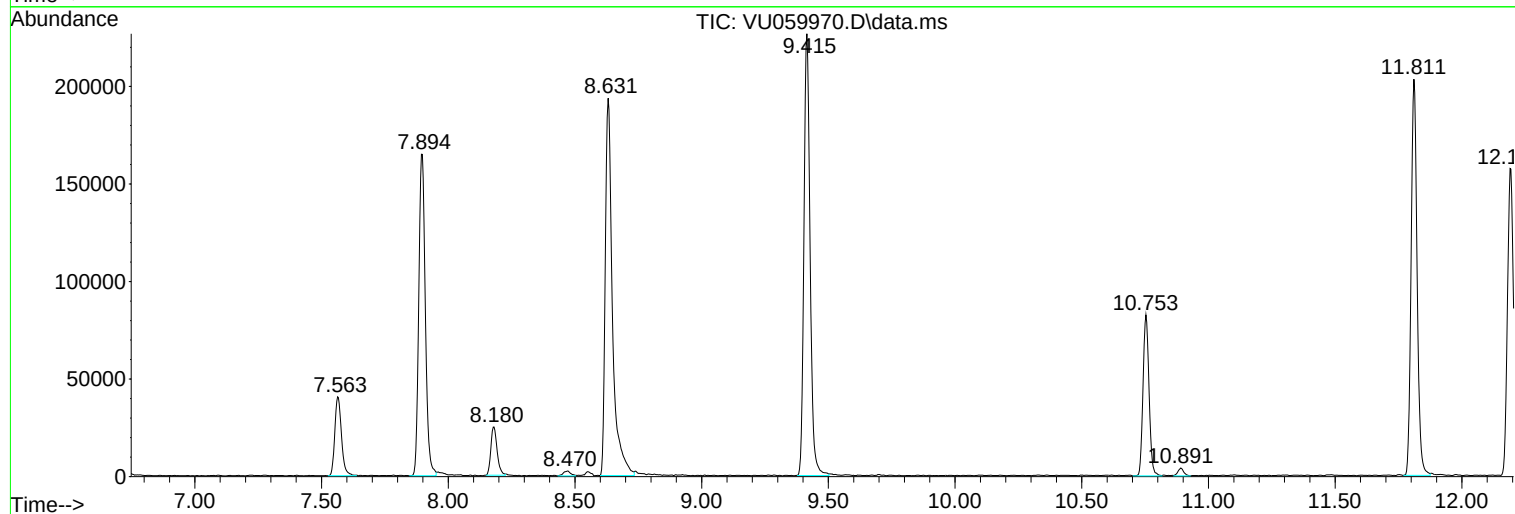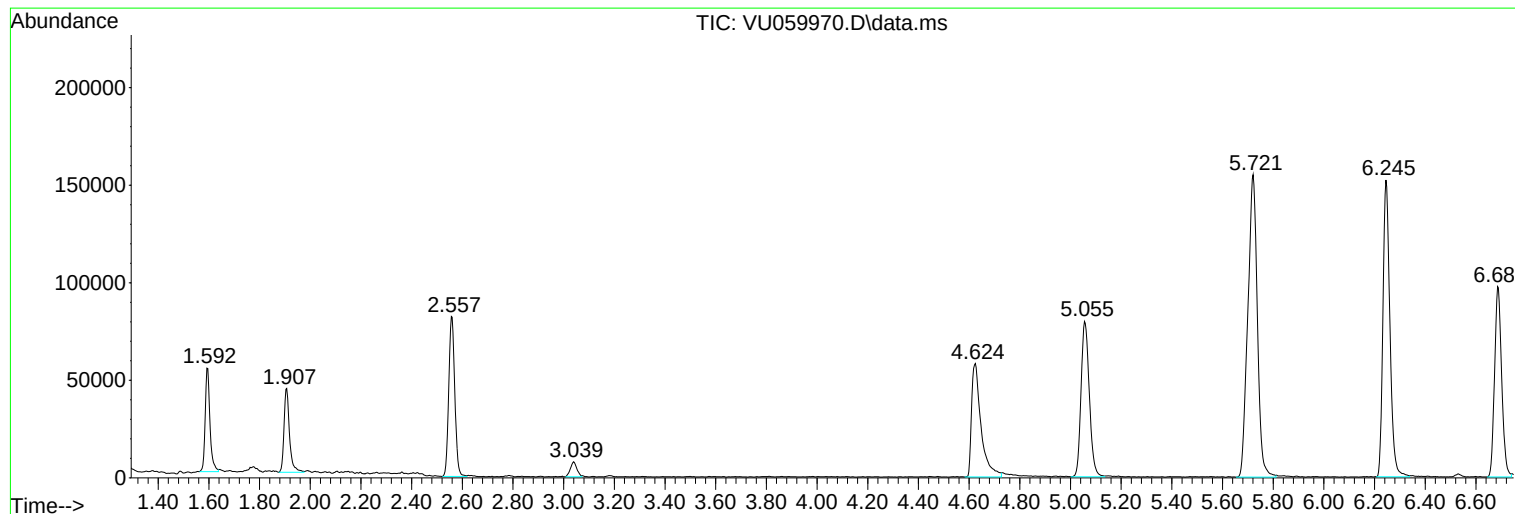

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071624\
Data File : VU059970.D
Acq On : 16 Jul 2024 13:28
Operator : MD/SY
Sample : P3217-22 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071624\
Data File : VU059970.D
Acq On : 16 Jul 2024 13:28
Operator : MD/SY
Sample : P3217-22 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZJ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc