
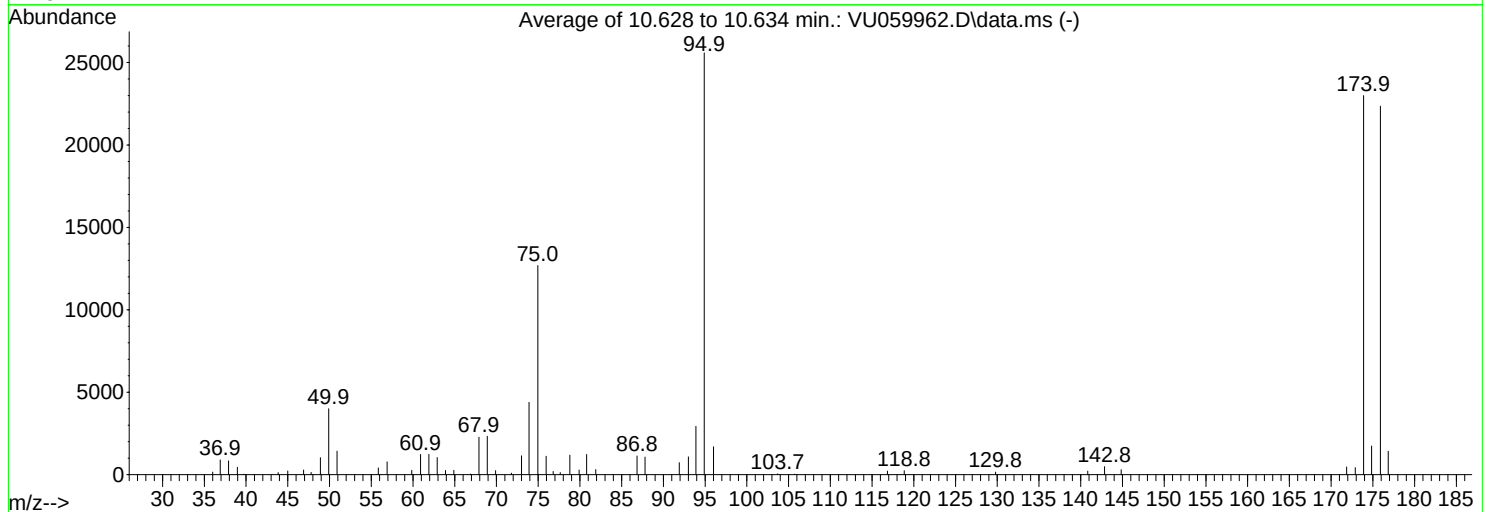


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071624\
Data File : VU059962.D
Acq On : 16 Jul 2024 08:39
Operator : MD/SY
Sample : BFB174
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB174

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Jul 17 02:25:31 2024

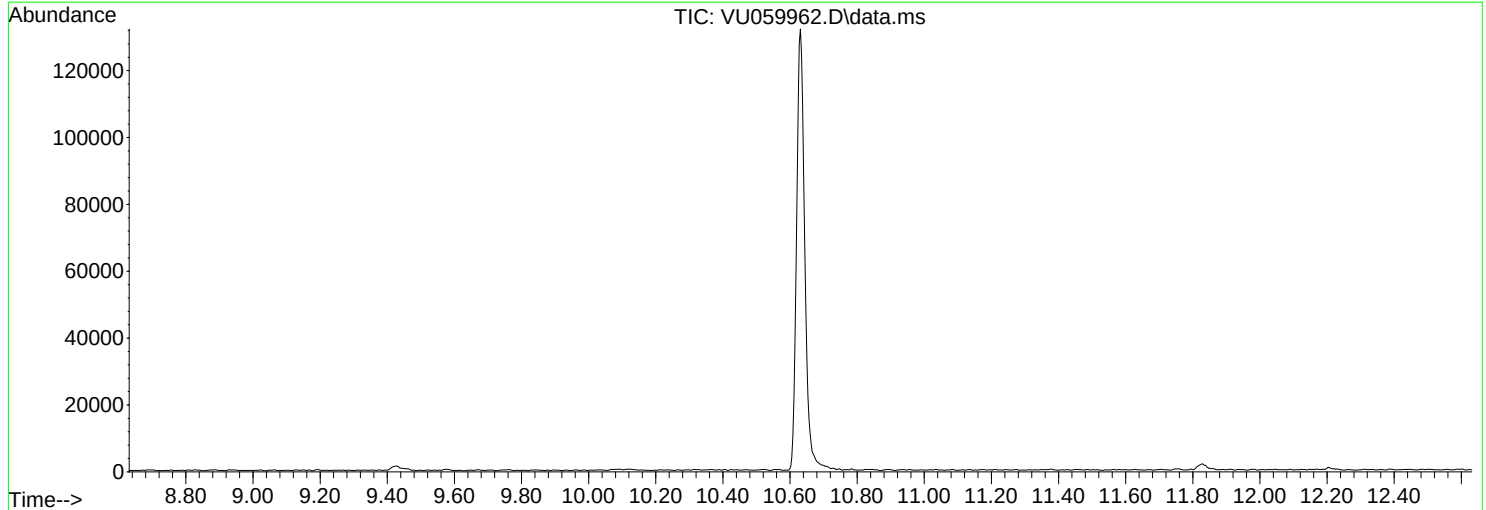

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.6	4004	PASS
75	95	30	80	49.6	12685	PASS
95	95	100	100	100.0	25589	PASS
96	95	5	9	6.6	1690	PASS
173	174	0.00	2	1.9	432	PASS
174	95	50	120	89.9	22997	PASS
175	174	5	9	7.6	1741	PASS
176	174	95	101	97.2	22352	PASS
177	176	5	9	6.3	1415	PASS

Scan 2892 (10.589 min): VU059962.D\data.ms
BFB174

m/z	Abundance
39.70	213.0
43.80	293.0

Instrument :
MSVOA_U
ClientSampleId :
BFB174

m/z	Abundance
36.00	130.0
36.90	843.0
37.90	826.0
39.00	409.0
39.80	254.0
43.90	392.0
45.00	187.0
46.90	244.0
47.80	136.0
48.90	1009.0
49.90	4141.0
50.90	1413.0
55.80	407.0
56.90	840.0
59.80	251.0
60.90	1320.0
61.90	1218.0
62.90	1059.0
63.90	284.0
65.00	249.0
67.90	2430.0
68.90	2322.0
69.90	280.0
71.80	154.0
73.00	1109.0
73.90	4447.0
75.00	12671.0
75.90	1213.0
76.80	159.0
77.70	103.0
78.80	1152.0
79.90	256.0
80.80	1196.0
81.90	328.0
86.90	1204.0
87.80	1071.0
91.90	734.0
93.00	1046.0
93.90	2906.0
94.90	25928.0
96.00	1847.0
103.70	136.0
105.70	102.0
116.80	265.0
118.80	217.0
129.80	194.0
140.80	170.0
142.90	492.0
144.80	332.0
171.80	433.0
172.90	369.0
173.90	22808.0
174.80	1650.0
175.90	21496.0
176.90	1325.0

Instrument :
MSVOA_U
ClientSampleId :
BFB174

m/z	Abundance
36.00	161.0
36.90	908.0
37.90	849.0
38.90	468.0
39.80	231.0
43.90	406.0
45.00	240.0
46.90	312.0
47.80	136.0
48.90	1093.0
49.90	4197.0
50.90	1492.0
55.90	430.0
56.90	808.0
59.80	264.0
60.90	1272.0
61.90	1230.0
62.90	1058.0
63.90	260.0
65.00	229.0
67.90	2295.0
68.90	2407.0
69.90	244.0
71.80	122.0
73.00	1204.0
73.90	4581.0
75.00	13182.0
76.00	1129.0
76.80	193.0
77.60	137.0
78.80	1217.0
79.90	285.0
80.80	1264.0
81.90	326.0
86.90	1170.0
87.80	1083.0
91.90	755.0
93.00	1145.0
93.90	3038.0
94.90	26304.0
96.00	1725.0
116.90	215.0
118.80	251.0
129.80	165.0
140.80	210.0
142.80	474.0
144.80	315.0
171.80	503.0
172.90	462.0
173.90	23728.0
174.90	1808.0
175.90	22936.0
176.90	1490.0

Instrument :
MSVOA_U
ClientSampleId :
BFB174

m/z	Abundance
36.00	179.0
36.90	936.0
37.90	839.0
38.90	468.0
39.80	235.0
43.90	460.0
45.00	248.0
46.90	303.0
47.80	125.0
48.90	996.0
49.90	3675.0
50.90	1372.0
55.90	391.0
56.90	672.0
59.90	261.0
60.90	1086.0
61.90	1253.0
62.90	1009.0
63.90	223.0
64.80	299.0
66.90	106.0
67.90	2095.0
68.90	2266.0
69.90	216.0
73.00	1120.0
73.90	4131.0
74.90	12203.0
76.00	1022.0
76.80	218.0
77.60	148.0
78.80	1179.0
79.90	304.0
80.80	1220.0
81.90	266.0
86.80	1025.0
87.80	1047.0
91.90	682.0
93.00	1056.0
93.90	2862.0
94.90	24536.0
96.00	1499.0
116.90	157.0
118.90	249.0
129.80	119.0
140.90	258.0
142.80	483.0
144.90	263.0
171.90	468.0
172.90	465.0
173.90	22456.0
174.90	1764.0
175.90	22624.0
176.80	1430.0

Instrument :
MSVOA_U
ClientSampleId :
BFB174