



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
Data File : VU063510.D
Acq On : 16 Jul 2025 08:13
Operator : MD/SY
Sample : BFB
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Jul 17 03:49:40 2025

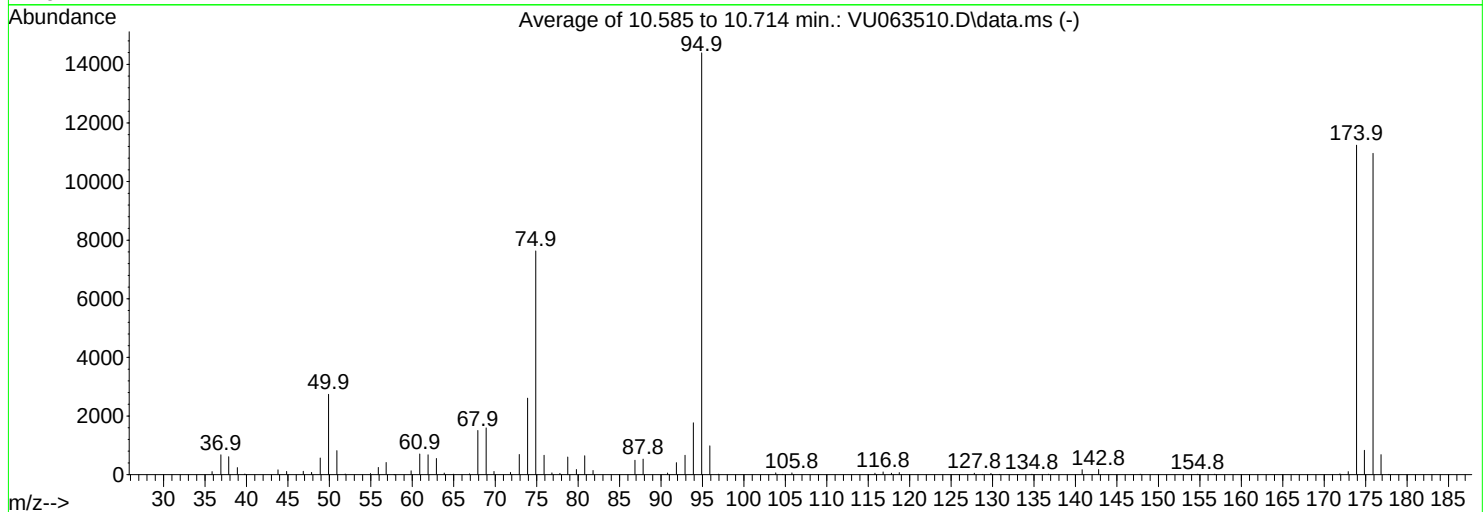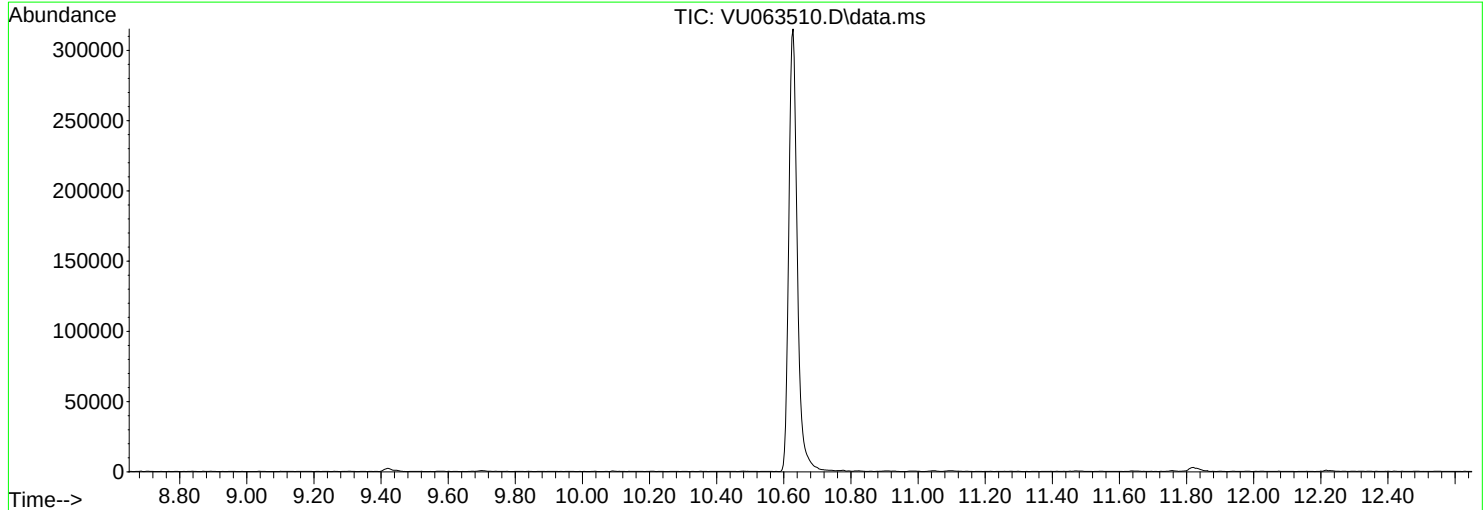

AutoFind: Averaged scan 2891 to 2931; Bkg corrected with scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	2743	PASS
75	95	30	60	53.0	7631	PASS
95	95	100	100	100.0	14392	PASS
96	95	5	9	6.8	984	PASS
173	174	0.00	2	0.9	104	PASS
174	95	50	100	78.1	11242	PASS
175	174	5	9	7.4	829	PASS
176	174	95	101	97.5	10965	PASS
177	176	5	9	6.2	681	PASS