

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071718\
 Data File : VU025481.D
 Acq On : 18 Jul 2018 01:12
 Operator : MD/SY
 Sample : J4024-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1S0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.661	16	22	26	rVB3	801	866	0.08%	0.010%
2	0.687	26	30	33	rBV2	920	796	0.08%	0.009%
3	0.863	83	85	86	rBV	509	117	0.01%	0.001%
4	0.873	86	88	90	rBV2	357	166	0.02%	0.002%
5	1.089	148	155	175	rBV	235160	270856	25.69%	3.161%
6	1.400	247	252	266	rVB	108119	114597	10.87%	1.337%
7	1.683	334	340	350	rVB	90152	107086	10.16%	1.250%
8	2.275	515	524	536	rBV	198523	295210	28.00%	3.445%
9	2.738	666	668	670	rBV2	383	130	0.01%	0.002%
10	3.043	761	763	766	rBV2	289	186	0.02%	0.002%
11	3.114	781	785	789	rBV3	647	594	0.06%	0.007%
12	3.384	865	869	870	rBV	640	450	0.04%	0.005%
13	3.523	910	912	914	rBV2	434	270	0.03%	0.003%
14	3.706	967	969	971	rBV	353	200	0.02%	0.002%
15	3.757	984	985	987	rVB	327	96	0.01%	0.001%
16	3.876	1020	1022	1023	rBV	258	132	0.01%	0.002%
17	3.889	1023	1026	1028	rVV3	442	281	0.03%	0.003%
18	4.021	1065	1067	1069	rBV	599	308	0.03%	0.004%
19	4.053	1073	1077	1081	rVV3	506	449	0.04%	0.005%
20	4.092	1087	1089	1092	rBV2	654	299	0.03%	0.003%
21	4.178	1101	1116	1142	rBV	92476	237815	22.55%	2.775%
22	4.548	1230	1231	1234	rBV	249	148	0.01%	0.002%
23	4.654	1247	1264	1283	rBV	184589	432187	40.99%	5.043%
24	4.770	1296	1300	1305	rVB4	1060	882	0.08%	0.010%
25	4.802	1305	1310	1314	rBV7	867	879	0.08%	0.010%
26	4.931	1348	1350	1352	rBV2	349	142	0.01%	0.002%
27	5.079	1390	1396	1398	rBV3	893	733	0.07%	0.009%
28	5.133	1411	1413	1414	rBV	328	113	0.01%	0.001%
29	5.198	1431	1433	1435	rBV	254	111	0.01%	0.001%
30	5.346	1453	1479	1498	rBV2	348219	1054426	100.00%	12.305%
31	5.664	1576	1578	1582	rBV4	445	293	0.03%	0.003%
32	5.776	1610	1613	1614	rBV	373	205	0.02%	0.002%
33	5.809	1622	1623	1625	rBV	362	161	0.02%	0.002%
34	5.889	1634	1648	1665	rBV	387577	760203	72.10%	8.871%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071718\
 Data File : VU025481.D
 Acq On : 18 Jul 2018 01:12
 Operator : MD/SY
 Sample : J4024-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1S0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
 Title : VOC Analysis

35	6.336	1772	1787	1805	rBV	247646	491461	46.61%	5.735%
36	6.452	1820	1823	1824	rBV2	498	274	0.03%	0.003%
37	6.600	1866	1869	1870	rBV	276	154	0.01%	0.002%
38	6.648	1881	1884	1887	rBV	493	358	0.03%	0.004%
39	6.702	1899	1901	1903	rBV	447	239	0.02%	0.003%
40	6.792	1927	1929	1932	rBV3	467	333	0.03%	0.004%
41	6.899	1959	1962	1965	rBV3	538	357	0.03%	0.004%
42	7.169	2044	2046	2049	rBV2	418	273	0.03%	0.003%
43	7.185	2049	2051	2053	rBV2	548	311	0.03%	0.004%
44	7.230	2053	2065	2082	rVV	136111	242665	23.01%	2.832%
45	7.310	2088	2090	2091	rBV	385	144	0.01%	0.002%
46	7.567	2156	2170	2199	rBV	483347	841883	79.84%	9.824%
47	7.850	2248	2258	2279	rVB2	97370	164236	15.58%	1.917%
48	8.146	2348	2350	2351	rBV	614	239	0.02%	0.003%
49	8.313	2391	2402	2430	rVB	299084	511005	48.46%	5.963%
50	8.706	2520	2524	2525	rBV	582	367	0.03%	0.004%
51	9.091	2631	2644	2671	rBV	531230	879795	83.44%	10.267%
52	9.632	2810	2812	2819	rVB4	547	459	0.04%	0.005%
53	10.185	2982	2984	2986	rBV	474	237	0.02%	0.003%
54	10.435	3050	3062	3081	rBV	339856	546115	51.79%	6.373%
55	11.487	3376	3389	3405	rBV	516292	816579	77.44%	9.529%
56	11.863	3493	3506	3522	rBV	497072	789822	74.91%	9.217%
57	12.140	3589	3592	3594	rBV2	581	324	0.03%	0.004%
58	12.284	3635	3637	3641	rBV2	550	274	0.03%	0.003%


Sum of corrected areas: 8569291

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU071718\
Data File : VU025481.D
Acq On : 18 Jul 2018 01:12
Operator : MD/SY
Sample : J4024-14
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB1S0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

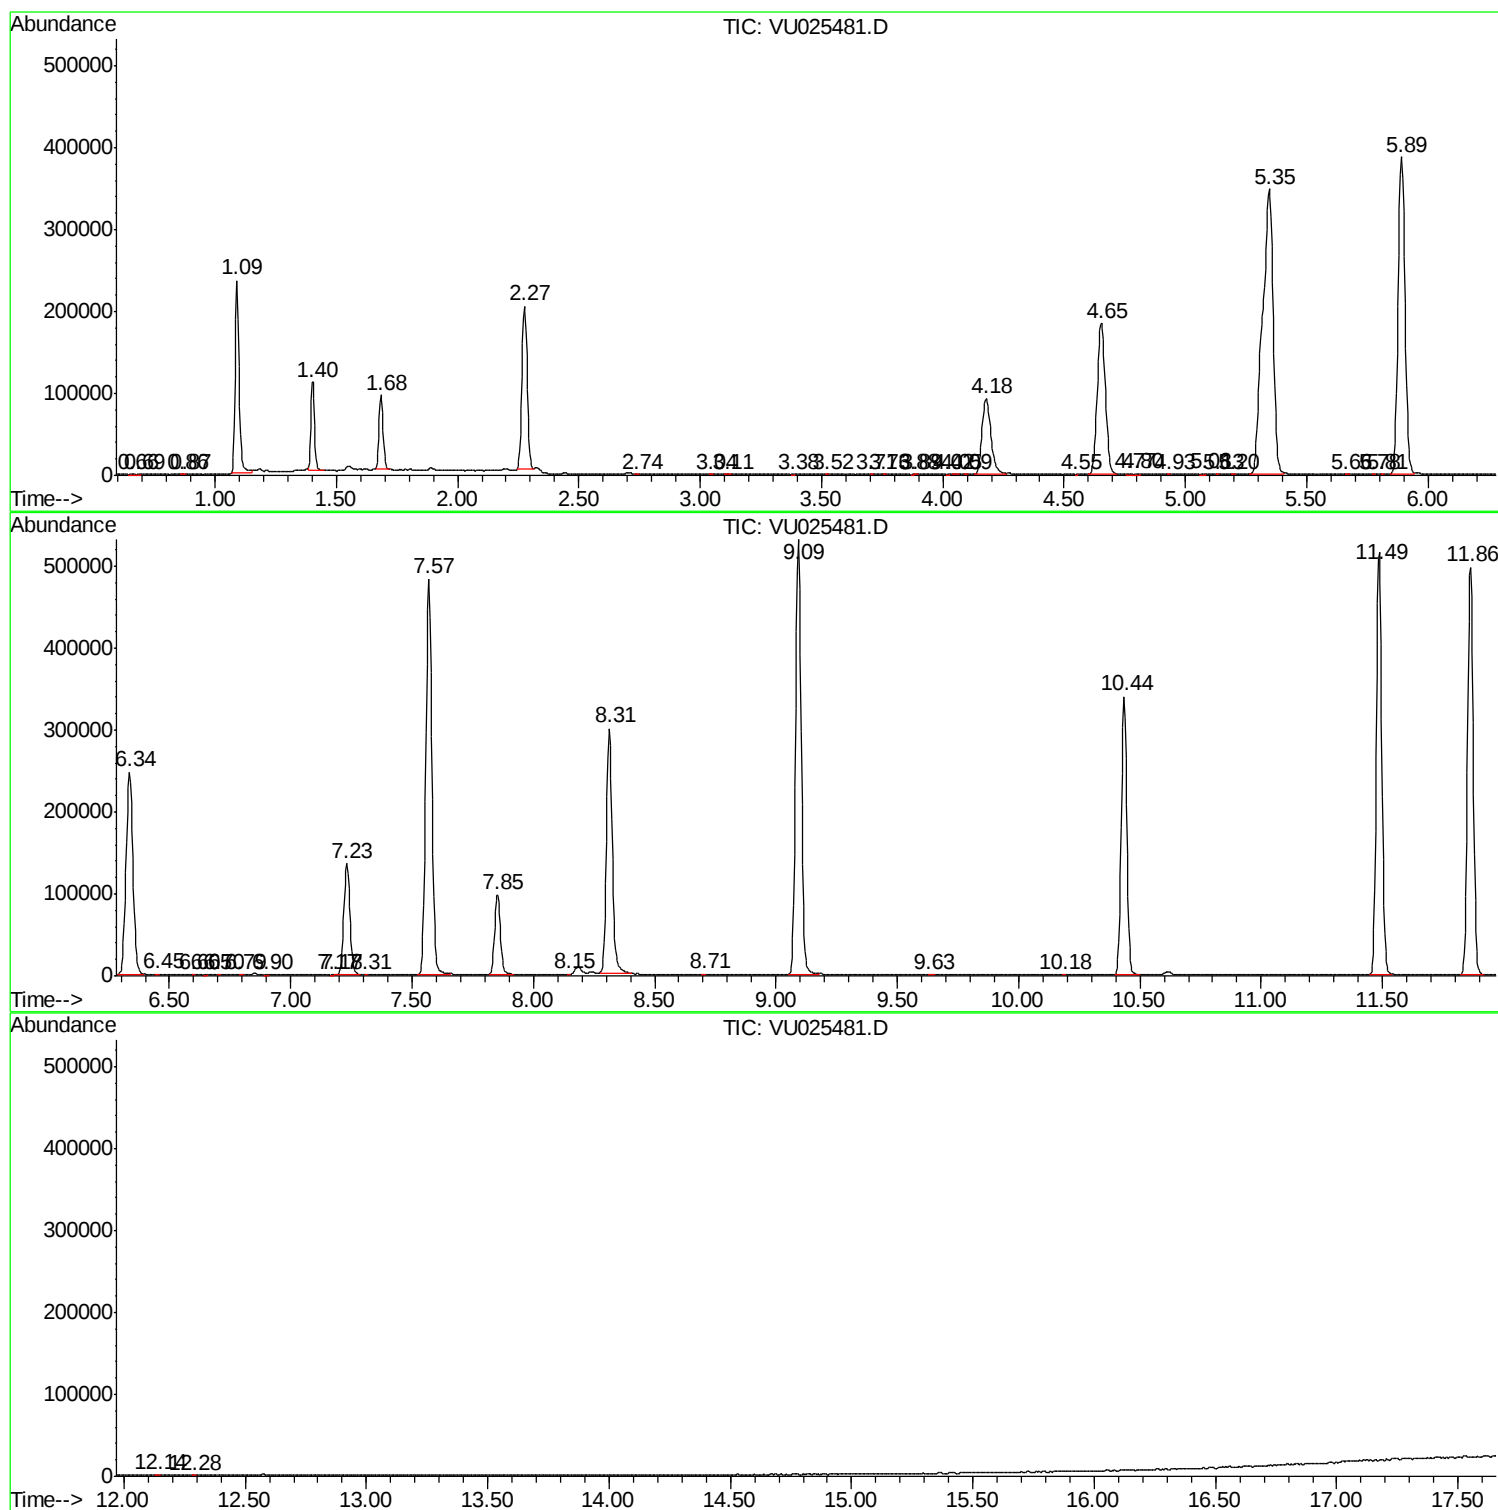

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071718\
Data File : VU025481.D
Acq On : 18 Jul 2018 01:12
Operator : MD/SY
Sample : J4024-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB1S0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071718\
Data File : VU025481.D
Acq On : 18 Jul 2018 01:12
Operator : MD/SY
Sample : J4024-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB1S0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc