


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071718\
Data File : VU025452.D
Acq On : 17 Jul 2018 10:04
Operator : MD/SY
Sample : BFB38
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB38

Integration File: LSCINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
Title : VOC Analysis
Last Update : Thu Jul 19 01:07:14 2018

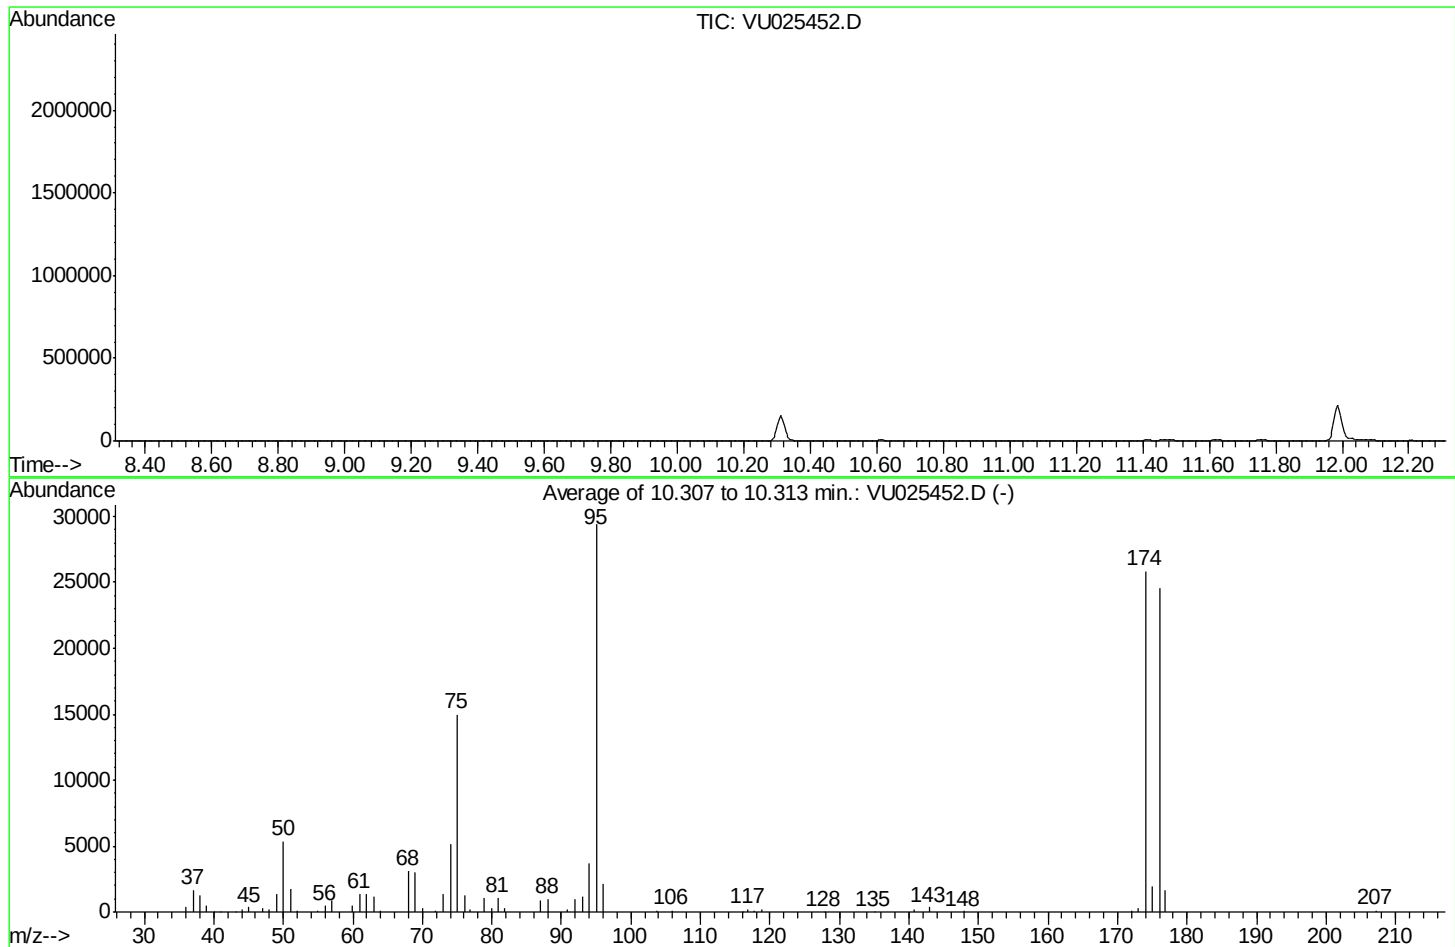

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	5341	PASS
75	95	30	80	51.0	14998	PASS
95	95	100	100	100.0	29400	PASS
96	95	5	9	7.3	2133	PASS
173	174	0.00	2	1.1	284	PASS
174	95	50	120	88.0	25864	PASS
175	174	5	9	7.4	1906	PASS
176	174	95	101	95.1	24594	PASS
177	176	5	9	6.7	1637	PASS

Scan 3011 (10.271 min): VU025452.D
BFB38

m/z	Abundance
35.90	487.0
37.90	175.0
40.00	127.0
40.90	111.0
44.00	529.0
207.00	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
35.90	939.0
37.00	1753.0
38.00	1449.0
39.00	490.0
39.90	222.0
41.00	139.0
44.00	816.0
45.00	408.0
46.90	315.0
48.00	145.0
49.00	1346.0
50.00	5359.0
51.00	1630.0
52.00	125.0
56.00	408.0
57.00	794.0
59.90	469.0
61.00	1445.0
62.00	1351.0
63.00	1069.0
63.90	118.0
68.00	3010.0
69.00	2924.0
70.00	261.0
71.90	152.0
73.00	1311.0
74.00	4708.0
75.00	14338.0
76.00	1153.0
76.90	265.0
78.90	937.0
79.90	318.0
80.90	1106.0
81.80	216.0
87.00	856.0
88.00	911.0
90.80	135.0
92.00	899.0
93.00	1118.0
94.00	3596.0
95.00	28352.0
96.00	2077.0
103.70	130.0
105.80	162.0
116.90	236.0
117.80	115.0
118.80	184.0
135.00	101.0
140.80	221.0
142.90	310.0
173.10	237.0
174.00	24384.0
175.00	1814.0
176.00	22848.0
176.90	1747.0
207.20	186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
35.90	942.0
37.00	1760.0
38.00	1489.0
39.00	491.0
39.90	163.0
41.00	152.0
43.10	103.0
44.00	800.0
45.00	391.0
46.90	321.0
48.00	165.0
49.00	1412.0
50.00	5500.0
51.00	1815.0
52.00	133.0
54.90	113.0
56.00	467.0
57.00	885.0
59.90	487.0
61.00	1441.0
62.00	1414.0
63.00	1157.0
63.90	123.0
68.00	3252.0
69.00	3118.0
69.90	254.0
71.90	109.0
73.00	1472.0
74.00	5384.0
75.00	15508.0
76.10	1249.0
76.90	251.0
78.90	1088.0
79.90	339.0
80.90	1140.0
81.80	272.0
87.00	920.0
88.00	1011.0
90.90	174.0
92.00	996.0
93.00	1187.0
94.00	3825.0
95.00	30376.0
96.00	2184.0
103.70	139.0
105.90	142.0
116.80	259.0
117.80	127.0
118.80	151.0
140.80	245.0
142.90	374.0
147.90	107.0
172.00	133.0
173.10	271.0
174.00	26816.0
175.00	1953.0
176.00	25368.0
176.90	1700.0
207.10	159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
35.90	893.0
37.00	1478.0
38.00	1379.0
39.00	479.0
40.00	134.0
41.00	149.0
44.00	693.0
45.00	323.0
47.00	298.0
47.90	193.0
49.00	1368.0
50.00	5166.0
51.00	1910.0
52.00	127.0
54.90	116.0
56.00	465.0
57.00	837.0
59.90	464.0
61.00	1338.0
62.00	1398.0
63.00	1202.0
63.90	130.0
68.00	3129.0
69.00	3085.0
69.90	260.0
73.00	1424.0
74.00	5346.0
75.00	15148.0
76.10	1315.0
76.90	193.0
78.90	1132.0
79.90	308.0
80.90	1002.0
81.80	277.0
87.00	943.0
88.00	1097.0
90.90	210.0
92.00	938.0
93.00	1198.0
94.00	3671.0
95.00	29472.0
96.00	2139.0
103.70	127.0
105.90	107.0
116.00	118.0
116.80	205.0
117.80	116.0
118.90	158.0
127.80	116.0
140.80	270.0
142.90	380.0
147.90	124.0
172.00	168.0
172.90	344.0
174.00	26392.0
175.00	1952.0
176.00	25568.0
176.90	1465.0
206.90	170.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38