

Data File : VU033279.D
Acq On : 17 Jul 2019 09:56
Operator : JC/SP
Sample : K3772-01DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A52T8DL

Quant Time: Jul 18 08:04:10 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR071619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 18 08:01:21 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	128525	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	135493	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	59755	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	58388	4.51	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.20%
7) Chloroethane-d5	1.67	69	54309	5.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.60%
11) 1,1-Dichloroethene-d2	2.26	63	94780	3.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.80%
20) 2-Butanone-d5	4.17	46	122520	50.23	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.46%
24) Chloroform-d	4.62	84	94857	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.40%
26) 1,2-Dichloroethane-d4	5.29	65	52094	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.00%
32) Benzene-d6	5.32	84	181363	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.20%
36) 1,2-Dichloropropane-d6	6.31	67	58530	4.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.40%
41) Toluene-d8	7.55	98	160618	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.00%
43) trans-1,3-Dichloropropene-	7.84	79	22646	4.71	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.20%
46) 2-Hexanone-d5	8.30	63	97355	49.26	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.52%
57) 1,1,2,2-Tetrachloroethane-	10.42	84	49781	4.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.80%
64) 1,2-Dichlorobenzene-d4	11.85	152	59204	5.09	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.80%

Target Compounds

					Qvalue
6) Bromomethane	1.62	94	5876	0.670 ug/L	93
12) 1,1-Dichloroethene	2.27	96	6948	0.658 ug/L	# 1
13) Acetone	2.32	43	38677	18.111 ug/L	82
14) Carbon disulfide	2.46	76	76257	2.231 ug/L	100
15) Methyl Acetate	2.60	43	52496	9.842 ug/L	98
16) Methylene chloride	2.68	84	18089	1.405 ug/L	93
17) Methyl tert-butyl Ether	2.99	73	81759	2.956 ug/L	99
21) 2-Butanone	4.26	43	24414	9.947 ug/L	96
22) cis-1,2-Dichloroethene	4.20	96	16847	1.709 ug/L	97
25) Chloroform	4.65	83	3806	0.196 ug/L	96
27) 1,2-Dichloroethane	5.39	62	16910	1.464 ug/L	98
30) Cyclohexane	4.97	56	35562	2.530 ug/L	99
33) Benzene	5.37	78	51554	1.344 ug/L	100
34) Trichloroethene	6.16	95	9563	0.942 ug/L	96
35) Methylcyclohexane	6.39	83	73118	4.779 ug/L	97
40) 4-Methyl-2-pentanone	7.45	43	38419	6.461 ug/L	98
42) Toluene	7.62	91	166831	4.050 ug/L	100

Data File : VU033279.D
Acq On : 17 Jul 2019 09:56
Operator : JC/SP
Sample : K3772-01DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A52T8DL

Quant Time: Jul 18 08:04:10 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR071619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 18 08:01:21 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) trans-1,3-Dichloropropene	7.83	75	1442	0.120	ug/L	85
47) Tetrachloroethene	8.21	164	9333	1.147	ug/L	97
48) 2-Hexanone	8.35	43	30677	7.054	ug/L	97
49) Dibromochloromethane	8.21	129	9314	1.042	ug/L #	12
50) 1,2-Dibromoethane	8.58	107	3502	0.492	ug/L #	97
52) Ethylbenzene	9.23	91	97121	2.209	ug/L	100
53) m,p-Xylene	9.36	106	32562	1.960	ug/L	91
59) 1,2,3-Trichloropropane	11.47	75	7895	1.167	ug/L	91
62) 1,3-Dichlorobenzene	11.40	146	27377	1.533	ug/L	98
63) 1,4-Dichlorobenzene	11.40	146	27377	1.456	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU033279.D
Acq On : 17 Jul 2019 09:56
Operator : JC/SP
Sample : K3772-01DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A52T8DL

Quant Time: Jul 18 08:04:10 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR071619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 18 08:01:21 2019
Response via : Initial Calibration

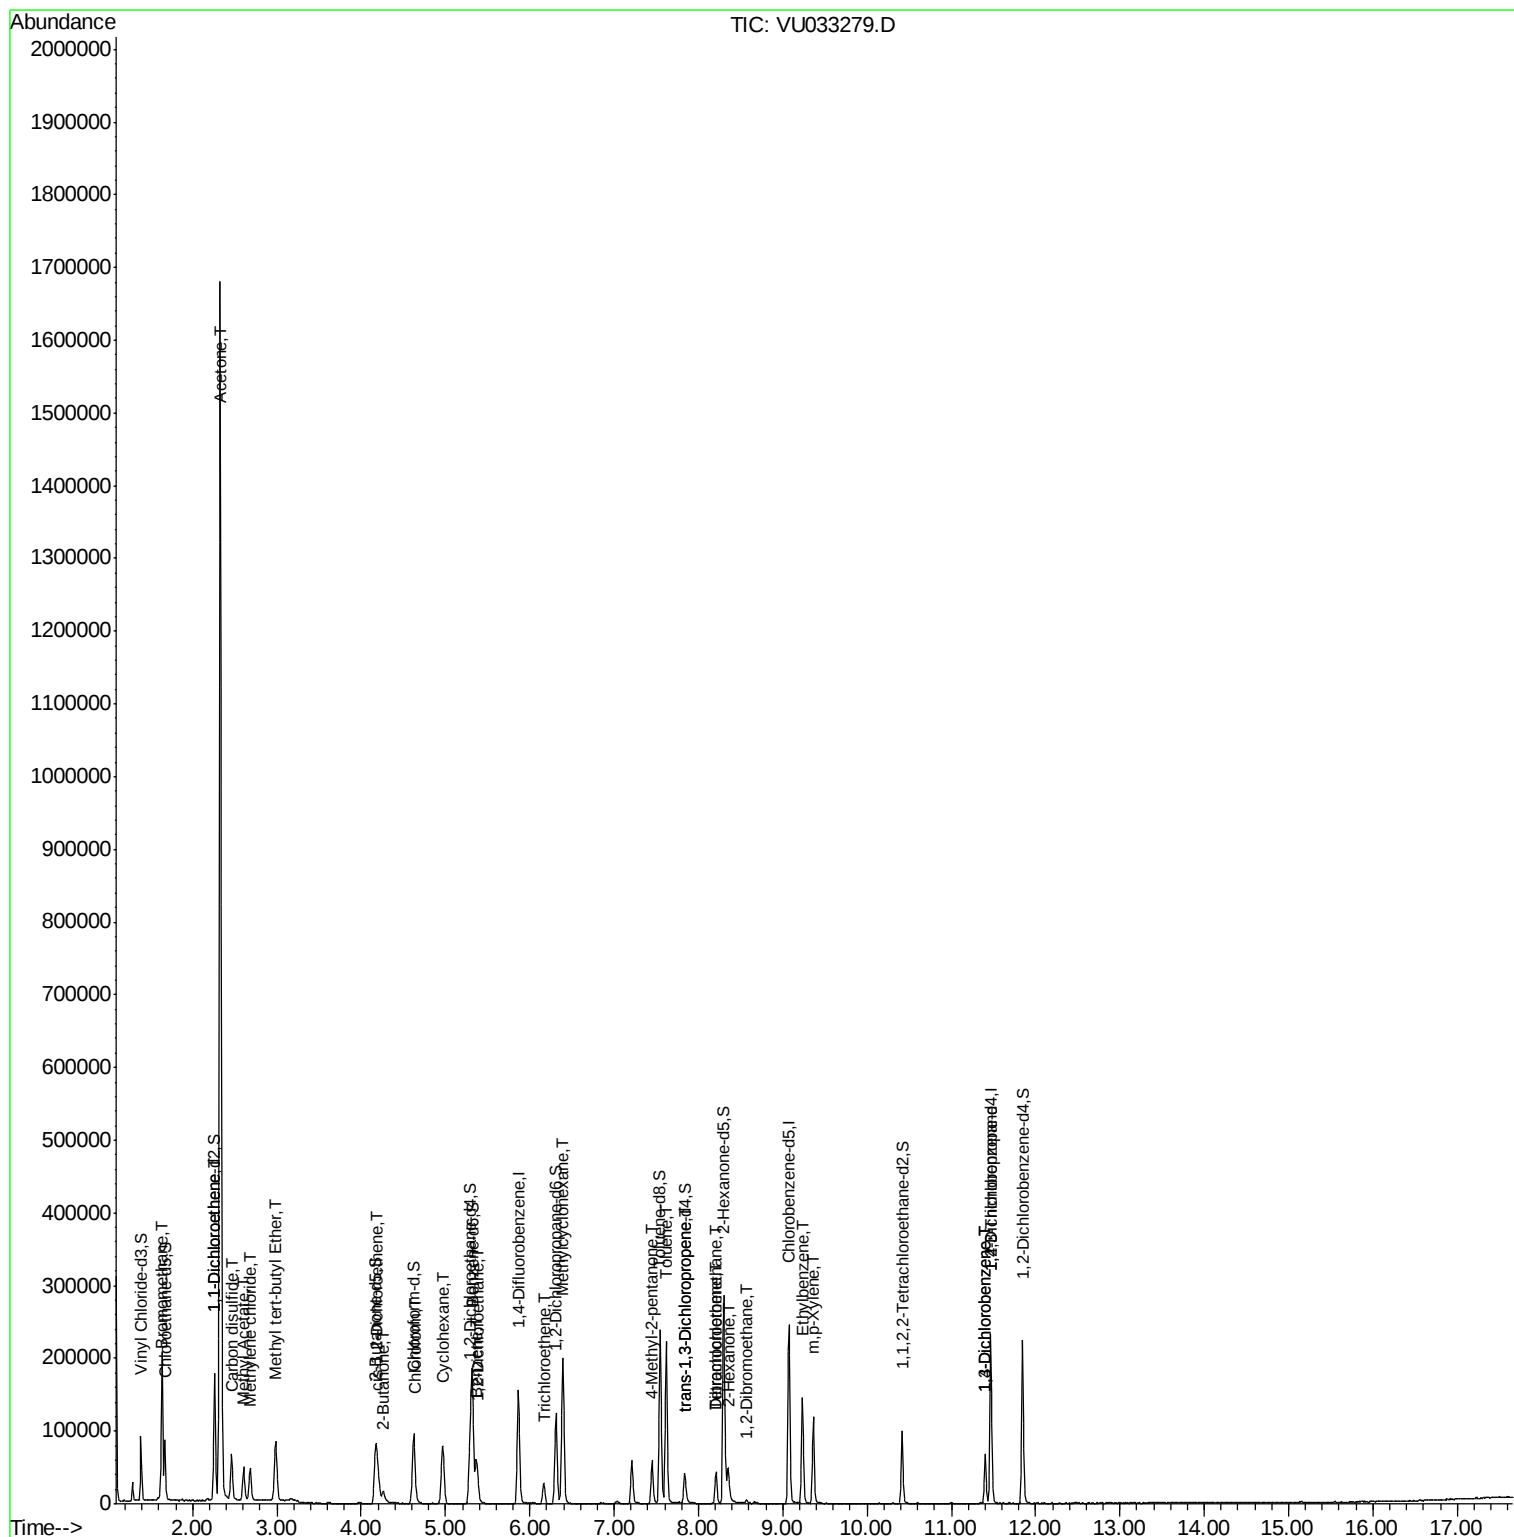

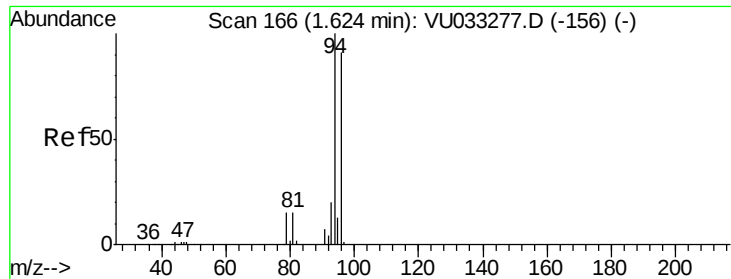

#6

Bromomethane

Concen: 0.670 ug/L

RT: 1.62 min Scan# 165

Delta R.T. -0.00 min

Lab File: VU033279.D

Acq: 17 Jul 2019 09:56

Instrument :

MSVOA_U

ClientSampled :


A52T8DL

Tgt Ion: 94 Resp: 5876

Ion Ratio Lower Upper




94 100

96 96.1 62.4 116.0

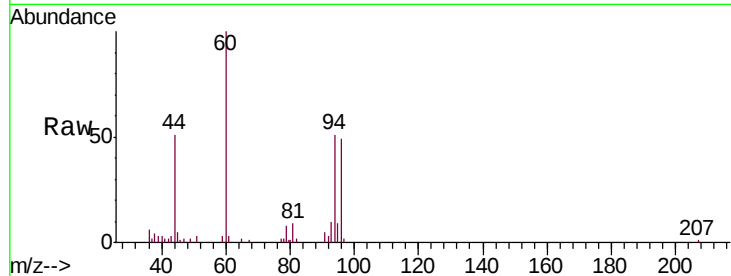

Abundance Ion 94.00 (93.70 to 94.70): VU0

Ion 96.00 (95.70 to 96.70): VU0

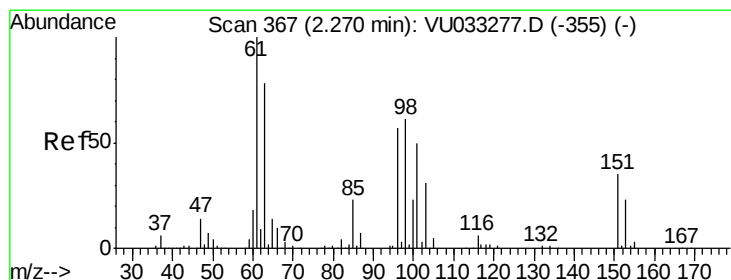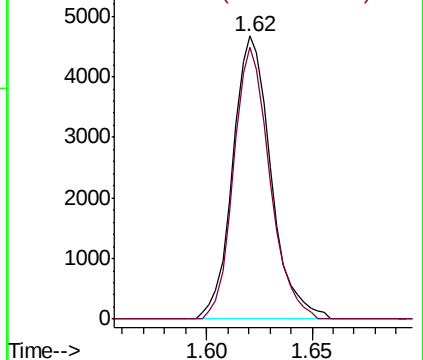

#12

1,1-Dichloroethene

Concen: 0.658 ug/L

RT: 2.27 min Scan# 367

Delta R.T. -0.00 min

Lab File: VU033279.D

Acq: 17 Jul 2019 09:56


Tgt Ion: 96 Resp: 6948

Ion Ratio Lower Upper

96 100

61 246.3 129.3 240.1#



63 839.0 108.9 202.3#




Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.05 (60.75 to 61.75): VU0

Ion 63.00 (62.70 to 63.70): VU0

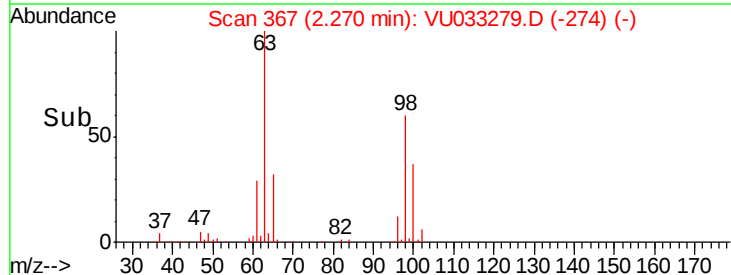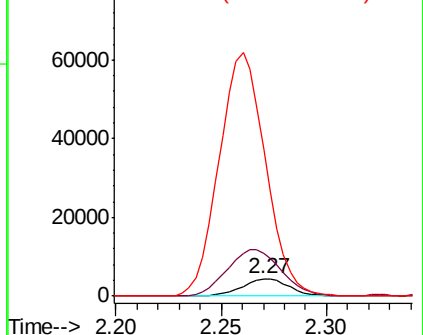



#13

Acetone

Concen: 18.111 ug/L

RT: 2.32 min Scan# 383

Delta R.T. -0.01 min

Lab File: VU033279.D

Acq: 17 Jul 2019 09:56

Instrument :

MSVOA_U

ClientSampleId :


A52T8DL

Tgt Ion: 43 Resp: 38677

Ion Ratio Lower Upper

43 100

58 23.3 0.0 66.6

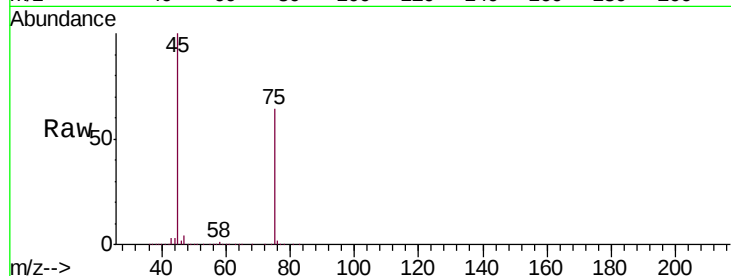

Abundance Ion 43.05 (42.75 to 43.75): VU033277.D (-371) (-)

Ion 58.05 (57.75 to 58.75): VU033277.D (-371) (-)

2.32

20000



15000

10000

5000

0

Time--> 2.20 2.30 2.40



#14

Carbon disulfide

Concen: 2.231 ug/L

RT: 2.46 min Scan# 427

Delta R.T. -0.00 min

Lab File: VU033279.D


Acq: 17 Jul 2019 09:56

Tgt Ion: 76 Resp: 76257

Ion Ratio Lower Upper

76 100

78 9.0 7.1 10.7



Abundance Ion 76.05 (75.75 to 76.75): VU033277.D (-414) (-)

Ion 78.00 (77.70 to 78.70): VU033277.D (-414) (-)

2.46

50000

40000


30000


20000

10000

0

Time--> 2.40 2.50 2.60









#15
Methyl Acetate
Concen: 9.842 ug/L
RT: 2.60 min Scan# 471
Delta R.T. -0.00 min
Lab File: VU033279.D
Acq: 17 Jul 2019 09:56




Instrument :
MSVOA_U
ClientSampleId :
A52T8DL


Tgt Ion: 43 Resp: 52496
Ion Ratio Lower Upper
43 100
74 23.2 17.8 26.8

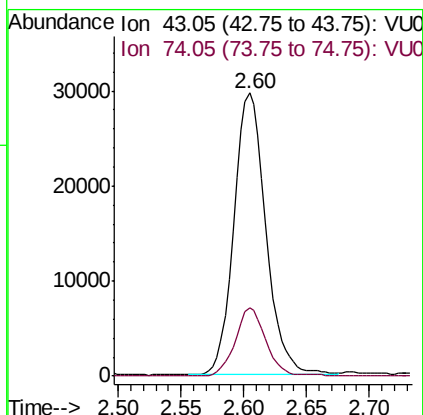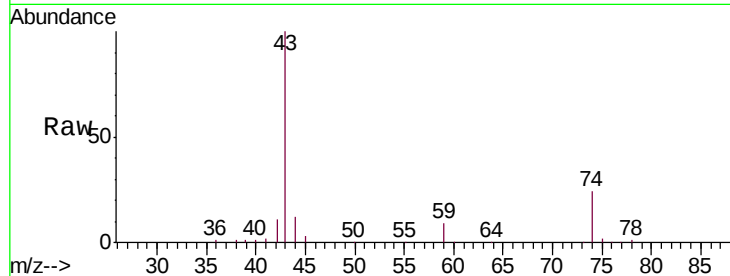

#16
Methylene chloride
Concen: 1.405 ug/L
RT: 2.68 min Scan# 496
Delta R.T. -0.00 min
Lab File: VU033279.D
Acq: 17 Jul 2019 09:56

Tgt Ion: 84 Resp: 18089
Ion Ratio Lower Upper
84 100
86 65.0 42.5 78.9
49 132.9 86.9 161.3

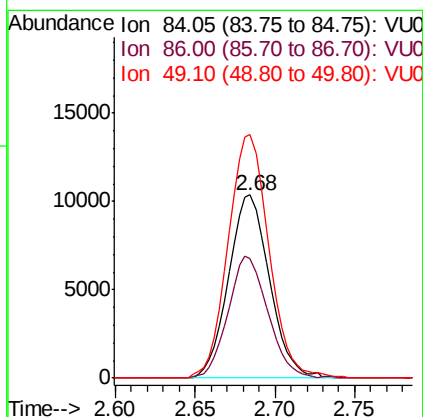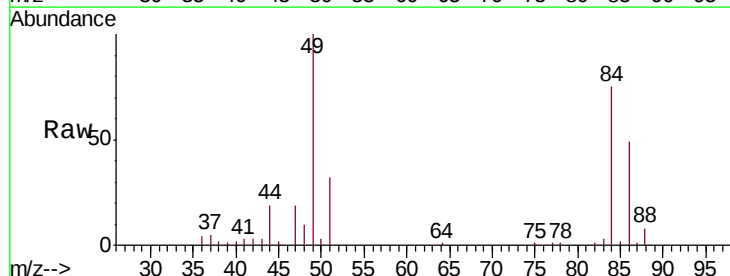



#17

Methyl tert-butyl Ether

Concen: 2.956 ug/L

RT: 2.99 min Scan# 590

Delta R.T. 0.00 min

Lab File: VU033279.D

Acq: 17 Jul 2019 09:56

Instrument :

MSVOA_U

ClientSampleId :

A52T8DL


Tgt Ion: 73 Resp: 81759

Ion Ratio Lower Upper

73 100

43 21.3 16.3 24.5




57 22.8 18.6 28.0



Abundance Ion 73.10 (72.80 to 73.80): VU033279.D (-496) (-)

Ion 43.05 (42.75 to 43.75): VU033279.D (-496) (-)

Ion 57.10 (56.80 to 57.80): VU033279.D (-496) (-)

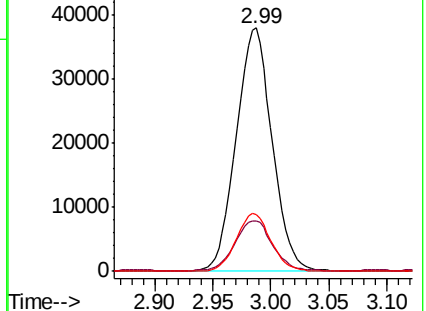

#21

2-Butanone

Concen: 9.947 ug/L

RT: 4.26 min Scan# 986

Delta R.T. -0.00 min

Lab File: VU033279.D


Acq: 17 Jul 2019 09:56

Tgt Ion: 43 Resp: 24414

Ion Ratio Lower Upper



43 100


72 24.9 13.5 40.4



Abundance Ion 43.05 (42.75 to 43.75): VU033279.D (-893) (-)

Ion 72.10 (71.80 to 72.80): VU033279.D (-893) (-)

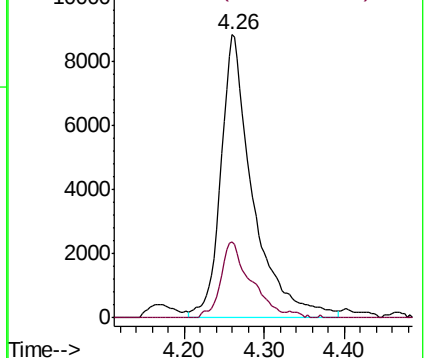

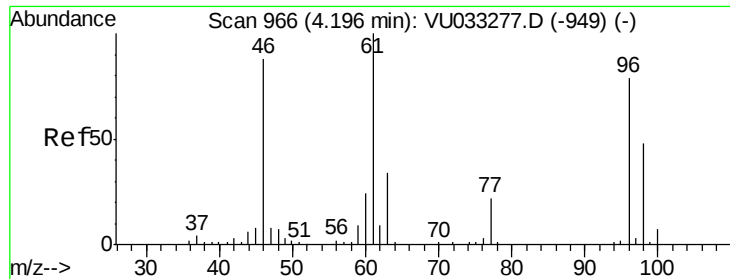

#22

cis-1,2-Dichloroethene

Concen: 1.709 ug/L

RT: 4.20 min Scan# 967

Delta R.T. 0.00 min

Lab File: VU033279.D

Acq: 17 Jul 2019 09:56

Instrument :

MSVOA_U

ClientSampleId :

A52T8DL


Tgt Ion: 96 Resp: 16847

Ion Ratio Lower Upper

96 100

61 130.4 89.2 165.6




68 0.0 0.0 0.0



Abundance Ion 96.00 (95.70 to 96.70): VU033279.D (-873) (-)

Ion 61.05 (60.75 to 61.75): VU033279.D (-873) (-)

Ion 68.15 (67.85 to 68.85): VU033279.D (-873) (-)

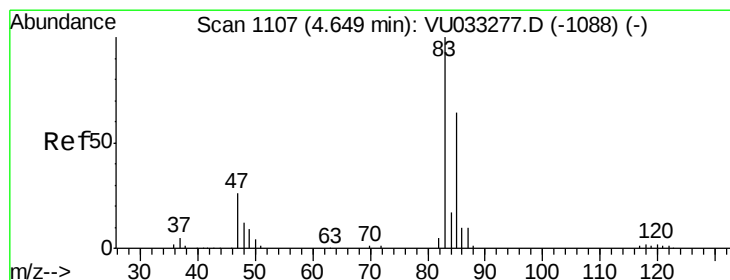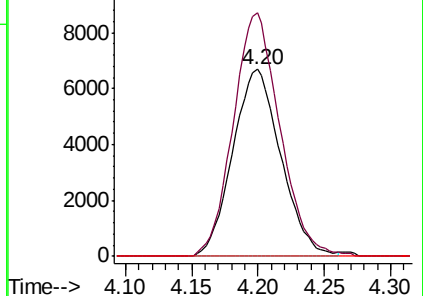

#25

Chloroform

Concen: 0.196 ug/L

RT: 4.65 min Scan# 1106

Delta R.T. -0.00 min

Lab File: VU033279.D


Acq: 17 Jul 2019 09:56

Tgt Ion: 83 Resp: 3806

Ion Ratio Lower Upper



83 100


85 61.7 45.4 84.4



Abundance Ion 83.05 (82.75 to 83.75): VU033279.D (-1014) (-)

Ion 85.00 (84.70 to 85.70): VU033279.D (-1014) (-)

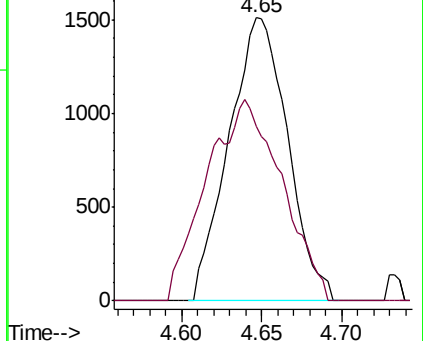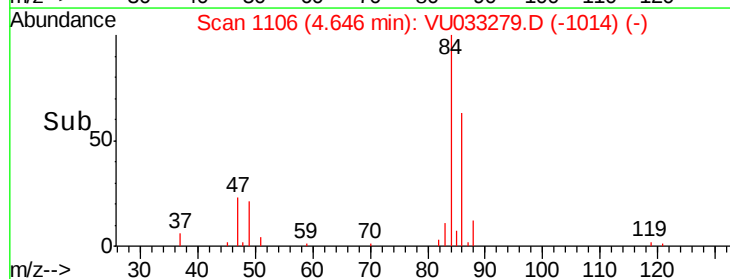

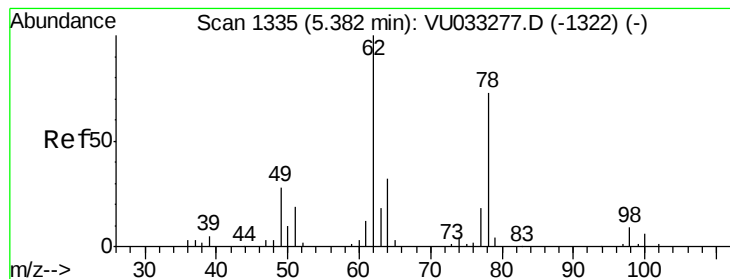

#27

1,2-Dichloroethane

Concen: 1.464 ug/L

RT: 5.39 min Scan# 1336

Delta R.T. 0.00 min

Lab File: VU033279.D

Acq: 17 Jul 2019 09:56

Instrument :

MSVOA_U

ClientSampleId :


A52T8DL

Tgt Ion: 62 Resp: 16910

Ion Ratio Lower Upper




62 100

98 8.9 6.6 10.0



Abundance Ion 62.00 (61.70 to 62.70): VU033277.D (-1322) (-)

Ion 98.05 (97.75 to 98.75): VU033279.D (-1242) (-)

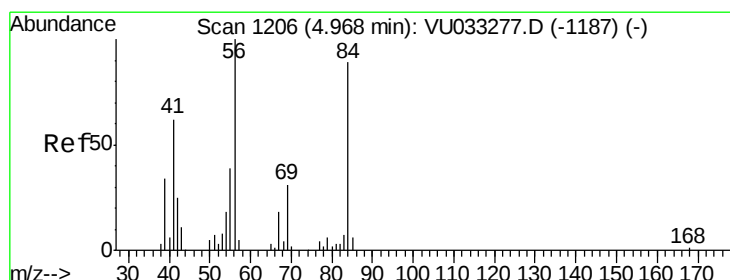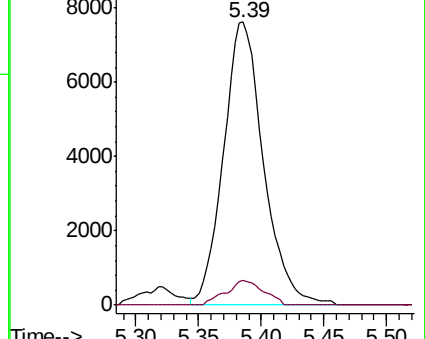

#30

Cyclohexane

Concen: 2.530 ug/L

RT: 4.97 min Scan# 1206

Delta R.T. -0.00 min

Lab File: VU033279.D

Acq: 17 Jul 2019 09:56


Tgt Ion: 56 Resp: 35562

Ion Ratio Lower Upper

56 100

69 31.5 23.9 35.9



84 87.3 69.5 104.3




Abundance Ion 56.10 (55.80 to 56.80): VU033277.D (-1187) (-)

Ion 69.15 (68.85 to 69.85): VU033279.D (-1113) (-)

Ion 84.15 (83.85 to 84.85): VU033279.D (-1113) (-)

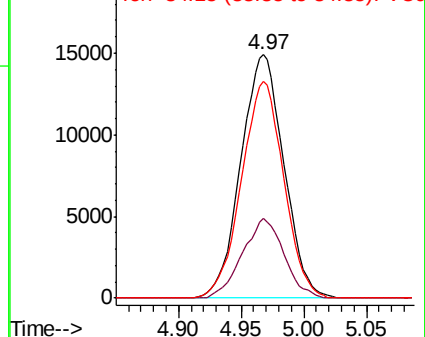

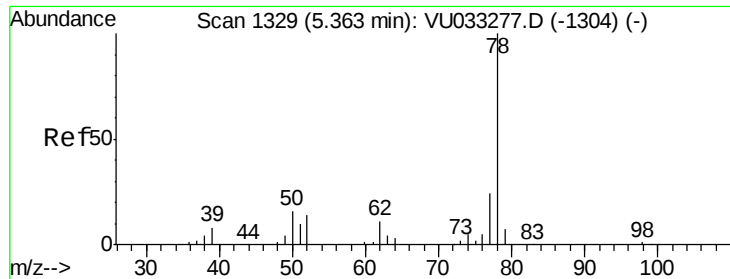

#33

Benzene

Concen: 1.344 ug/L

RT: 5.37 min Scan# 1330

Delta R.T. 0.00 min

Lab File: VU033279.D

Acq: 17 Jul 2019 09:56


Instrument :

MSVOA_U




ClientSampleId :

A52T8DL

Tgt Ion: 78 Resp: 51554



Abundance Ion 78.10 (77.80 to 78.80): VU0

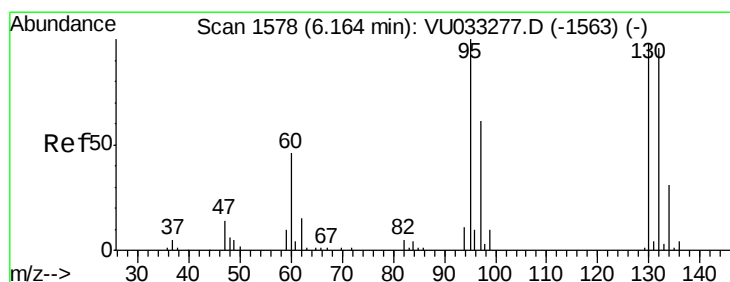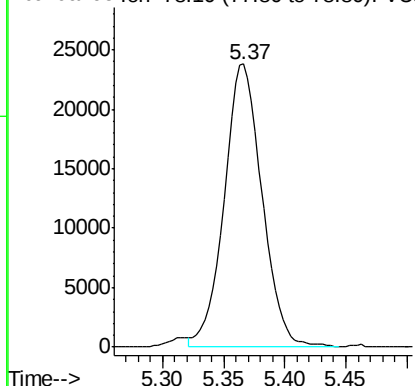

#34

Trichloroethene

Concen: 0.942 ug/L

RT: 6.16 min Scan# 1578

Delta R.T. -0.00 min

Lab File: VU033279.D

Acq: 17 Jul 2019 09:56

Tgt Ion: 95 Resp: 9563




Ion	Ratio	Lower	Upper
95	100		
97	56.7	44.5	82.7
132	92.6	66.6	123.8
130	96.4	68.9	127.9


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

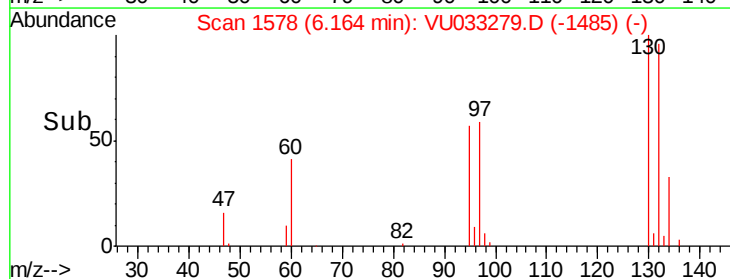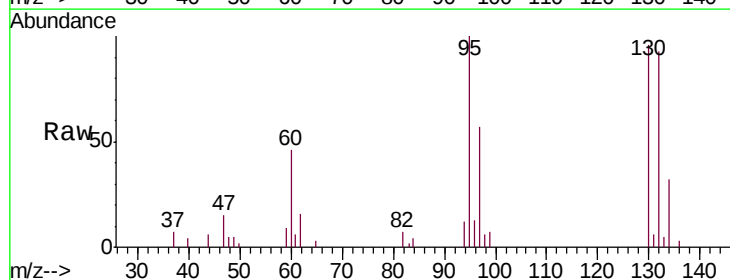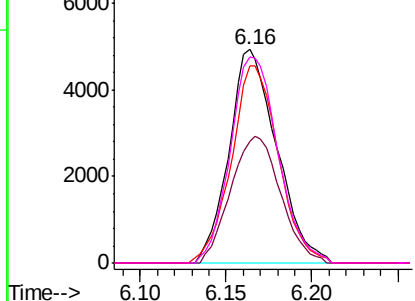


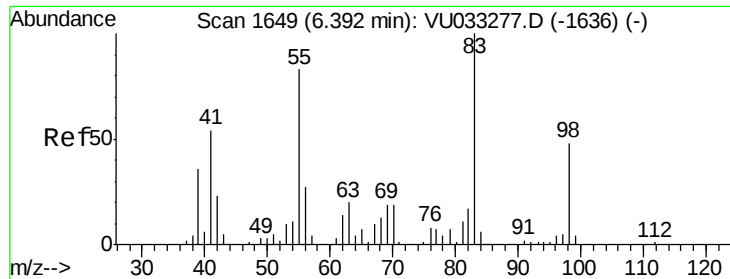




#35
Methylcyclohexane
Concen: 4.779 ug/L
RT: 6.39 min Scan# 1649
Delta R.T. -0.00 min
Lab File: VU033279.D
Acq: 17 Jul 2019 09:56

Instrument :
MSVOA_U
ClientSampleId :
A52T8DL

Tgt Ion: 83 Resp: 73118
Ion Ratio Lower Upper
83 100
55 82.3 62.6 94.0
98 46.2 36.2 54.2

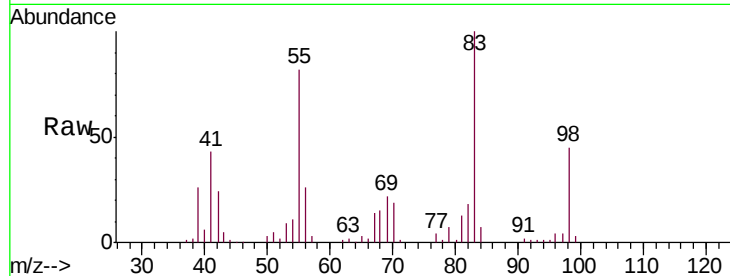


Abundance Ion 83.15 (82.85 to 83.85): VU0
Ion 55.10 (54.80 to 55.80): VU0
Ion 98.15 (97.85 to 98.85): VU0


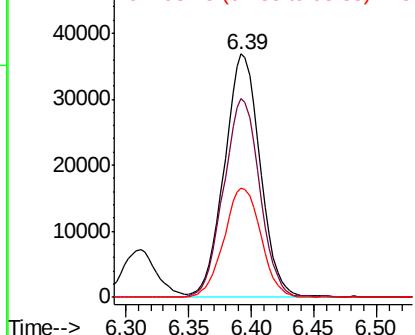



#40
4-Methyl-2-pentanone
Concen: 6.461 ug/L
RT: 7.45 min Scan# 1978
Delta R.T. 0.00 min
Lab File: VU033279.D
Acq: 17 Jul 2019 09:56

Tgt Ion: 43 Resp: 38419
Ion Ratio Lower Upper
43 100
58 39.2 32.4 48.6
100 14.3 11.9 17.9



Abundance Ion 43.05 (42.75 to 43.75): VU0
Ion 58.05 (57.75 to 58.75): VU0
Ion 100.15 (99.85 to 100.85): VU0

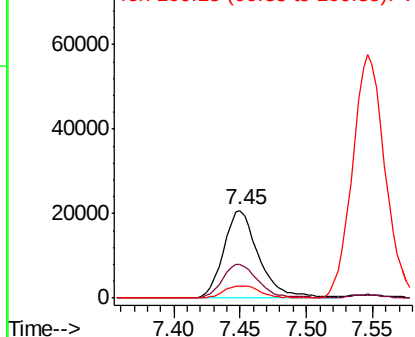



#42

Toluene

Concen: 4.050 ug/L

RT: 7.62 min Scan# 2030

Delta R.T. -0.00 min

Lab File: VU033279.D

Acq: 17 Jul 2019 09:56

Instrument :

MSVOA_U

ClientSampleId :


A52T8DL

Tgt Ion: 91 Resp: 166831

Ion Ratio Lower Upper

91 100

92 57.0 40.0 74.2

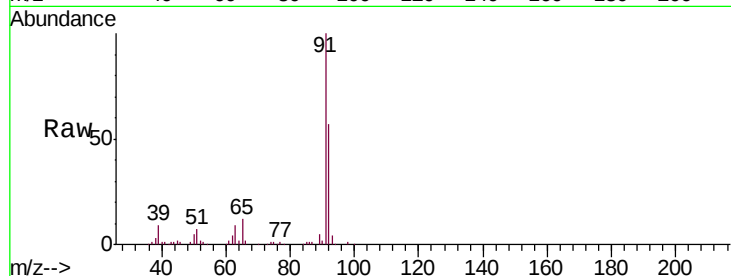

Abundance Ion 91.15 (90.85 to 91.85): VU033277.D (-2016) (-)

Ion 92.15 (91.85 to 92.85): VU033279.D (-1937) (-)

7.62

100000

80000

60000



40000

20000

0

7.55 7.60 7.65 7.70

Time-->



#44

trans-1,3-Dichloropropene

Concen: 0.120 ug/L

RT: 7.83 min Scan# 2097

Delta R.T. -0.03 min

Lab File: VU033279.D


Acq: 17 Jul 2019 09:56

Tgt Ion: 75 Resp: 1442

Ion Ratio Lower Upper

75 100

77 39.0 21.6 40.0



Abundance Ion 75.05 (74.75 to 75.75): VU033277.D (-2088) (-)

Ion 77.05 (76.75 to 77.75): VU033279.D (-2133) (-)

7.83

600


400


200

0

7.80 7.85

Time-->




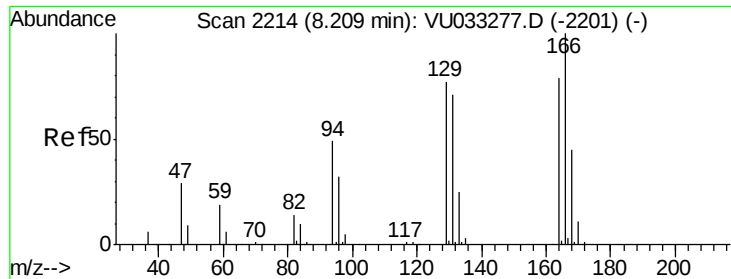




#47
Tetrachloroethene
Concen: 1.147 ug/L
RT: 8.21 min Scan# 2214
Delta R.T. -0.00 min
Lab File: VU033279.D
Acq: 17 Jul 2019 09:56

Instrument :
MSVOA_U
ClientSampleId :
A52T8DL

Tgt Ion:164 Resp: 9333
Ion Ratio Lower Upper
164 100
129 97.2 68.5 127.1
131 95.5 67.3 124.9
166 124.7 93.1 172.9

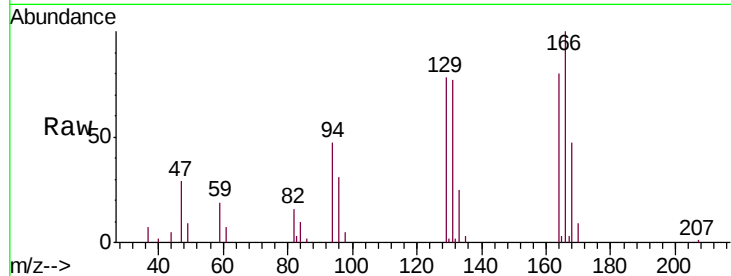


Abundance Ion 163.90 (163.60 to 164.60): V
Ion 128.95 (128.65 to 129.65): V
Ion 130.95 (130.65 to 131.65): V
Ion 165.90 (165.60 to 166.60): V


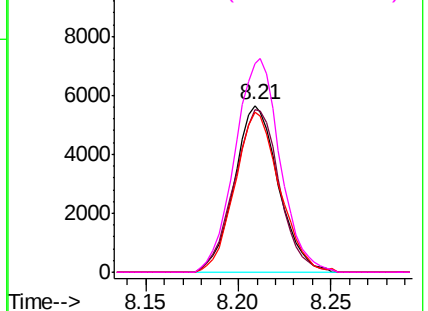



#48
2-Hexanone
Concen: 7.054 ug/L
RT: 8.35 min Scan# 2259
Delta R.T. 0.00 min
Lab File: VU033279.D
Acq: 17 Jul 2019 09:56

Tgt Ion: 43 Resp: 30677
Ion Ratio Lower Upper
43 100
58 52.5 44.1 66.1
57 19.2 15.8 23.8
100 10.2 9.4 14.2



Abundance Ion 43.05 (42.75 to 43.75): VU0
Ion 58.05 (57.75 to 58.75): VU0
Ion 57.20 (56.90 to 57.90): VU0
Ion 100.15 (99.85 to 100.85): VU0

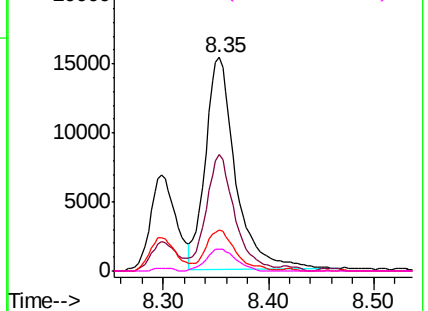



#49

Dibromochloromethane

Concen: 1.042 ug/L

RT: 8.21 min Scan# 2214

Delta R.T. -0.25 min

Lab File: VU033279.D

Acq: 17 Jul 2019 09:56

Instrument :

MSVOA_U

ClientSampleId :


A52T8DL

Tgt Ion:129 Resp: 9314

Ion Ratio Lower Upper




129 100

127 0.0 51.9 96.5#

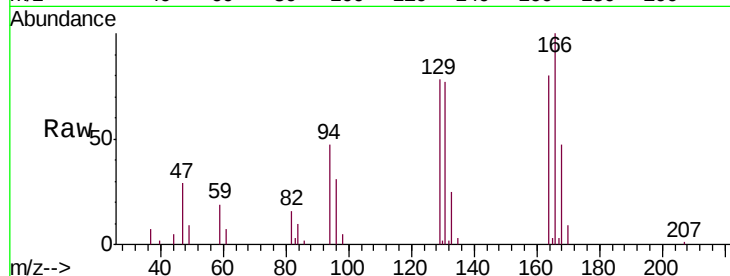

Abundance Ion 128.95 (128.65 to 129.65): V

Ion 126.90 (126.60 to 127.60): V

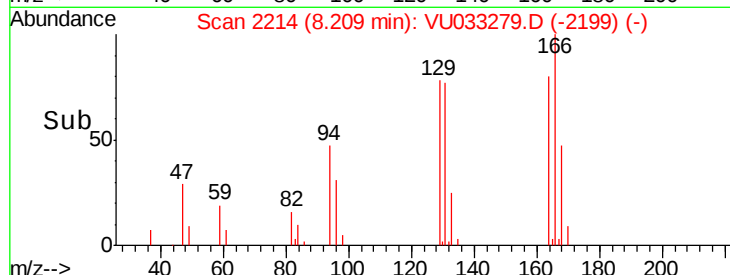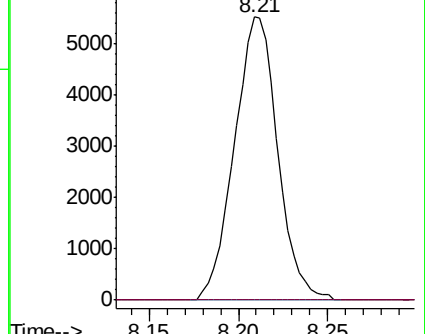

#50

1,2-Dibromoethane

Concen: 0.492 ug/L

RT: 8.58 min Scan# 2328

Delta R.T. 0.01 min

Lab File: VU033279.D

Acq: 17 Jul 2019 09:56


Tgt Ion:107 Resp: 3502

Ion Ratio Lower Upper

107 100

109 94.7 64.8 120.4



188 0.0 3.0 4.6#




Abundance Ion 106.95 (106.65 to 107.65): V

Ion 109.00 (108.70 to 109.70): V

Ion 187.90 (187.60 to 188.60): V




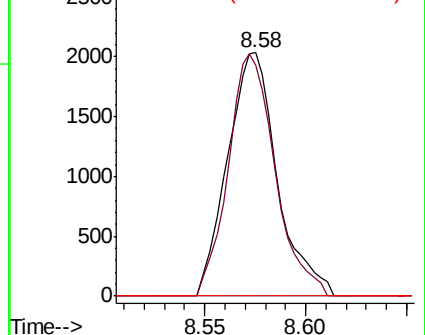


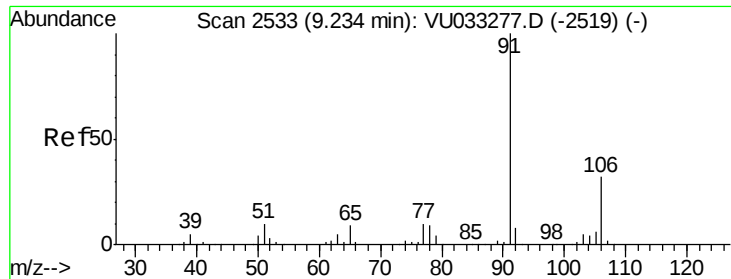

#52
Ethylbenzene
Concen: 2.209 ug/L
RT: 9.23 min Scan# 2533
Delta R.T. -0.00 min
Lab File: VU033279.D
Acq: 17 Jul 2019 09:56




Instrument :
MSVOA_U
ClientSampleId :
A52T8DL


Tgt Ion: 91 Resp: 97121
Ion Ratio Lower Upper
91 100
106 30.9 21.6 40.2

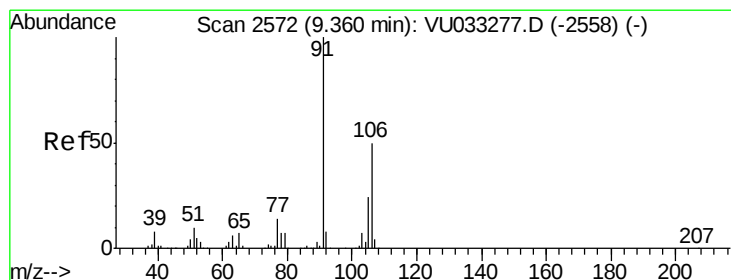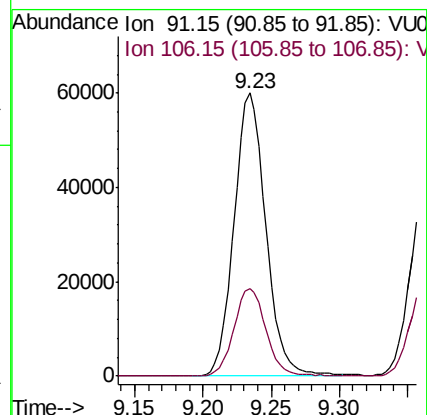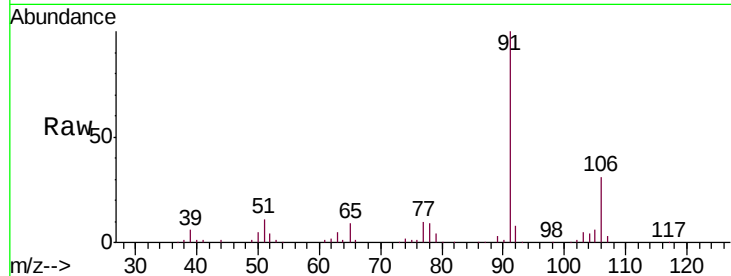

#53
m,p-Xylene
Concen: 1.960 ug/L
RT: 9.36 min Scan# 2573
Delta R.T. 0.00 min
Lab File: VU033279.D
Acq: 17 Jul 2019 09:56

Tgt Ion: 106 Resp: 32562
Ion Ratio Lower Upper
106 100
91 197.0 147.6 274.0

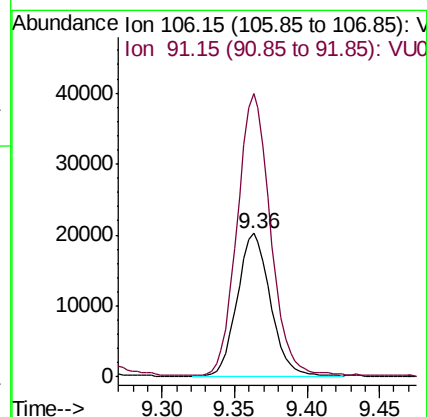



#59

1,2,3-Trichloropropane

Concen: 1.167 ug/L

RT: 11.47 min Scan# 3228

Delta R.T. 0.99 min

Lab File: VU033279.D

Acq: 17 Jul 2019 09:56

Instrument :

MSVOA_U

ClientSampleId :





A52T8DL

Tgt Ion: 75 Resp: 7895

Ion Ratio Lower Upper

75 100

77 38.2 26.5 39.7

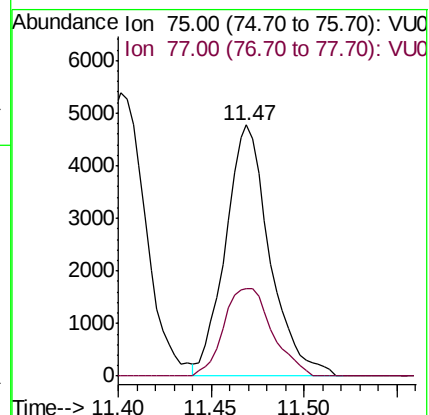

#62

1,3-Dichlorobenzene

Concen: 1.533 ug/L

RT: 11.40 min Scan# 3208

Delta R.T. 0.00 min

Lab File: VU033279.D

Acq: 17 Jul 2019 09:56




Tgt Ion: 146 Resp: 27377


Ion Ratio Lower Upper

146 100

111 42.9 28.6 53.2

148 63.7 45.0 83.6

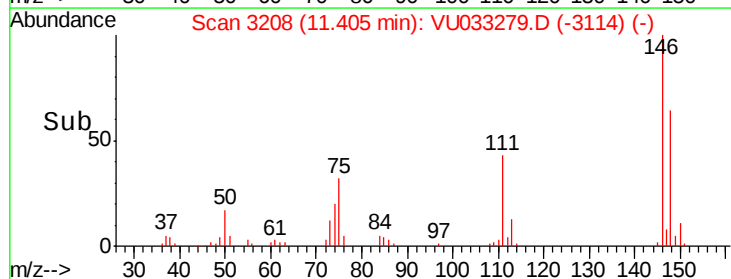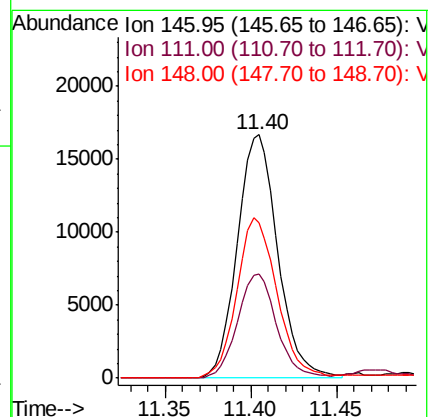


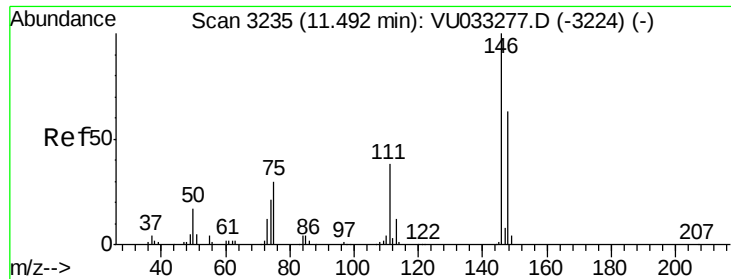

#63
 1,4-Dichlorobenzene
 Concen: 1.456 ug/L
 RT: 11.40 min Scan# 3208
 Delta R.T. -0.09 min
 Lab File: VU033279.D
 Acq: 17 Jul 2019 09:56

Instrument :
 MSVOA_U
 ClientSampleId :
 A52T8DL

Tgt Ion	Ratio	Lower	Upper
146	100		
111	42.9	27.9	51.7
148	63.7	44.1	81.9



Abundance Ion 145.95 (145.65 to 146.65): V
 Ion 111.00 (110.70 to 111.70): V
 Ion 148.00 (147.70 to 148.70): V

