


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU071719\
 Data File : VU033276.D
 Acq On : 17 Jul 2019 08:25
 Operator : JC/SP
 Sample : BFB26
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB26

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR071619WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jul 18 08:01:21 2019

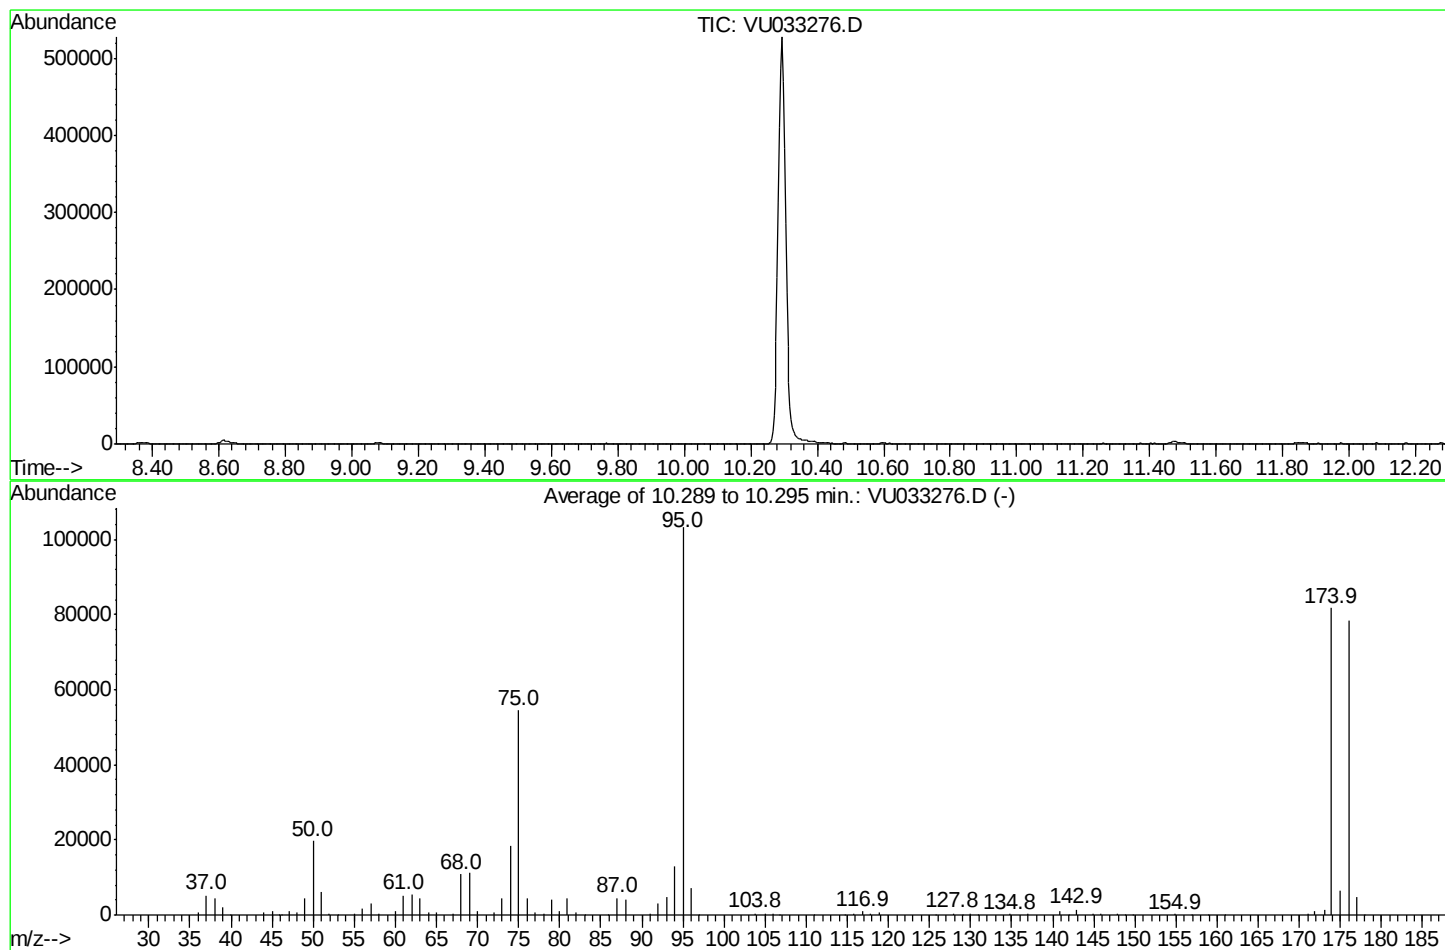

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	19746	PASS
75	95	30	80	52.8	54554	PASS
95	95	100	100	100.0	103293	PASS
96	95	5	9	6.9	7076	PASS
173	174	0.00	2	1.7	1412	PASS
174	95	50	120	79.2	81818	PASS
175	174	5	9	7.8	6415	PASS
176	174	95	101	95.8	78381	PASS
177	176	5	9	6.3	4914	PASS

Scan 2848 (10.247 min): VU033276.D
BFB26

m/z	Abundance
40.00	162.0
43.90	306.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.00	763.0
37.00	4890.0
38.00	4264.0
39.00	1781.0
39.90	335.0
44.00	1050.0
45.00	859.0
46.20	129.0
47.10	1148.0
47.90	644.0
49.00	4071.0
50.00	19256.0
51.00	5681.0
51.90	279.0
52.90	112.0
55.00	309.0
56.00	1598.0
57.00	2932.0
58.00	139.0
60.00	1014.0
61.00	5042.0
62.10	5103.0
63.00	4348.0
64.00	598.0
65.00	695.0
67.00	367.0
68.00	10188.0
69.00	10743.0
69.90	779.0
72.00	721.0
73.00	4389.0
74.00	17640.0
75.00	52736.0
76.00	4429.0
77.00	536.0
78.00	441.0
78.90	4018.0
80.00	1029.0
80.90	4440.0
81.90	824.0
85.80	137.0
87.00	4015.0
88.00	3930.0
90.90	358.0
92.00	3013.0
93.00	4432.0
94.00	12484.0
95.00	98984.0
96.00	7090.0
97.00	169.0
103.80	486.0
104.90	165.0
105.90	462.0
106.80	101.0
110.90	169.0
115.80	341.0
116.90	852.0
117.80	397.0
118.90	663.0
127.90	328.0
129.10	165.0
130.00	378.0
130.90	160.0
134.80	175.0
136.90	209.0
140.90	1084.0
142.90	1309.0
144.90	451.0
145.90	145.0
147.90	215.0
149.70	155.0
154.90	298.0
156.80	175.0
158.90	116.0
161.00	174.0
171.00	195.0
171.90	895.0
173.10	1372.0
174.00	76080.0
175.00	6103.0
176.00	72912.0
177.00	4684.0
177.90	159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.10	892.0
37.00	5351.0
38.00	4530.0
39.00	2012.0
39.90	315.0
44.00	1066.0
45.00	916.0
46.20	108.0
47.10	1224.0
47.90	687.0
49.00	4428.0
50.00	20296.0
51.00	6187.0
51.90	266.0
52.90	146.0
55.00	316.0
56.00	1729.0
57.00	3061.0
58.00	208.0
60.00	1060.0
61.00	5365.0
62.10	5528.0
63.00	4564.0
64.00	647.0
65.00	808.0
67.00	363.0
68.00	11213.0
69.00	11711.0
69.90	938.0
72.00	720.0
73.00	4645.0
74.00	18880.0
75.00	56232.0
76.00	4657.0
77.00	651.0
78.00	506.0
78.90	4208.0
79.90	1108.0
80.90	4754.0
81.90	816.0
83.00	124.0
85.80	115.0
87.00	4730.0
88.00	4178.0
91.00	383.0
92.00	3327.0
93.00	4836.0
94.00	13302.0
95.00	106256.0
96.00	7240.0
97.00	159.0
103.90	499.0
105.00	190.0
105.90	486.0
106.80	105.0
111.00	140.0
114.70	103.0
115.80	411.0
116.90	949.0
117.90	422.0
118.90	719.0
127.80	379.0
129.10	192.0
130.00	390.0
130.90	188.0
134.80	199.0
136.90	217.0
140.90	1193.0
142.00	112.0
142.90	1438.0
144.90	437.0
145.90	200.0
147.90	239.0
149.80	174.0
154.90	300.0
156.90	171.0
158.90	108.0
161.00	154.0
171.00	241.0
171.90	977.0
173.10	1426.0
174.00	84488.0
175.00	6619.0
176.00	80552.0
177.00	5065.0
177.90	131.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.00	925.0
37.00	5333.0
38.00	4514.0
39.00	2024.0
39.90	269.0
44.00	996.0
45.00	958.0
45.90	103.0
47.00	1134.0
48.00	658.0
49.00	4367.0
50.00	19688.0
51.00	6191.0
51.90	233.0
53.00	148.0
55.00	272.0
56.00	1664.0
57.00	2949.0
58.10	212.0
60.00	1007.0
61.00	5281.0
62.00	5514.0
63.00	4370.0
64.00	626.0
65.00	853.0
67.00	318.0
68.00	11285.0
69.00	11505.0
70.00	959.0
72.10	618.0
73.00	4600.0
74.00	18896.0
75.00	54696.0
76.00	4530.0
77.00	659.0
78.00	507.0
79.00	4156.0
79.90	1086.0
80.90	4588.0
81.90	801.0
83.00	128.0
87.00	4694.0
88.00	4139.0
91.00	412.0
92.00	3275.0
93.00	4811.0
94.00	12777.0
95.00	104640.0
96.00	6899.0
97.00	152.0
103.90	480.0
105.00	216.0
105.90	481.0
106.80	111.0
111.00	115.0
114.70	109.0
115.80	419.0
116.90	954.0
117.90	431.0
118.90	724.0
125.80	102.0
127.80	381.0
129.00	153.0
130.00	319.0
130.90	192.0
134.80	181.0
137.00	214.0
140.90	1245.0
142.90	1505.0
144.90	382.0
145.90	214.0
147.90	246.0
148.80	100.0
149.80	175.0
154.90	280.0
156.90	163.0
171.00	264.0
171.90	1017.0
173.10	1438.0
173.90	84888.0
175.00	6525.0
176.00	81680.0
177.00	4994.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26