

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071720\
 Data File : VU039546.D
 Acq On : 17 Jul 2020 12:58
 Operator : SY/MD
 Sample : L3313-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Jul 18 00:19:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 17 23:38:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.27	114	80536	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	78270	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	35755	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	20657	4.43	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.60%
7) Chloroethane-d5	1.93	69	23253	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.40%
11) 1,1-Dichloroethene-d2	2.58	63	31353	3.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.20%
20) 2-Butanone-d5	4.65	46	100695	47.15	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.30%
24) Chloroform-d	5.09	84	46889	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
26) 1,2-Dichloroethane-d4	5.72	65	31851	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.20%
32) Benzene-d6	5.74	84	93776	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
36) 1,2-Dichloropropane-d6	6.71	67	32504	4.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.20%
41) Toluene-d8	7.91	98	81735	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.00%
43) trans-1,3-Dichloropropene-	8.19	79	12728	4.35	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.00%
46) 2-Hexanone-d5	8.64	63	71577	41.28	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.56%
57) 1,1,2,2-Tetrachloroethane-	10.76	84	28244	4.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.00%
64) 1,2-Dichlorobenzene-d4	12.19	152	32944	5.16	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.20%


Target Compounds					Ovalue
16) Methylene chloride	3.07	84	2540	0.422 ug/L	99
25) Chloroform	5.11	83	5064	0.483 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU071720\
Data File : VU039546.D
Acq On : 17 Jul 2020 12:58
Operator : SY/MD
Sample : L3313-16
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Jul 18 00:19:48 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 17 23:38:36 2020
Response via : Initial Calibration

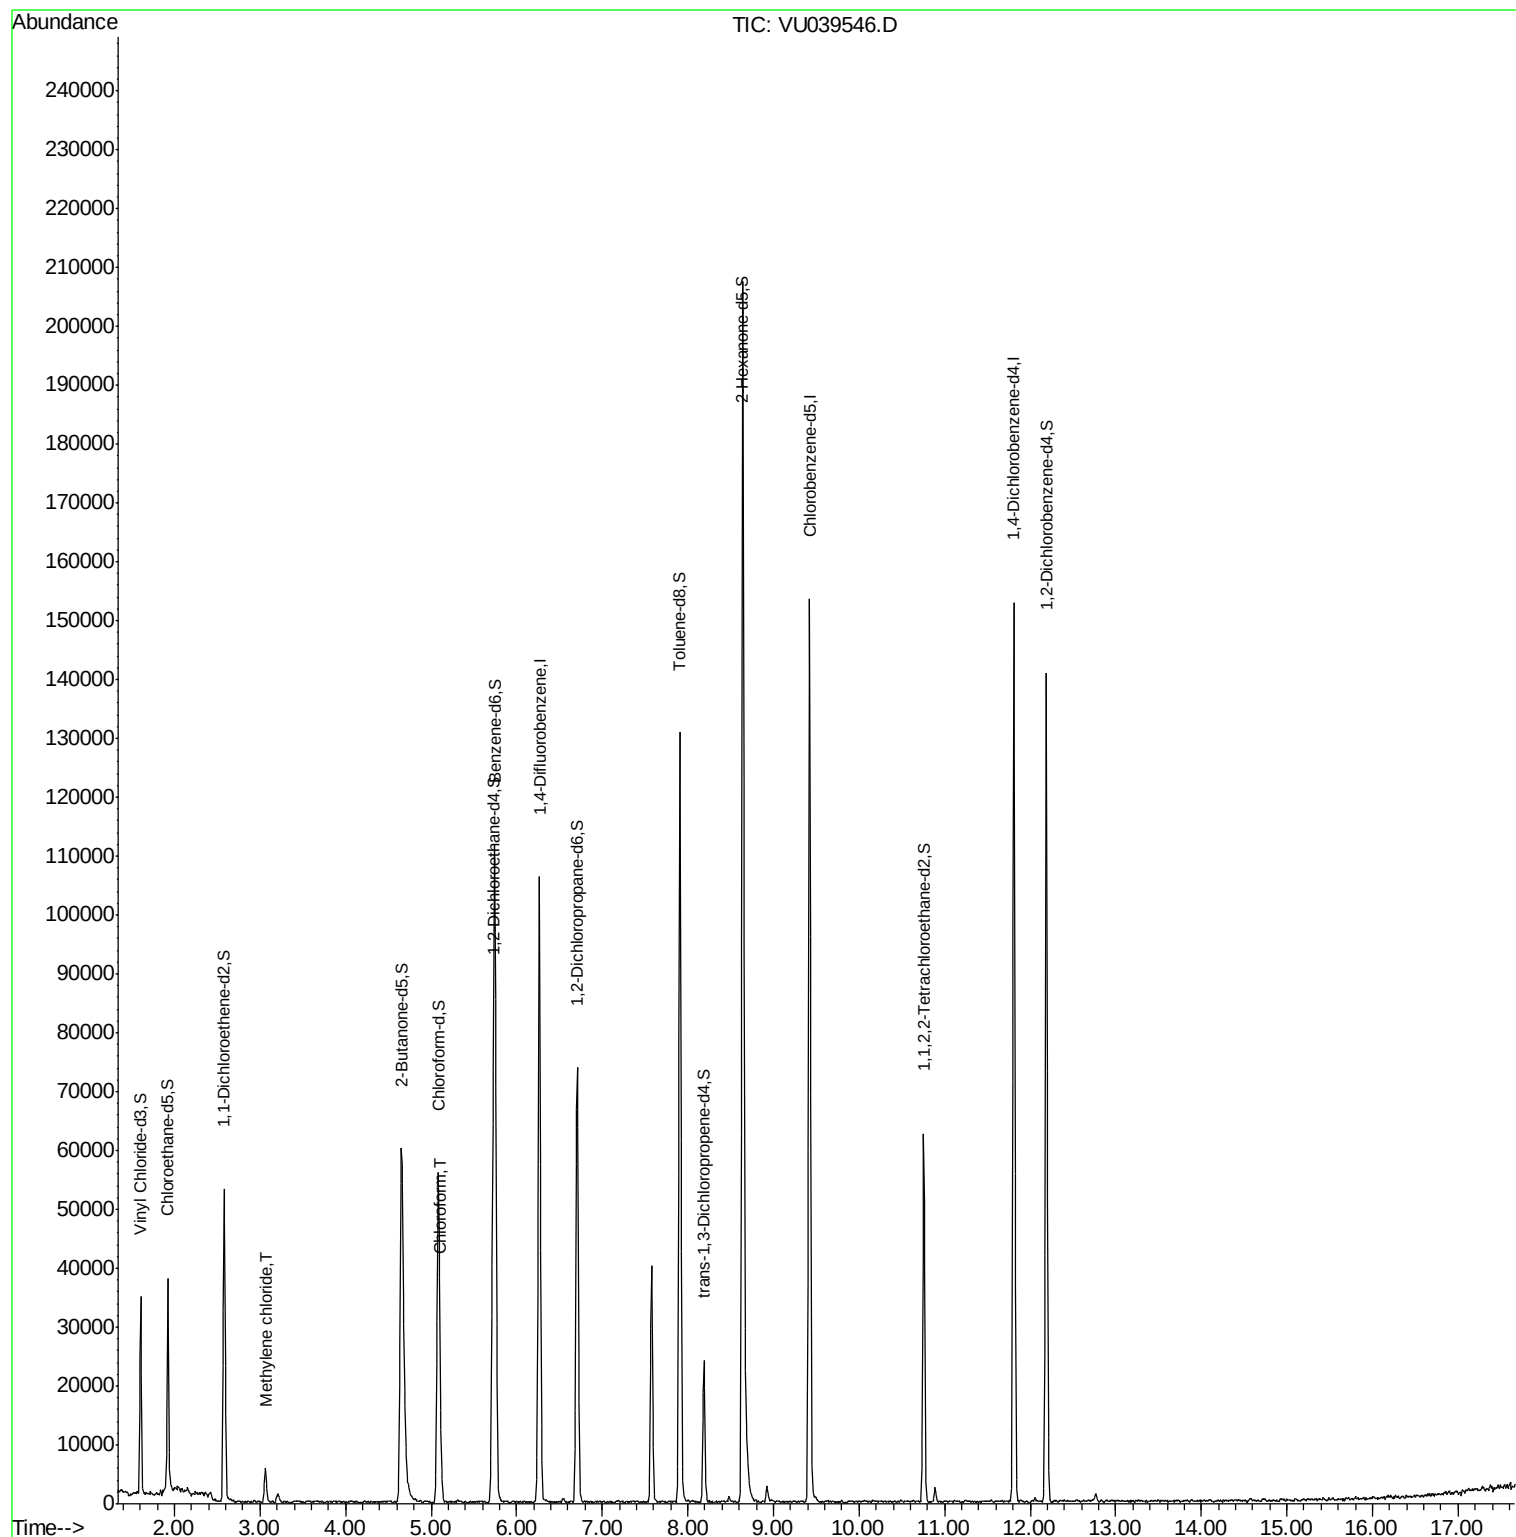

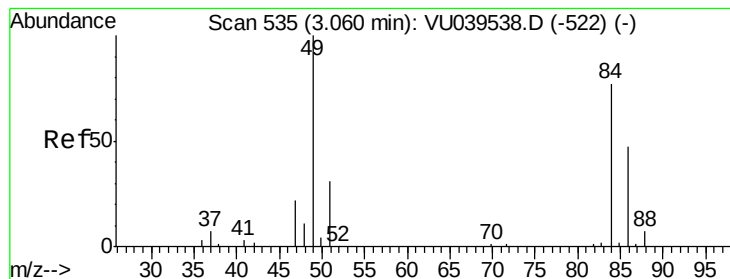

#16

Methylene chloride

Concen: 0.422 ug/L

RT: 3.07 min Scan# 537

Delta R.T. 0.01 min

Lab File: VU039546.D

Acq: 17 Jul 2020 12:58

Instrument :

MSVOA_U

ClientSampleId :

VHBLK01





Tot Ion: 84 Resp: 2540

Ion Ratio Lower Upper

84 100

86 61.2 43.5 80.9

49 130.5 91.1 169.1

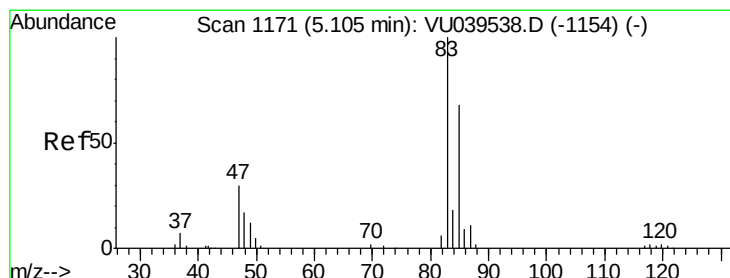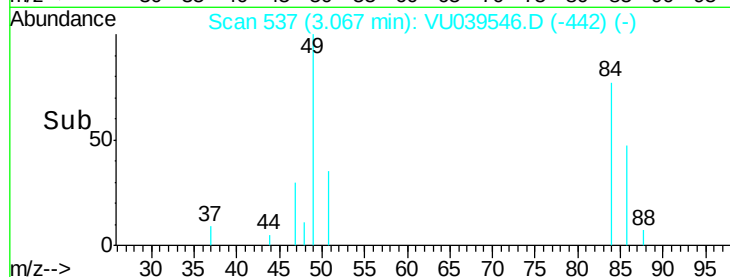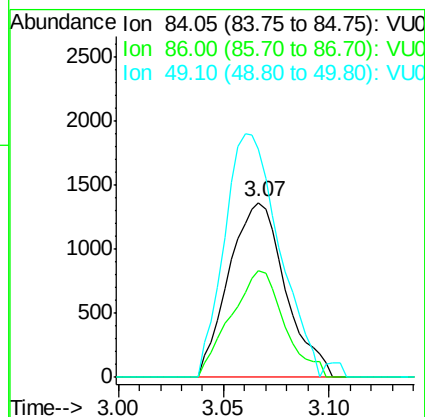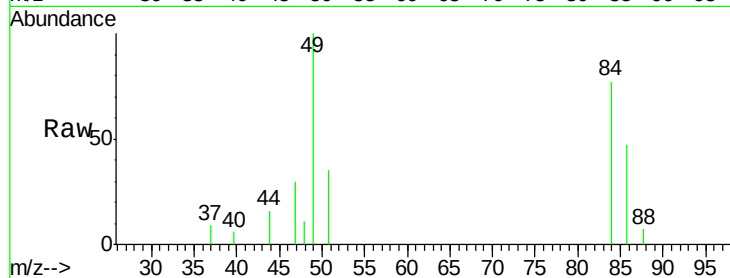

#25

Chloroform

Concen: 0.483 ug/L

RT: 5.11 min Scan# 1173

Delta R.T. 0.01 min

Lab File: VU039546.D

Acq: 17 Jul 2020 12:58

Tgt Ion: 83 Resp: 5064

Ion Ratio Lower Upper

83 100

85 72.3 44.9 83.5

