

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071720\
 Data File : VU039551.D
 Acq On : 17 Jul 2020 14:53
 Operator : SY/MD
 Sample : L3292-07DL 100X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFT83DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.607	75	83	96	rVB	29758	34876	8.79%	1.150%
2	1.925	173	182	198	rBV	30959	41059	10.35%	1.354%
3	2.581	375	386	403	rBV	53093	89204	22.48%	2.941%
4	3.064	526	536	552	rVB4	7425	12981	3.27%	0.428%
5	4.662	1015	1033	1073	rBV3	53204	187518	47.25%	6.182%
6	5.086	1150	1165	1189	rBV3	52870	126874	31.97%	4.182%
7	5.742	1347	1369	1387	rBV4	108896	293103	73.85%	9.662%
8	6.263	1517	1531	1551	rBV	117471	225119	56.72%	7.421%
9	6.556	1608	1622	1635	rBV2	23421	42773	10.78%	1.410%
10	6.707	1656	1669	1685	rBV2	71843	141755	35.72%	4.673%
11	7.575	1927	1939	1956	rBV	38408	67686	17.06%	2.231%
12	7.906	2027	2042	2056	rBV	128860	222827	56.15%	7.346%
13	8.189	2119	2130	2145	rBV3	23980	40267	10.15%	1.327%
14	8.559	2233	2245	2258	rBV2	117777	198857	50.11%	6.555%
15	8.642	2258	2271	2300	rBV	208888	396866	100.00%	13.083%
16	8.925	2351	2359	2370	rVB3	2858	4943	1.25%	0.163%
17	9.420	2500	2513	2532	rBV	173282	289811	73.02%	9.554%
18	10.758	2913	2929	2941	rBV	65497	102275	25.77%	3.372%
19	10.887	2963	2969	2986	rVB3	2771	4602	1.16%	0.152%
20	11.809	3243	3256	3270	rBV	169194	279220	70.36%	9.205%
21	12.189	3362	3374	3388	rVB2	142596	230866	58.17%	7.611%


Sum of corrected areas: 3033482

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU071720\
Data File : VU039551.D
Acq On : 17 Jul 2020 14:53
Operator : SY/MD
Sample : L3292-07DL 100X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT83DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

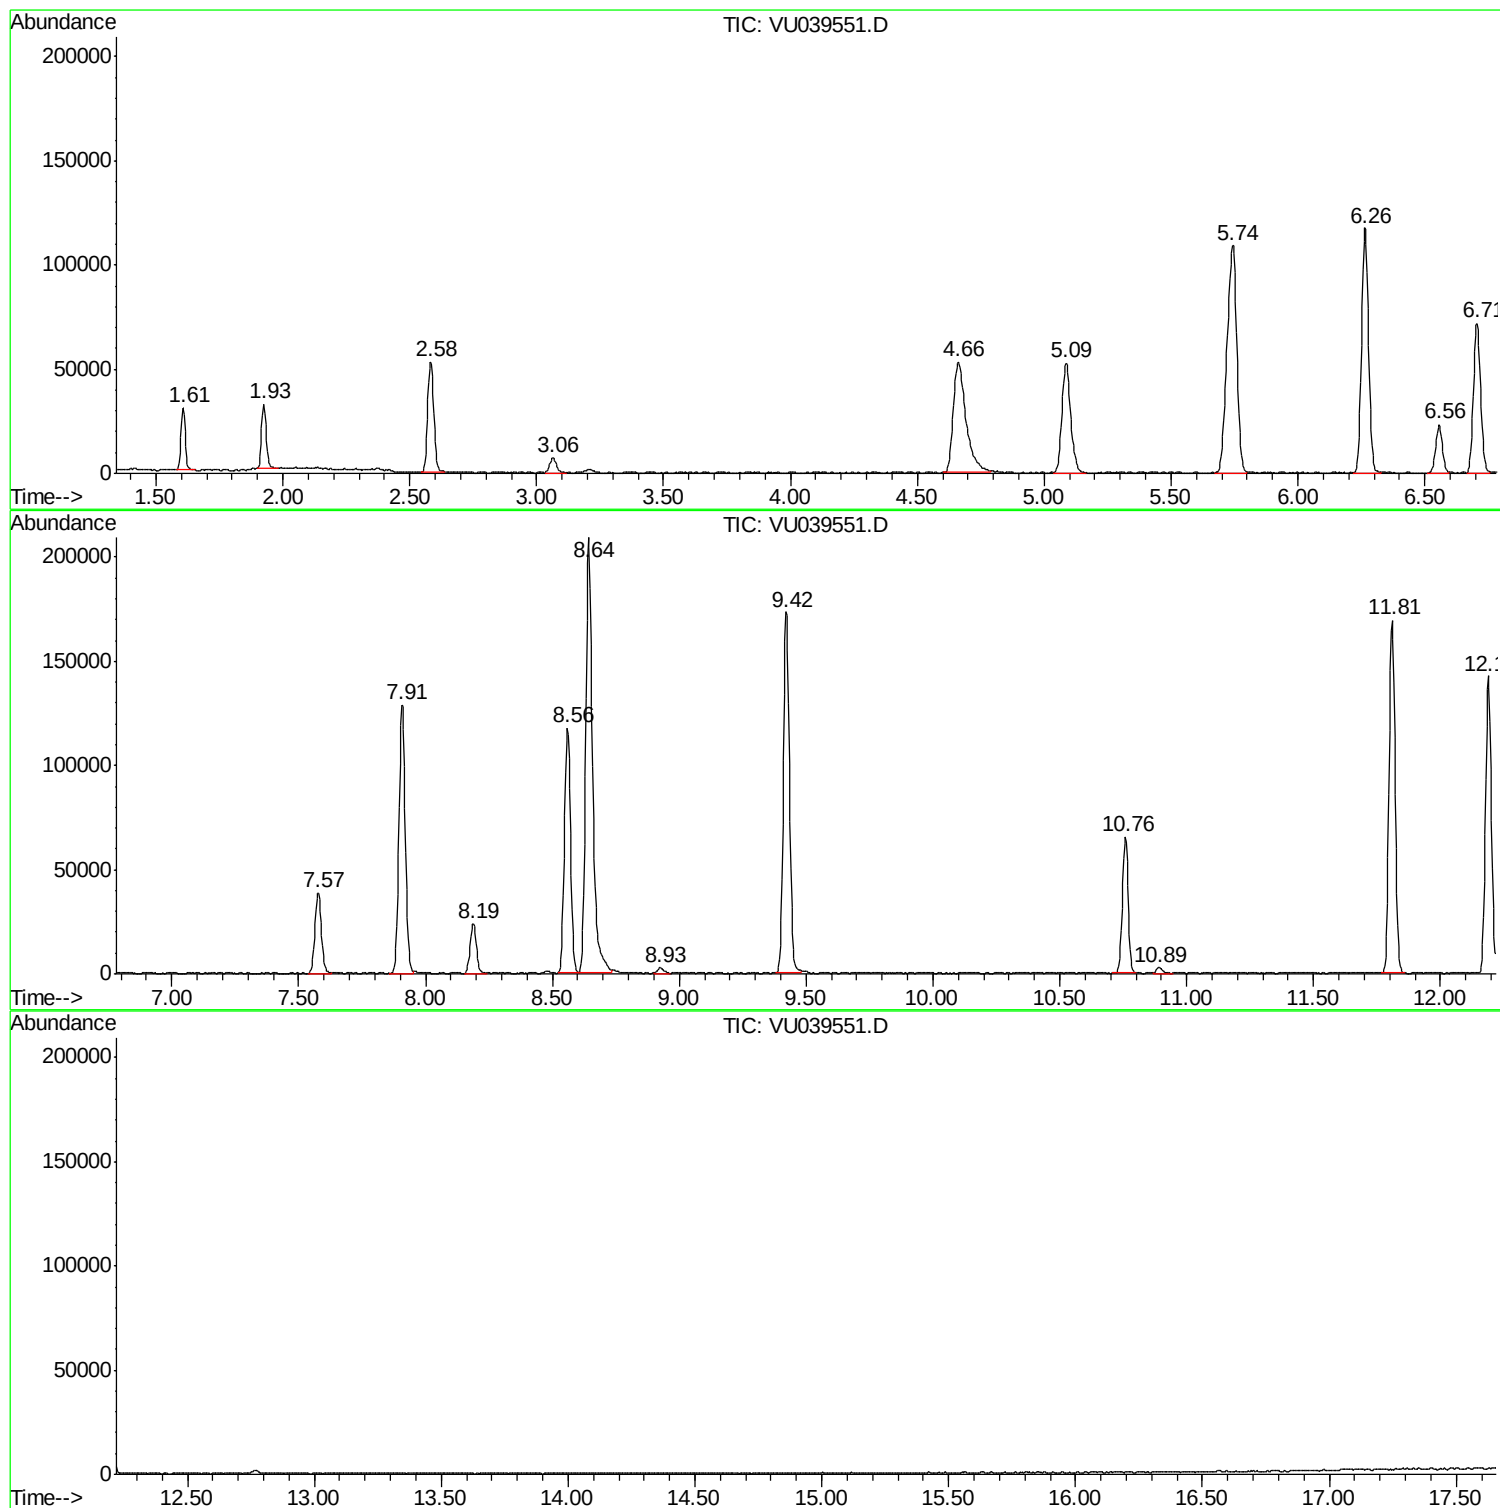

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071720\
Data File : VU039551.D
Acq On : 17 Jul 2020 14:53
Operator : SY/MD
Sample : L3292-07DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT83DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071720\
Data File : VU039551.D
Acq On : 17 Jul 2020 14:53
Operator : SY/MD
Sample : L3292-07DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT83DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc