

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071720\  
 Data File : VU039560.D  
 Acq On : 17 Jul 2020 19:07  
 Operator : SY/MD  
 Sample : L3292-16  
 Misc : 25.0mL/MSVOA U/WATER  
 ALS Vial : 26 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 BFT91

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR070720WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.594       | 374           | 390         | 405          | rBV5     | 247506         | 456865        | 4.20%           | 2.549%        |
| 2         | 4.687       | 1013          | 1041        | 1061         | rBV2     | 170049         | 515114        | 4.74%           | 2.874%        |
| 3         | 5.083       | 1150          | 1164        | 1187         | rBV2     | 59528          | 143952        | 1.32%           | 0.803%        |
| 4         | 5.742       | 1349          | 1369        | 1384         | rBV2     | 114192         | 311232        | 2.86%           | 1.737%        |
| 5         | 6.263       | 1517          | 1531        | 1551         | rBV      | 124928         | 237673        | 2.18%           | 1.326%        |
| 6         | 6.556       | 1605          | 1622        | 1651         | rBV      | 1939327        | 3665275       | 33.69%          | 20.452%       |
| 7         | 6.707       | 1656          | 1669        | 1685         | rVB      | 74459          | 146933        | 1.35%           | 0.820%        |
| 8         | 7.906       | 2029          | 2042        | 2057         | rBV      | 138253         | 238846        | 2.20%           | 1.333%        |
| 9         | 8.562       | 2230          | 2246        | 2261         | rBV      | 6710420        | 10878643      | 100.00%         | 60.702%       |
| 10        | 8.642       | 2261          | 2271        | 2302         | rVB      | 219605         | 456591        | 4.20%           | 2.548%        |
| 11        | 9.420       | 2500          | 2513        | 2532         | rBV      | 195006         | 322941        | 2.97%           | 1.802%        |
| 12        | 11.809      | 3244          | 3256        | 3273         | rBV      | 187304         | 304097        | 2.80%           | 1.697%        |
| 13        | 12.189      | 3361          | 3374        | 3391         | rVB      | 153138         | 243344        | 2.24%           | 1.358%        |


Sum of corrected areas: 17921506

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU071720\  
Data File : VU039560.D  
Acq On : 17 Jul 2020 19:07  
Operator : SY/MD  
Sample : L3292-16  
Misc : 25.0mL/MSVOA U/WATER  
ALS Vial : 26 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BFT91

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR070720WMA.M  
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

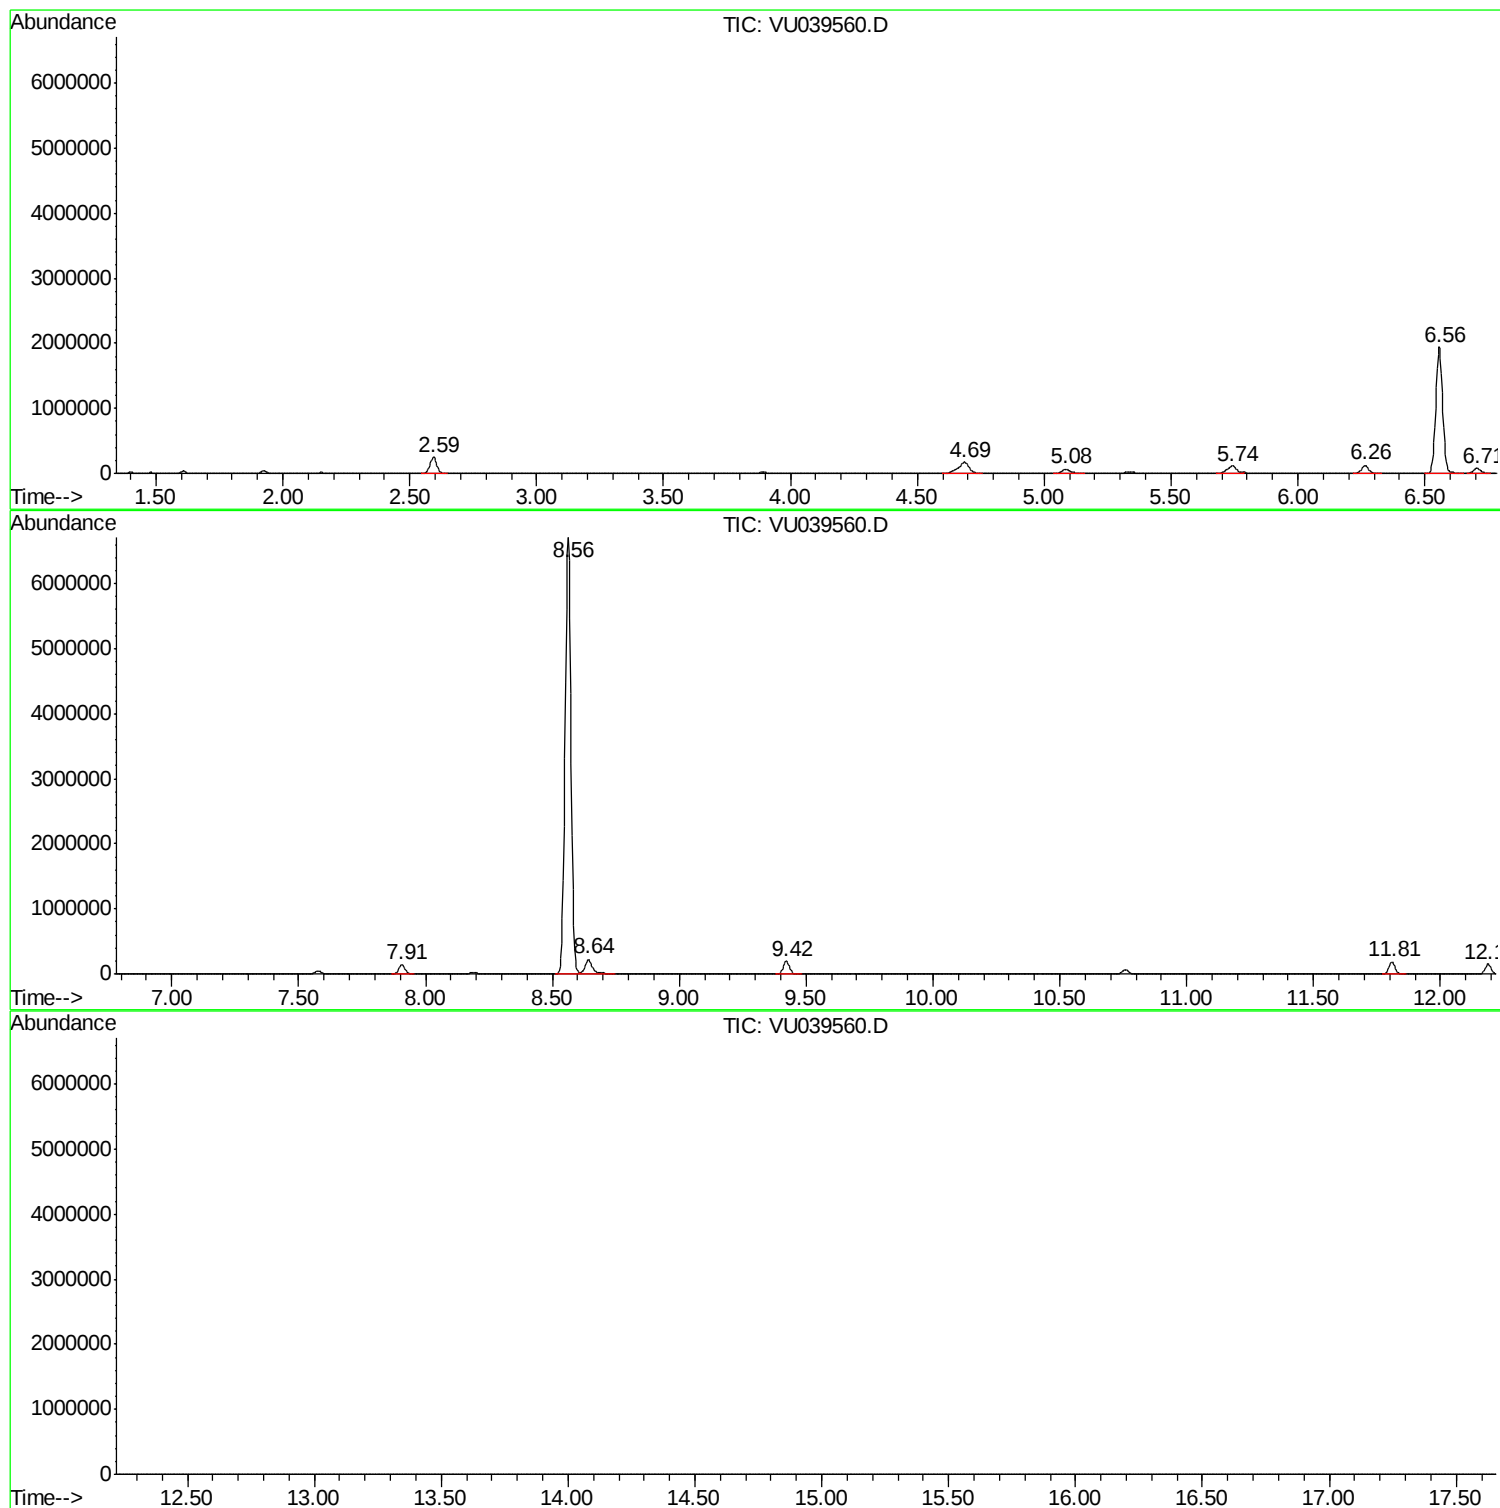

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_U\DATA\VU071720\  
Data File : VU039560.D  
Acq On : 17 Jul 2020 19:07  
Operator : SY/MD  
Sample : L3292-16  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 26 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BFT91

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR070720WMA.M  
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_U\DATA\VU071720\  
Data File : VU039560.D  
Acq On : 17 Jul 2020 19:07  
Operator : SY/MD  
Sample : L3292-16  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 26 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BFT91

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR070720WMA.M  
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |