


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU071720\
 Data File : VU039537.D
 Acq On : 17 Jul 2020 08:34
 Operator : SY/MD
 Sample : BFB04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB04

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Jul 20 11:02:35 2020

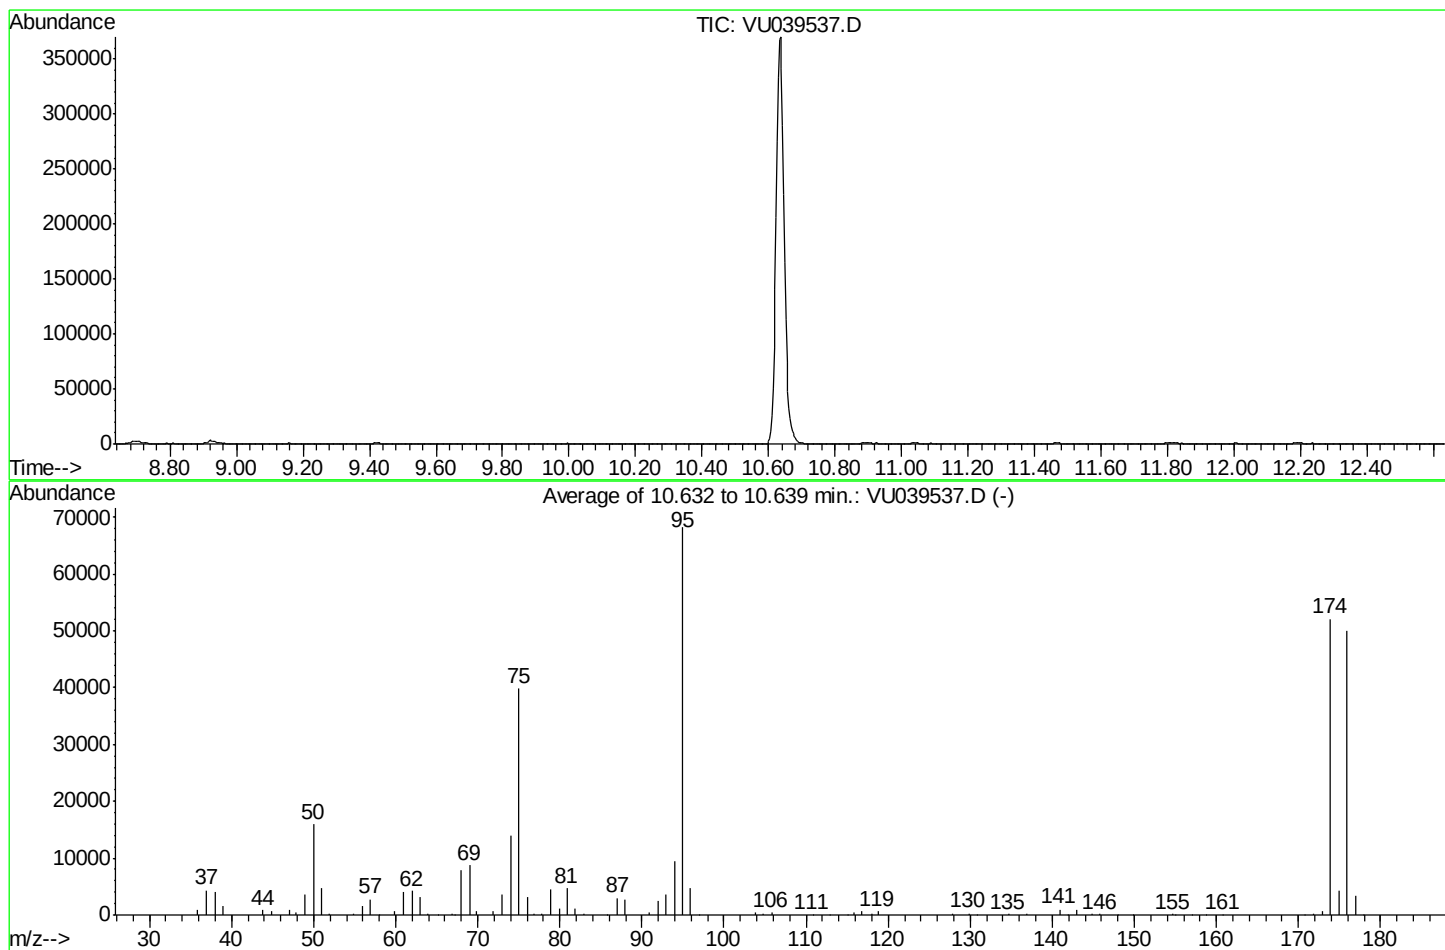

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	15884	PASS
75	95	30	80	58.4	39802	PASS
95	95	100	100	100.0	68189	PASS
96	95	5	9	7.1	4814	PASS
173	174	0.00	2	1.3	687	PASS
174	95	50	120	76.3	52024	PASS
175	174	5	9	8.3	4299	PASS
176	174	95	101	96.0	49957	PASS
177	176	5	9	6.6	3311	PASS

m/z	Abundance
35.90	915.0
36.90	4448.0
37.90	4273.0
39.00	1642.0
39.90	120.0
43.90	1310.0
45.00	748.0
47.00	855.0
47.90	566.0
49.00	3555.0
50.00	16320.0
51.00	5060.0
51.90	283.0
54.90	260.0
55.90	1755.0
57.00	2816.0
57.90	187.0
59.80	723.0
61.00	4347.0
62.00	4405.0
63.00	3408.0
63.90	265.0
65.10	103.0
66.90	198.0
67.90	8189.0
69.00	9171.0
69.90	686.0
71.90	632.0
73.00	3643.0
74.00	14039.0
75.00	40880.0
76.00	3339.0
76.90	339.0
77.90	284.0
78.80	4845.0
79.90	1274.0
80.90	4854.0
81.90	1205.0
82.90	109.0
85.80	184.0
87.00	3121.0
87.90	2943.0
90.90	493.0
91.90	2323.0
92.90	3658.0
94.00	9731.0
95.00	69904.0
95.90	4959.0
97.00	114.0
103.90	369.0
104.70	139.0
105.80	374.0
110.80	128.0
112.80	117.0
115.80	389.0
116.80	556.0
117.90	245.0
118.80	629.0
127.90	296.0
129.90	289.0
134.60	179.0
137.00	184.0
140.90	948.0
142.90	937.0
144.80	126.0
145.90	127.0
147.90	128.0
154.70	160.0
155.00	164.0
157.00	122.0
170.70	121.0
171.90	344.0
172.90	686.0
173.90	52528.0
174.90	4277.0
175.90	49888.0
176.90	3381.0
177.90	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
35.90	833.0
37.00	4406.0
38.00	4170.0
39.00	1599.0
39.80	148.0
43.90	1203.0
44.90	786.0
47.00	870.0
47.90	582.0
49.00	3749.0
50.00	16384.0
51.00	4842.0
51.90	290.0
54.90	244.0
55.90	1605.0
57.00	2803.0
57.90	121.0
59.80	777.0
61.00	4219.0
62.00	4342.0
63.00	3325.0
63.90	286.0
65.10	115.0
66.90	165.0
67.90	8094.0
69.00	8968.0
69.90	712.0
71.90	639.0
73.00	3765.0
74.00	14368.0
75.00	41016.0
76.00	3301.0
76.80	329.0
77.80	239.0
78.80	4726.0
79.90	1193.0
80.90	4781.0
81.90	1131.0
82.90	145.0
85.80	142.0
87.00	3190.0
87.90	2831.0
90.90	474.0
91.90	2534.0
92.90	3776.0
94.00	9577.0
95.00	70112.0
95.90	4980.0
97.00	114.0
103.90	393.0
104.70	152.0
105.90	419.0
110.90	112.0
115.00	110.0
115.80	379.0
116.80	629.0
117.90	285.0
118.80	650.0
127.90	289.0
129.90	320.0
130.70	114.0
134.70	155.0
136.90	201.0
140.90	994.0
142.00	123.0
142.90	946.0
144.90	139.0
145.80	120.0
147.90	114.0
149.80	108.0
154.70	168.0
157.00	119.0
158.80	101.0
171.80	311.0
172.90	728.0
173.90	53288.0
174.90	4433.0
175.90	51600.0
176.90	3417.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
35.90	690.0
37.00	4189.0
38.00	3758.0
39.00	1444.0
39.80	174.0
43.90	955.0
44.90	718.0
47.00	764.0
47.80	528.0
48.90	3476.0
50.00	14950.0
51.00	4361.0
51.90	283.0
54.90	235.0
55.90	1395.0
56.90	2632.0
59.90	782.0
61.00	3754.0
62.00	3872.0
63.00	3011.0
64.00	283.0
65.10	137.0
66.80	119.0
67.10	119.0
67.90	7316.0
69.00	7941.0
69.90	701.0
71.90	508.0
72.90	3540.0
74.00	13658.0
75.00	37512.0
76.00	3053.0
76.80	336.0
77.70	218.0
78.90	4129.0
79.90	1101.0
80.90	4249.0
81.80	1025.0
82.90	164.0
87.00	2759.0
87.90	2447.0
90.80	371.0
91.90	2520.0
93.00	3535.0
94.00	8804.0
95.00	64552.0
96.00	4504.0
97.00	117.0
103.90	427.0
104.70	154.0
105.90	424.0
110.90	104.0
115.00	104.0
115.90	343.0
116.80	634.0
118.00	264.0
118.80	560.0
127.90	250.0
129.80	306.0
130.80	110.0
134.80	132.0
136.90	182.0
140.90	927.0
141.90	146.0
142.90	885.0
144.90	121.0
145.80	116.0
149.80	117.0
154.70	174.0
160.80	101.0
171.80	281.0
173.00	648.0
173.90	50256.0
174.90	4188.0
175.90	48384.0
176.90	3135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

Scan 2877 (10.591 min): VU039537.D
BFB04

m/z	Abundance
39.80	184.0
43.80	346.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04