

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071723\
 Data File : VU054795.D
 Acq On : 17 Jul 2023 16:06
 Operator : MD/SY
 Sample : VU0717WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK098

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

Signal : TIC: VU054795.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	89	95	109	rBV	98272	138004	18.58%	2.135%
2	2.551	383	392	408	rVB	144885	233481	31.43%	3.613%
3	3.007	531	534	536	rBV3	910	648	0.09%	0.010%
4	3.245	605	608	611	rBV2	947	605	0.08%	0.009%
5	3.441	664	669	672	rBV2	536	431	0.06%	0.007%
6	3.535	695	698	701	rBV4	806	565	0.08%	0.009%
7	3.763	765	769	771	rBV3	722	521	0.07%	0.008%
8	3.869	792	802	804	rBV4	826	1002	0.13%	0.016%
9	3.885	804	807	809	rBV4	658	479	0.06%	0.007%
10	4.059	858	861	863	rBV3	951	568	0.08%	0.009%
11	4.268	923	926	928	rBV2	503	358	0.05%	0.006%
12	4.409	967	970	974	rBV2	527	399	0.05%	0.006%
13	4.560	1015	1017	1021	rBV2	683	426	0.06%	0.007%
14	4.618	1024	1035	1061	rBV2	74734	186723	25.14%	2.889%
15	4.888	1118	1119	1123	rBV3	573	413	0.06%	0.006%
16	5.056	1155	1171	1191	rBV	135554	303200	40.82%	4.691%
17	5.261	1232	1235	1236	rBV2	717	464	0.06%	0.007%
18	5.342	1258	1260	1262	rBV2	681	330	0.04%	0.005%
19	5.718	1356	1377	1395	rBV2	276078	742761	100.00%	11.492%
20	5.956	1448	1451	1453	rBV2	648	531	0.07%	0.008%
21	5.985	1458	1460	1462	rBV2	793	425	0.06%	0.007%
22	6.043	1474	1478	1481	rBV4	705	651	0.09%	0.010%
23	6.101	1493	1496	1499	rBV4	548	374	0.05%	0.006%
24	6.123	1499	1503	1508	rVV4	860	823	0.11%	0.013%
25	6.197	1523	1526	1528	rBV3	958	599	0.08%	0.009%
26	6.242	1528	1540	1560	rVV	270091	520941	70.14%	8.060%
27	6.438	1596	1601	1604	rBV5	836	824	0.11%	0.013%
28	6.528	1621	1629	1638	rBV9	2286	4308	0.58%	0.067%
29	6.686	1662	1678	1697	rBV2	177286	350129	47.14%	5.417%
30	6.895	1741	1743	1746	rBV3	465	325	0.04%	0.005%
31	6.943	1753	1758	1762	rBV3	661	835	0.11%	0.013%
32	6.965	1762	1765	1767	rVV2	757	433	0.06%	0.007%
33	7.335	1877	1880	1882	rVB3	604	333	0.04%	0.005%
34	7.432	1904	1910	1913	rBV3	721	555	0.07%	0.009%
35	7.445	1913	1914	1918	rBV3	636	392	0.05%	0.006%
36	7.560	1938	1950	1969	rBV	104249	184597	24.85%	2.856%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071723\
 Data File : VU054795.D
 Acq On : 17 Jul 2023 16:06
 Operator : MD/SY
 Sample : VU0717WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK098

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

37	7.792	2016	2022	2028	rBV4	1886	2565	0.35%	0.040%
38	7.895	2041	2054	2069	rBV	346921	607071	81.73%	9.393%
39	8.123	2122	2125	2127	rBV	854	469	0.06%	0.007%
40	8.178	2131	2142	2161	rBV	74038	129115	17.38%	1.998%
41	8.348	2191	2195	2199	rVB4	1120	966	0.13%	0.015%
42	8.425	2217	2219	2222	rBV2	543	412	0.06%	0.006%
43	8.631	2271	2283	2309	rBV	241406	449402	60.50%	6.953%
44	8.891	2361	2364	2366	rBV3	853	597	0.08%	0.009%
45	9.055	2411	2415	2416	rBV3	845	460	0.06%	0.007%
46	9.129	2435	2438	2440	rBV2	1107	731	0.10%	0.011%
47	9.239	2470	2472	2478	rVB5	753	644	0.09%	0.010%
48	9.309	2489	2494	2496	rBV	561	467	0.06%	0.007%
49	9.415	2512	2527	2548	rBV	407571	680973	91.68%	10.536%
50	9.573	2571	2576	2583	rVB4	2116	2507	0.34%	0.039%
51	9.637	2594	2596	2599	rVB2	946	423	0.06%	0.007%
52	9.689	2609	2612	2622	rVB8	2384	3727	0.50%	0.058%
53	9.769	2634	2637	2638	rBV2	695	383	0.05%	0.006%
54	9.930	2684	2687	2689	rBV2	901	538	0.07%	0.008%
55	9.969	2695	2699	2704	rBV4	631	646	0.09%	0.010%
56	10.084	2732	2735	2736	rBV2	882	480	0.06%	0.007%
57	10.161	2757	2759	2764	rVB2	807	407	0.05%	0.006%
58	10.187	2764	2767	2771	rBV3	489	414	0.06%	0.006%
59	10.210	2771	2774	2777	rBV3	519	392	0.05%	0.006%
60	10.255	2784	2788	2791	rBV3	349	329	0.04%	0.005%
61	10.351	2815	2818	2820	rBV2	452	372	0.05%	0.006%
62	10.412	2833	2837	2839	rBV4	733	536	0.07%	0.008%
63	10.428	2839	2842	2844	rBV3	578	421	0.06%	0.007%
64	10.557	2879	2882	2884	rBV4	947	573	0.08%	0.009%
65	10.579	2887	2889	2893	rVB3	712	454	0.06%	0.007%
66	10.605	2893	2897	2899	rBV3	515	368	0.05%	0.006%
67	10.753	2931	2943	2959	rBV	303121	495772	66.75%	7.671%
68	10.866	2975	2978	2980	rBV2	742	468	0.06%	0.007%
69	10.891	2984	2986	2988	rBV2	712	406	0.05%	0.006%
70	10.968	3007	3010	3015	rVB6	642	553	0.07%	0.009%
71	10.997	3015	3019	3021	rBV3	473	317	0.04%	0.005%
72	11.065	3035	3040	3041	rBV4	865	633	0.09%	0.010%
73	11.145	3063	3065	3070	rBV	444	347	0.05%	0.005%
74	11.184	3075	3077	3078	rBV2	730	316	0.04%	0.005%
75	11.216	3085	3087	3091	rBV3	601	420	0.06%	0.006%
76	11.309	3114	3116	3122	rBV5	498	401	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071723\
 Data File : VU054795.D
 Acq On : 17 Jul 2023 16:06
 Operator : MD/SY
 Sample : VU0717WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK098

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

77	11.367	3132	3134	3136	rBV2	714	346	0.05%	0.005%
78	11.412	3143	3148	3152	rVB4	1496	1055	0.14%	0.016%
79	11.682	3229	3232	3237	rBV4	730	460	0.06%	0.007%
80	11.808	3260	3271	3292	rBV	465643	741347	99.81%	11.470%
81	12.107	3360	3364	3368	rBV5	982	930	0.13%	0.014%
82	12.190	3378	3390	3408	rBV	390054	637880	85.88%	9.870%
83	12.309	3425	3427	3434	rVB4	665	527	0.07%	0.008%
84	12.557	3502	3504	3508	rBV3	819	579	0.08%	0.009%
85	12.637	3526	3529	3530	rBV3	559	316	0.04%	0.005%
86	12.782	3570	3574	3577	rBV3	1025	958	0.13%	0.015%
87	13.049	3652	3657	3660	rBV5	536	680	0.09%	0.011%
88	13.219	3704	3710	3711	rBV6	1923	1632	0.22%	0.025%
89	13.303	3734	3736	3739	rBV2	971	708	0.10%	0.011%
90	13.470	3782	3788	3791	rBV4	919	776	0.10%	0.012%
91	13.486	3791	3793	3796	rBV3	642	336	0.05%	0.005%
92	13.541	3806	3810	3812	rBV3	729	535	0.07%	0.008%
93	13.830	3897	3900	3901	rBV2	1087	640	0.09%	0.010%
94	13.846	3901	3905	3912	rVB6	3371	4547	0.61%	0.070%
95	14.248	4028	4030	4032	rVB	811	327	0.04%	0.005%
96	14.303	4041	4047	4049	rBV5	1451	1357	0.18%	0.021%
97	14.621	4143	4146	4149	rBV4	640	502	0.07%	0.008%
98	14.640	4149	4152	4156	rVV5	1031	746	0.10%	0.012%
99	15.155	4310	4312	4313	rBV2	807	383	0.05%	0.006%
100	15.801	4511	4513	4515	rBV3	993	614	0.08%	0.010%




Sum of corrected areas: 6463109

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071723\
Data File : VU054795.D
Acq On : 17 Jul 2023 16:06
Operator : MD/SY
Sample : VU0717WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK098

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

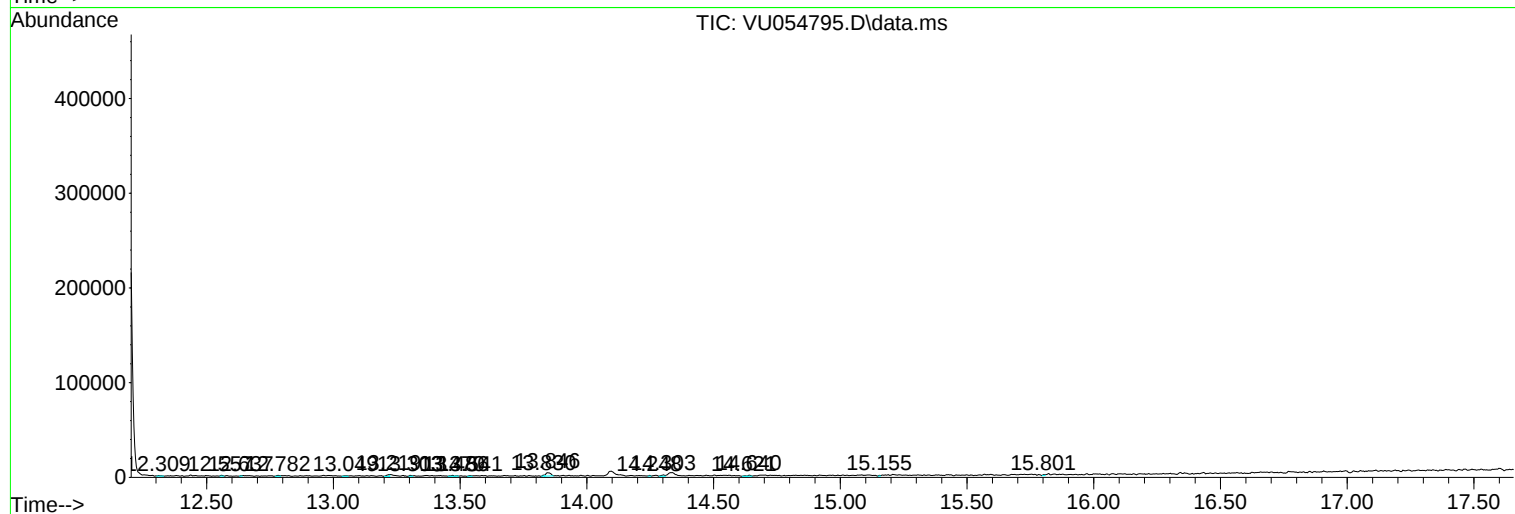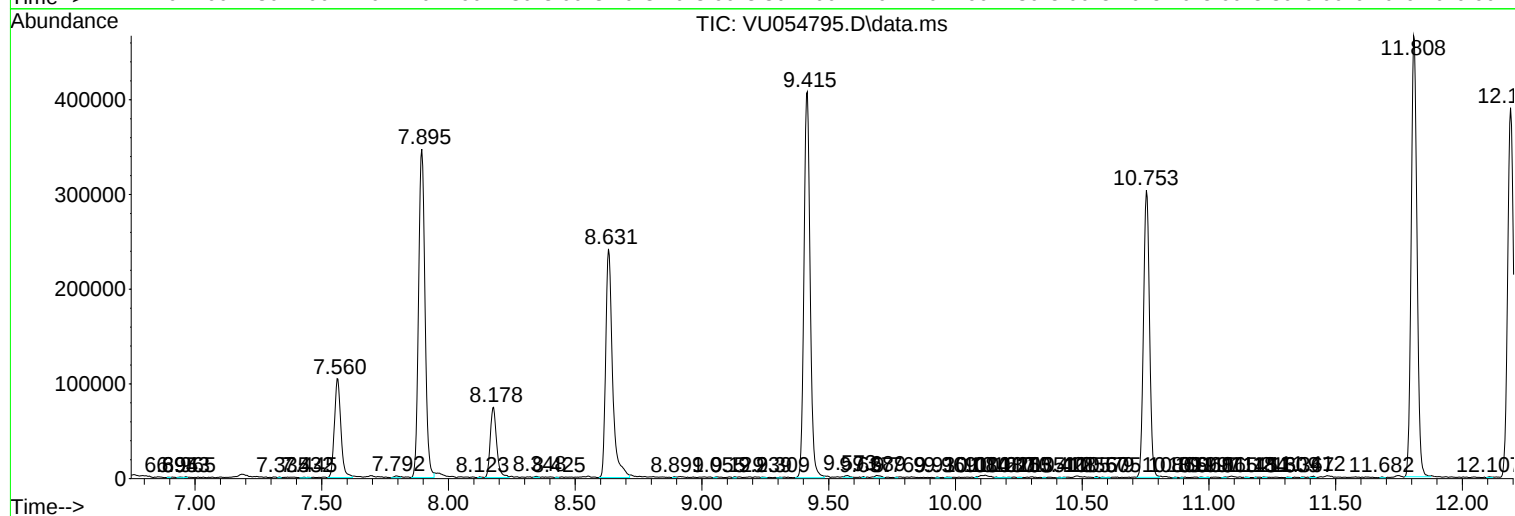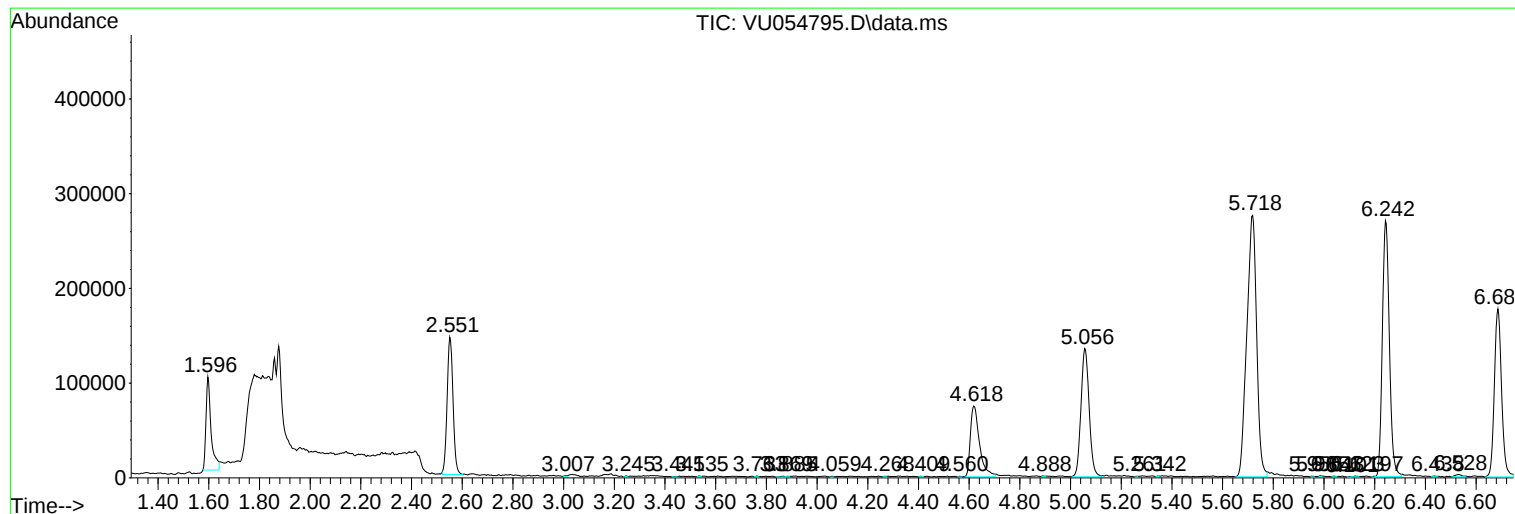

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071723\
Data File : VU054795.D
Acq On : 17 Jul 2023 16:06
Operator : MD/SY
Sample : VU0717WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK098

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071723\
Data File : VU054795.D
Acq On : 17 Jul 2023 16:06
Operator : MD/SY
Sample : VU0717WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK098

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------