


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071723\
Data File : VU054787.D
Acq On : 17 Jul 2023 08:59
Operator : MD/SY
Sample : BFB001
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB001

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Title : VOC Analysis
Last Update : Tue Jul 18 05:50:33 2023

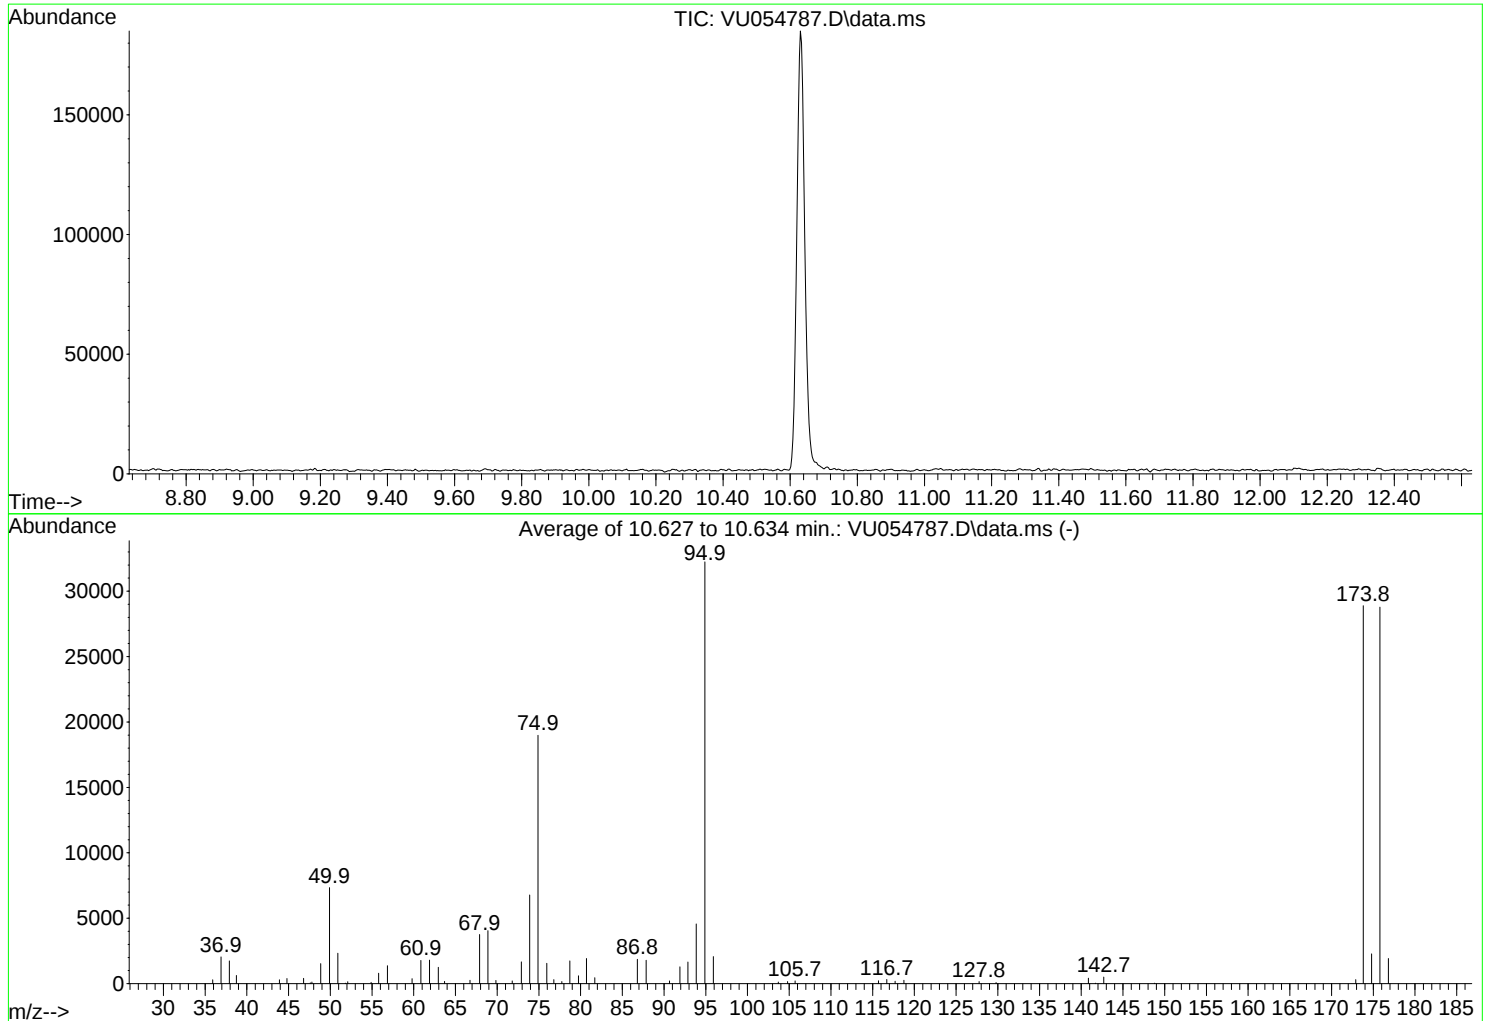

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2893

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	7345	PASS
75	95	30	80	58.9	18984	PASS
95	95	100	100	100.0	32243	PASS
96	95	5	9	6.4	2068	PASS
173	174	0.00	2	1.0	303	PASS
174	95	50	120	89.6	28891	PASS
175	174	5	9	7.9	2273	PASS
176	174	95	101	99.6	28781	PASS
177	176	5	9	6.7	1922	PASS

m/z	Abundance
38.80	107.0
40.00	167.0
40.90	250.0
42.80	176.0
43.90	699.0
54.80	157.0
69.70	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001

m/z	Abundance
35.90	319.0
36.90	1969.0
37.90	1745.0
38.70	741.0
39.80	160.0
40.90	202.0
42.80	153.0
43.90	969.0
44.80	461.0
46.80	336.0
47.60	175.0
48.90	1486.0
49.90	7276.0
50.90	2333.0
52.00	128.0
55.00	233.0
55.80	786.0
56.80	1368.0
59.80	336.0
60.80	1903.0
61.90	1750.0
63.00	1219.0
63.70	182.0
66.70	281.0
67.90	3868.0
68.90	4014.0
69.90	387.0
71.90	202.0
72.90	1851.0
73.90	6402.0
74.90	18192.0
76.00	1536.0
76.80	305.0
77.80	166.0
78.70	1687.0
79.80	528.0
80.70	1831.0
81.70	396.0
86.80	1824.0
87.80	1643.0
90.70	239.0
91.90	1240.0
92.90	1679.0
93.90	4540.0
94.90	31600.0
95.90	2198.0
104.80	189.0
105.70	198.0
115.70	246.0
116.70	270.0
117.70	224.0
118.90	229.0
127.70	128.0
140.90	401.0
142.70	408.0
172.90	261.0
173.80	27408.0
174.80	2227.0
175.80	27432.0
176.80	1953.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001

m/z	Abundance
35.90	306.0
36.90	2124.0
37.90	1777.0
38.80	752.0
39.80	145.0
40.90	211.0
42.70	147.0
43.90	1025.0
44.80	399.0
46.80	444.0
47.80	170.0
48.90	1557.0
49.90	7563.0
50.90	2389.0
52.10	167.0
55.00	274.0
55.80	812.0
56.90	1380.0
59.80	377.0
60.80	1817.0
61.90	1841.0
63.00	1267.0
63.70	183.0
66.80	272.0
67.90	3858.0
68.90	4116.0
69.90	348.0
71.80	209.0
72.90	1706.0
73.90	7005.0
74.90	19696.0
76.00	1564.0
76.80	328.0
77.70	170.0
78.70	1799.0
79.70	628.0
80.70	1971.0
81.70	476.0
86.80	1909.0
87.90	1868.0
90.70	207.0
91.90	1312.0
92.90	1684.0
93.90	4594.0
94.90	33136.0
95.90	2091.0
103.70	149.0
104.80	161.0
105.70	210.0
115.70	223.0
116.70	337.0
117.70	198.0
118.70	263.0
127.80	170.0
129.80	113.0
140.80	443.0
142.70	560.0
172.90	312.0
173.80	29752.0
174.80	2382.0
175.80	29712.0
176.80	1966.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001

m/z	Abundance
35.90	245.0
36.90	2028.0
37.90	1697.0
38.80	720.0
39.80	171.0
40.90	183.0
42.70	121.0
43.90	994.0
44.80	330.0
46.80	422.0
47.80	195.0
48.80	1556.0
49.90	7195.0
50.90	2246.0
51.80	122.0
52.20	140.0
55.00	258.0
55.80	788.0
56.90	1371.0
59.80	421.0
60.90	1609.0
61.90	1822.0
62.90	1264.0
63.70	163.0
66.80	224.0
67.90	3557.0
68.90	4030.0
69.90	342.0
71.70	201.0
72.90	1421.0
73.90	6940.0
74.90	19064.0
75.90	1572.0
76.80	292.0
77.80	131.0
78.70	1731.0
79.70	638.0
80.70	1945.0
81.70	476.0
86.80	1850.0
87.90	1855.0
90.60	185.0
91.90	1321.0
92.80	1607.0
93.80	4540.0
94.90	31992.0
95.90	1915.0
103.70	213.0
104.80	127.0
105.70	216.0
115.70	211.0
116.70	337.0
117.60	119.0
118.70	292.0
127.80	165.0
129.80	128.0
140.80	423.0
141.70	109.0
142.70	551.0
148.80	101.0
172.90	335.0
173.80	29512.0
174.80	2210.0
175.80	29200.0
176.80	1846.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001