

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU059993.D
 Acq On : 17 Jul 2024 14:32
 Operator : MD/SY
 Sample : P3260-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jul 18 02:48:37 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 18 02:31:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	231321	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	231888	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	99310	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	54487	36.686	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	73.380%		
7) Chloroethane-d5	1.904	69	50306	40.268	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	80.540%		
11) 1,1-Dichloroethene-d2	2.557	63	72287	27.396	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	54.800%#		
21) 2-Butanone-d5	4.618	46	102894	99.686	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	99.690%		
24) Chloroform-d	5.055	84	123359	42.890	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.780%		
26) 1,2-Dichloroethane-d4	5.695	65	77281	45.189	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.380%		
32) Benzene-d6	5.721	84	238374	40.144	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.280%		
36) 1,2-Dichloropropane-d6	6.682	67	80881	44.010	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.020%		
41) Toluene-d8	7.894	98	198677	35.184	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	70.360%#		
43) trans-1,3-Dichloroprop...	8.174	79	31986	37.194	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.380%		
47) 2-Hexanone-d5	8.627	63	66334	85.645	ug/L	-0.01
Spiked Amount 100.000	Range 45 - 130		Recovery =	85.650%		
56) 1,1,2,2-Tetrachloroeth...	10.749	84	134035	47.517	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.040%		
66) 1,2-Dichlorobenzene-d4	12.187	152	79833	43.746	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.500%		
Target Compounds						
					Qvalue	
60) 1,2,3-Trichloropropane	11.804	75	10945	5.807	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU059993.D
Acq On : 17 Jul 2024 14:32
Operator : MD/SY
Sample : P3260-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Jul 18 02:48:37 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 18 02:31:59 2024
Response via : Initial Calibration

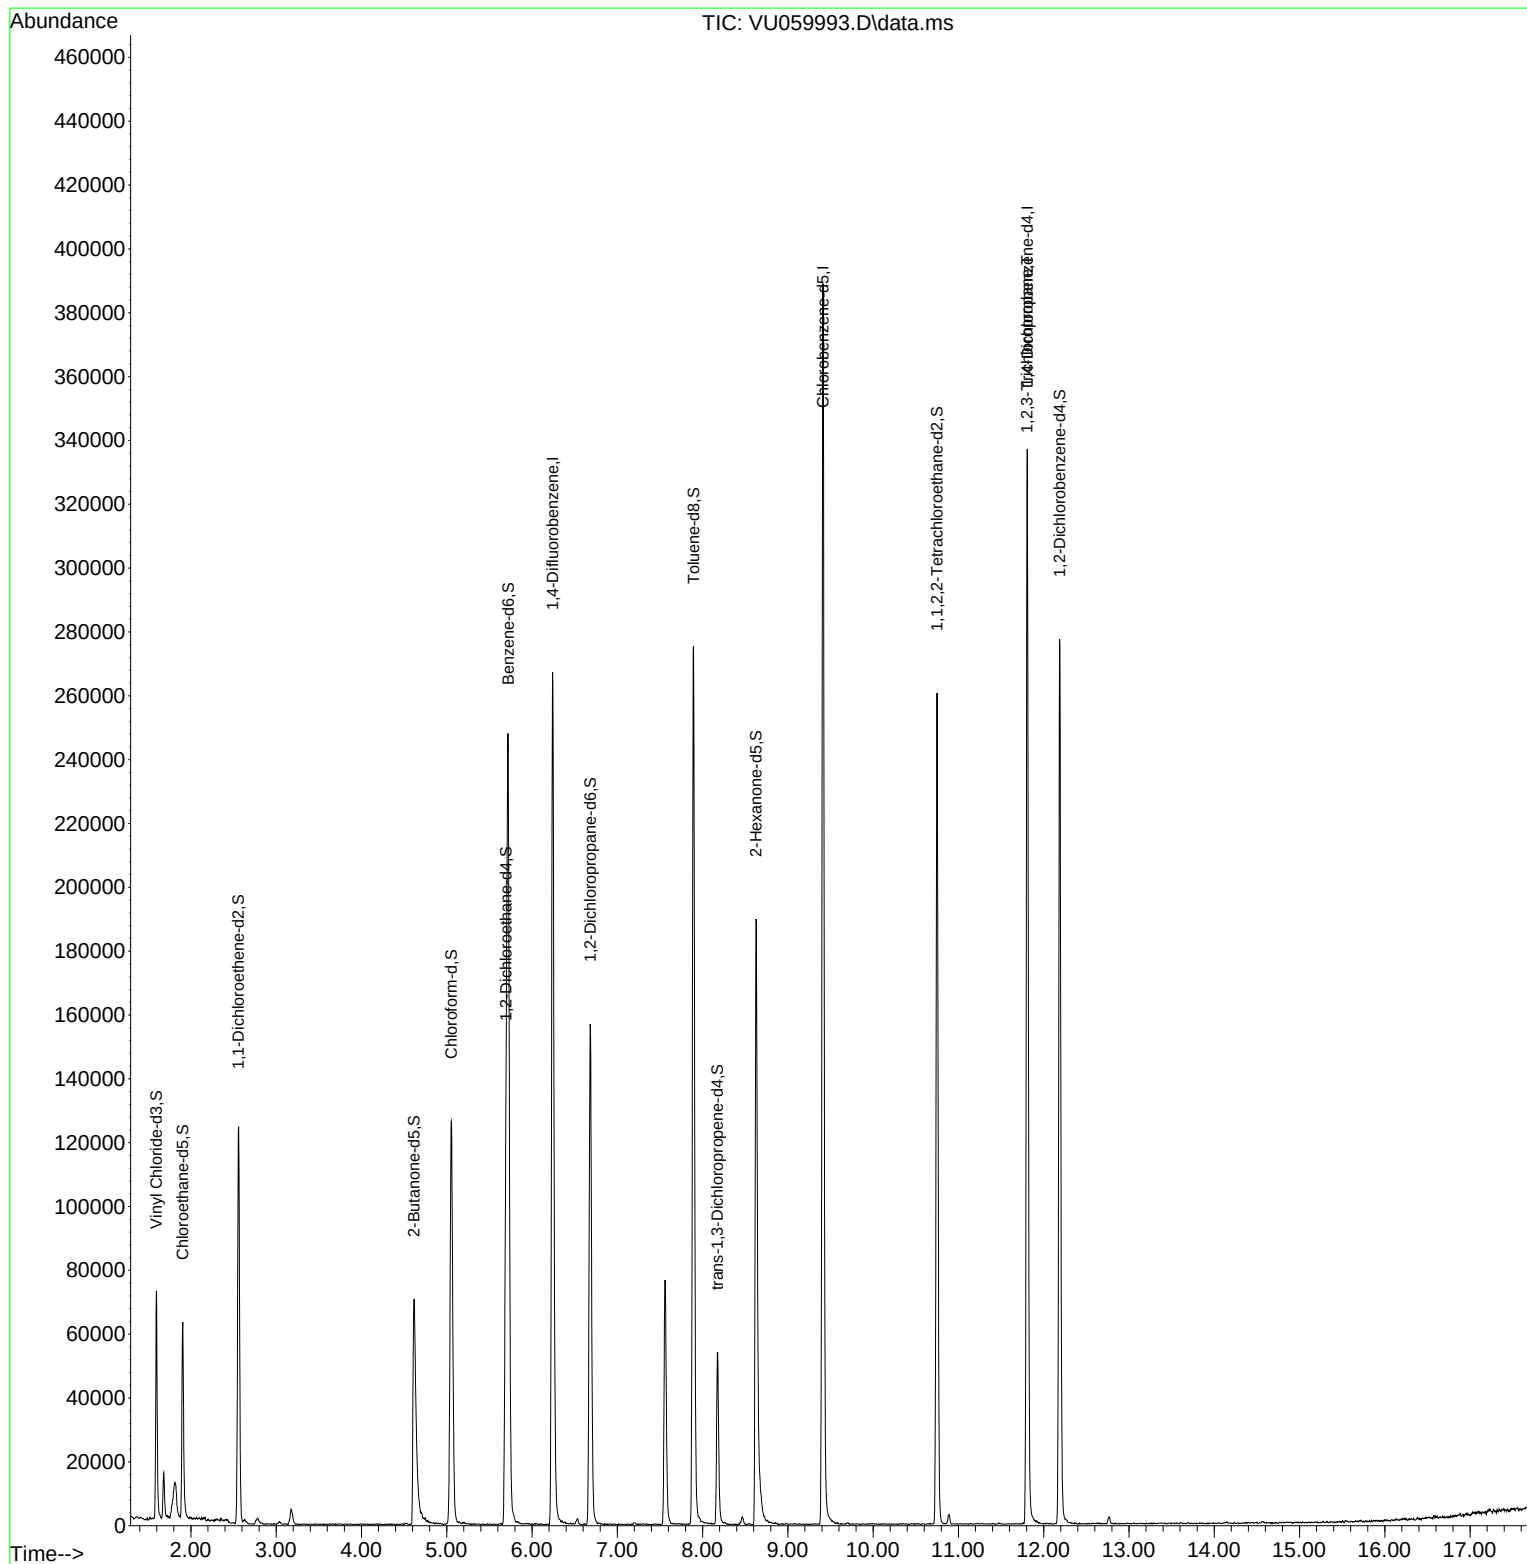

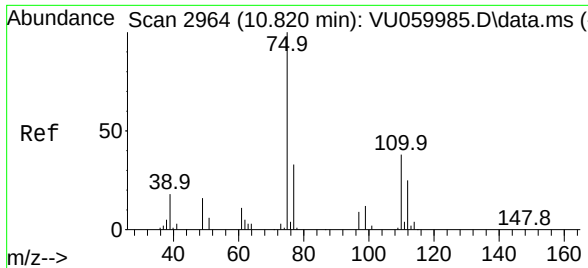

#60
1,2,3-Trichloropropane
Concen: 5.807 ug/L
RT: 11.804 min Scan# 31
Delta R.T. 0.984 min
Lab File: VU059993.D
Acq: 17 Jul 2024 14:32

Instrument :
MSVOA_U
ClientSampleId :

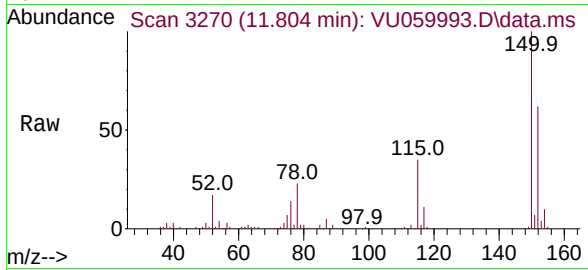

Tgt Ion: 75 Resp: 10945
Ion Ratio Lower Upper
75 100
77 34.9 25.5 38.3
110 1.6 30.7 46.1#

