

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU059997.D
 Acq On : 17 Jul 2024 16:06
 Operator : MD/SY
 Sample : P3260-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jul 18 02:49:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 18 02:31:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	213277	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	219132	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	92662	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	53069	38.754	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	77.500%		
7) Chloroethane-d5	1.904	69	48384	42.006	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	84.020%		
11) 1,1-Dichloroethene-d2	2.560	63	69175	28.434	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	56.860%#		
21) 2-Butanone-d5	4.618	46	104066	109.351	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	109.350%		
24) Chloroform-d	5.055	84	121900	45.968	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.940%		
26) 1,2-Dichloroethane-d4	5.695	65	75638	47.971	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.940%		
32) Benzene-d6	5.721	84	234142	41.727	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.460%		
36) 1,2-Dichloropropane-d6	6.682	67	79911	46.013	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.020%		
41) Toluene-d8	7.894	98	196496	36.823	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	73.640%#		
43) trans-1,3-Dichloroprop...	8.177	79	32213	39.639	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	79.280%		
47) 2-Hexanone-d5	8.627	63	70749	96.663	ug/L	-0.01
Spiked Amount 100.000	Range 45 - 130		Recovery =	96.660%		
56) 1,1,2,2-Tetrachloroeth...	10.750	84	131024	49.154	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.300%		
66) 1,2-Dichlorobenzene-d4	12.190	152	81165	47.667	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.340%		
Target Compounds						
					Qvalue	
34) Trichloroethene	6.537	95	14295	9.053	ug/L	97
37) 1,2-Dichloropropane	6.682	63	8302	5.097	ug/L #	88
45) 1,1,2-Trichloroethane	8.544	97	4274	2.506	ug/L #	1
46) Tetrachloroethene	8.547	164	597604	460.029	ug/L	99
49) Dibromochloromethane	8.811	129	3091	1.839	ug/L	91
60) 1,2,3-Trichloropropane	11.807	75	9487	5.395	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU059997.D
Acq On : 17 Jul 2024 16:06
Operator : MD/SY
Sample : P3260-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Jul 18 02:49:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 18 02:31:59 2024
Response via : Initial Calibration

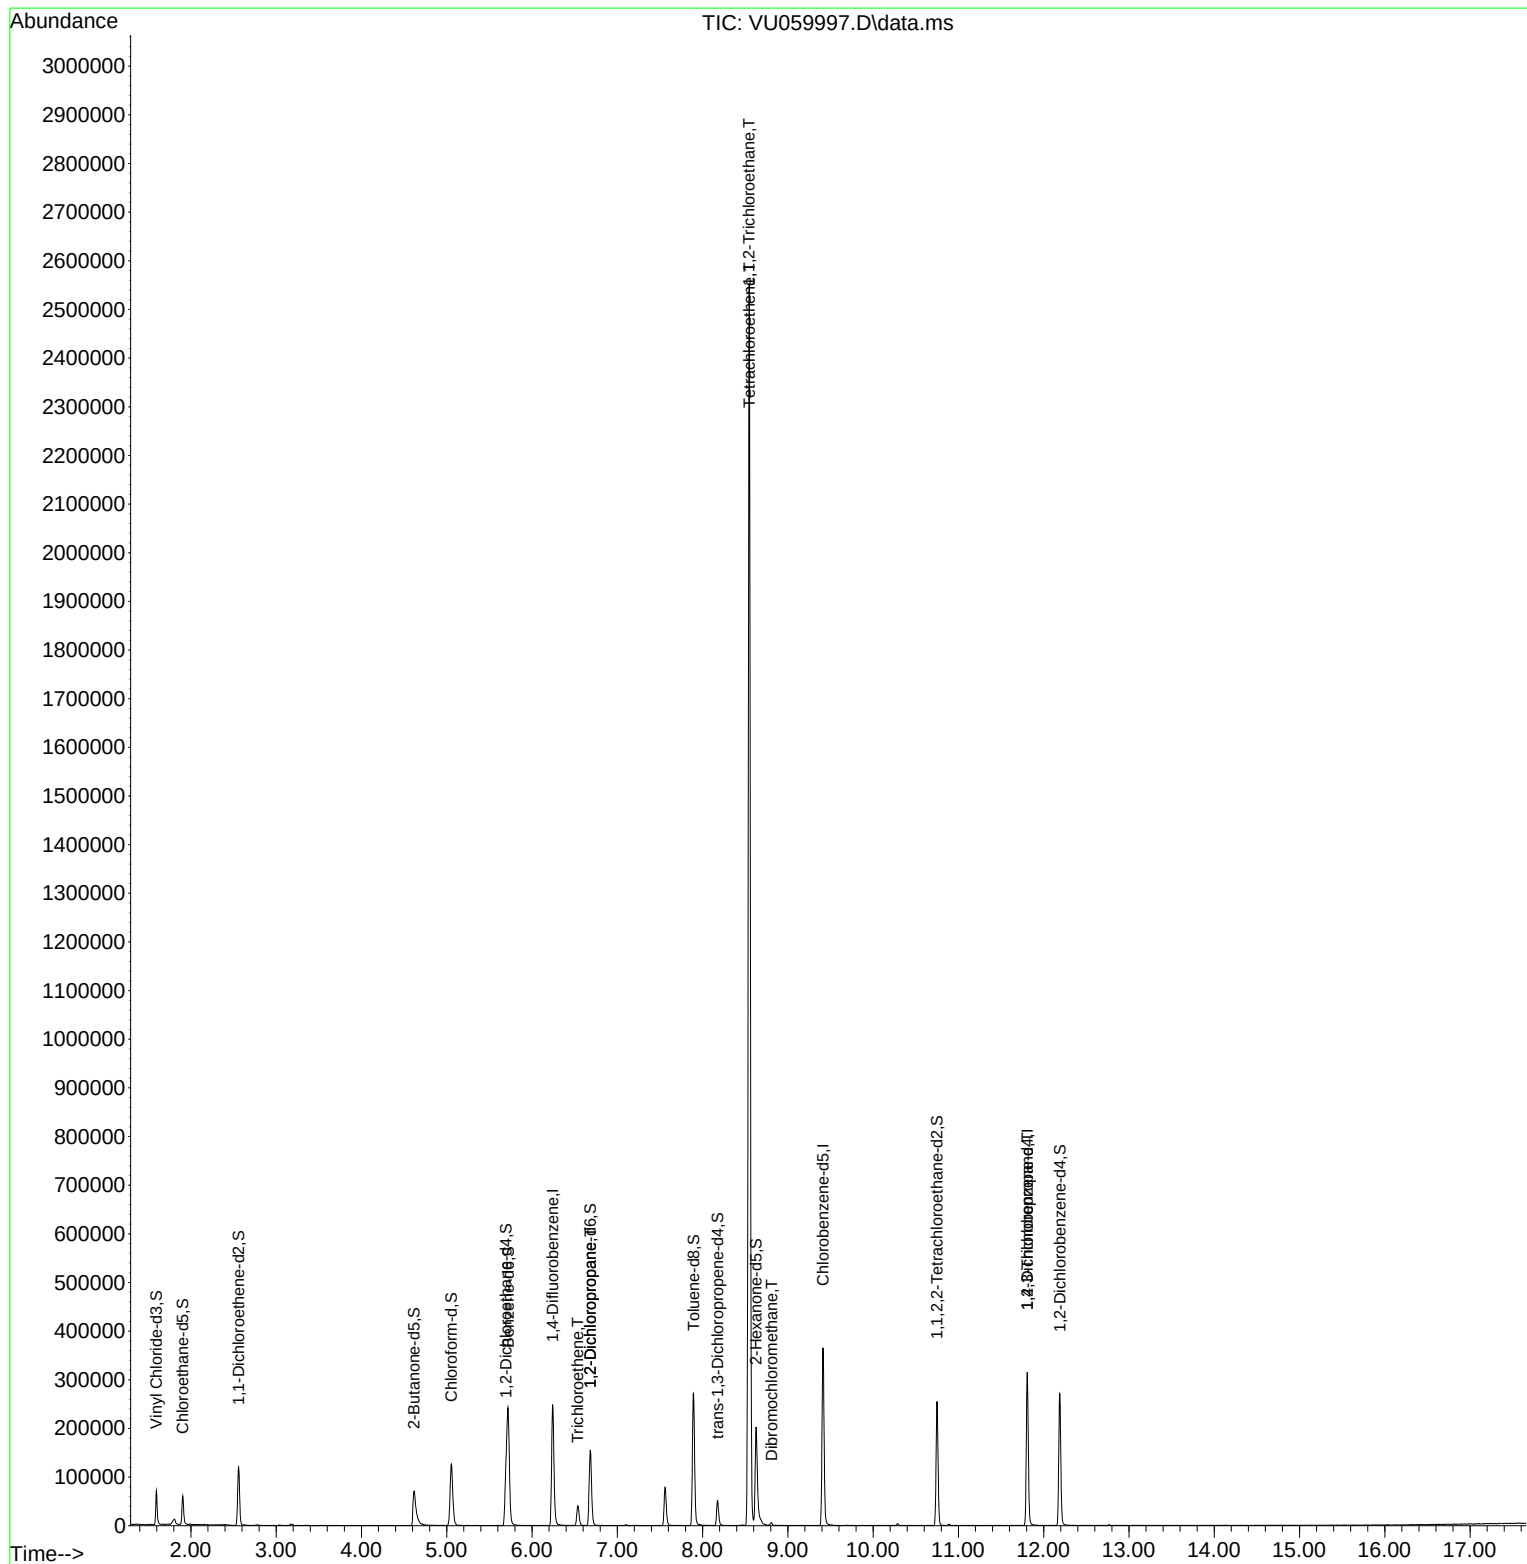

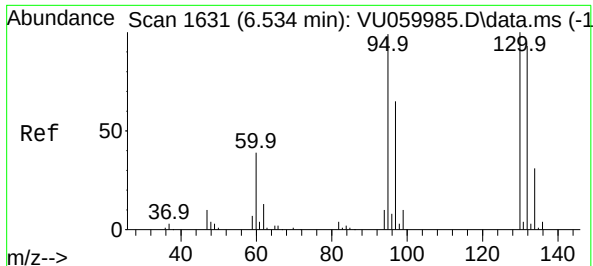




#34
Trichloroethene
Concen: 9.053 ug/L
RT: 6.537 min Scan# 1631
Delta R.T. 0.003 min
Lab File: VU059997.D
Acq: 17 Jul 2024 16:06

Instrument :
MSVOA_U
ClientSampleId :

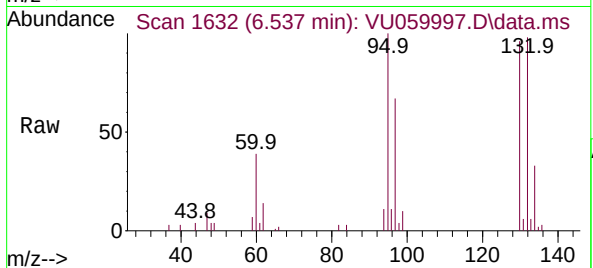

Tgt Ion: 95 Resp: 14295




Ion	Ratio	Lower	Upper
95	100		
97	67.2	45.8	85.2
132	97.8	69.8	129.6
130	96.4	70.8	131.6

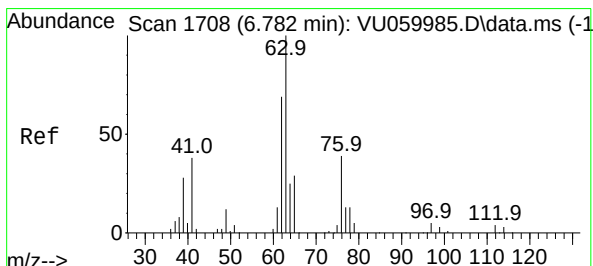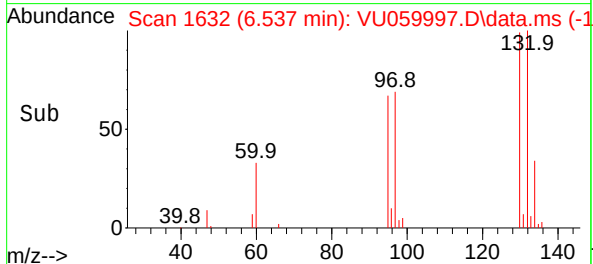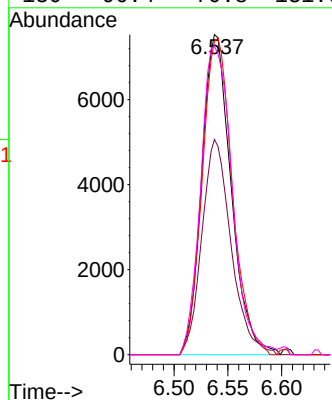


#37
1,2-Dichloropropane
Concen: 5.097 ug/L
RT: 6.682 min Scan# 1677
Delta R.T. -0.100 min
Lab File: VU059997.D
Acq: 17 Jul 2024 16:06

Tgt Ion: 63 Resp: 8302

Ion	Ratio	Lower	Upper
63	100		
112	0.0	3.0	4.6#


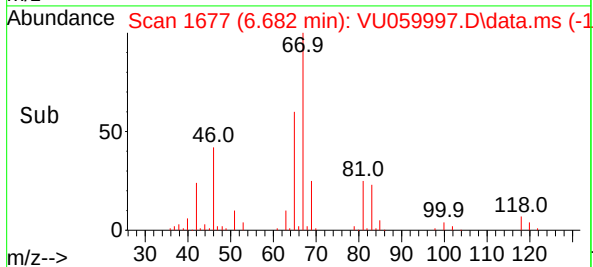
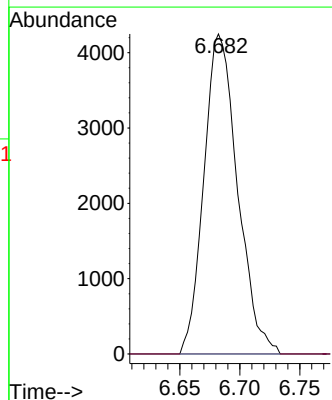
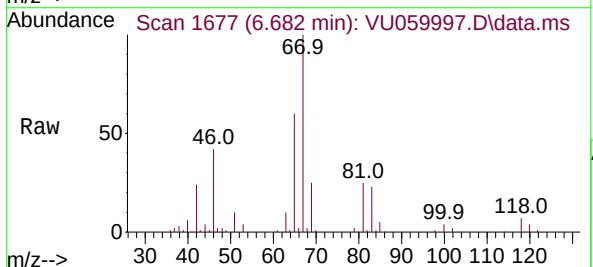


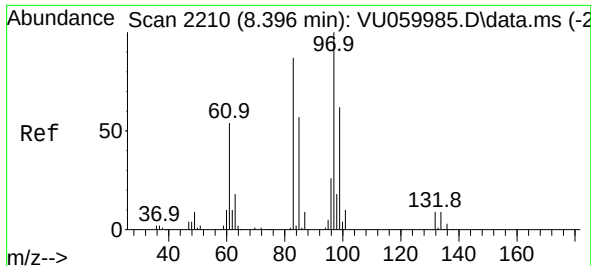

#45
1,1,2-Trichloroethane
Concen: 2.506 ug/L
RT: 8.544 min Scan# 2210
Delta R.T. 0.148 min
Lab File: VU059997.D
Acq: 17 Jul 2024 16:06




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 97 Resp: 4274
Ion Ratio Lower Upper
97 100
99 16.7 43.1 80.1#
83 299.1 60.4 112.2#
85 42.9 38.8 72.0

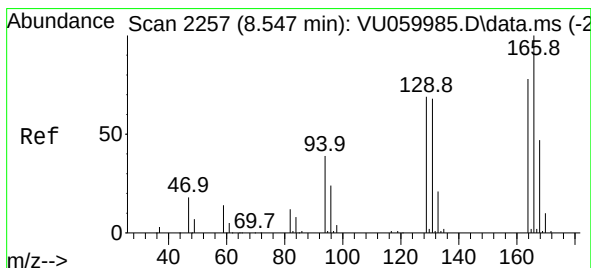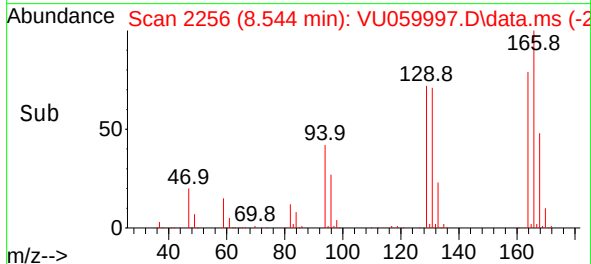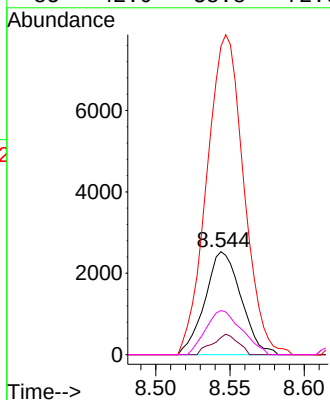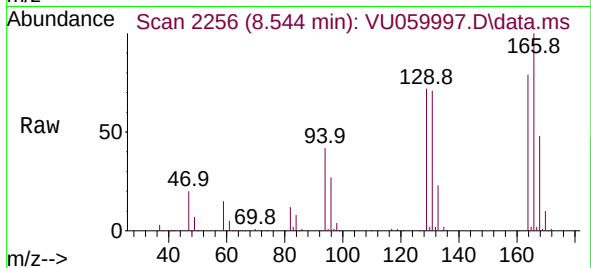

#46
Tetrachloroethene
Concen: 460.029 ug/L
RT: 8.547 min Scan# 2257
Delta R.T. 0.000 min
Lab File: VU059997.D
Acq: 17 Jul 2024 16:06

Tgt Ion:164 Resp: 597604
Ion Ratio Lower Upper
164 100
129 91.0 62.7 116.5
131 88.8 62.3 115.7
166 127.7 88.9 165.1

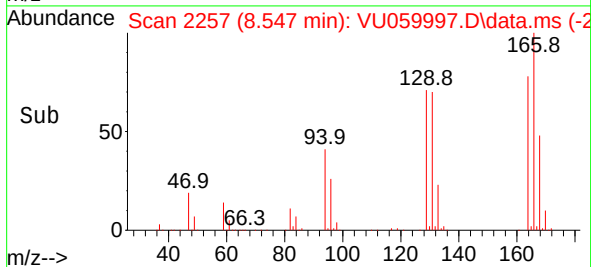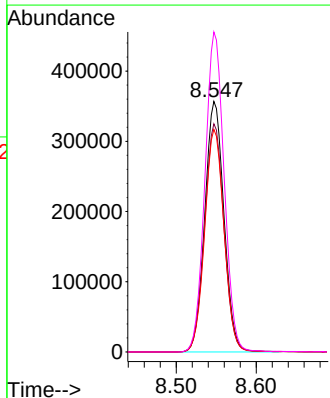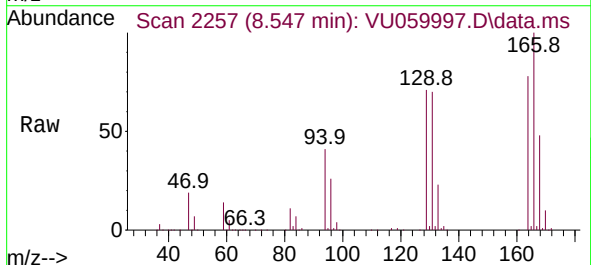

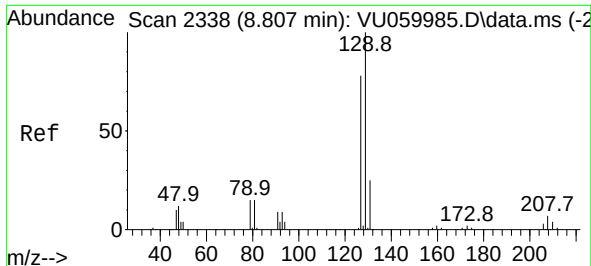

#49

Dibromochloromethane

Concen: 1.839 ug/L

RT: 8.811 min Scan# 2339

Delta R.T. 0.003 min

Lab File: VU059997.D

Acq: 17 Jul 2024 16:06

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion:129 Resp: 3091

Ion Ratio Lower Upper

129 100

127 69.2 54.0 100.2

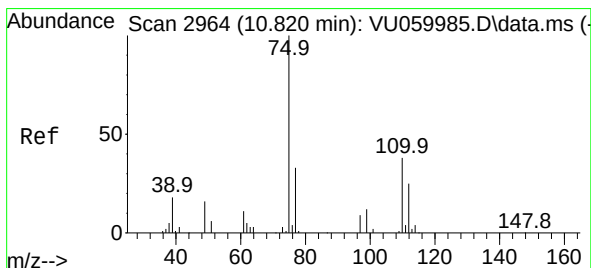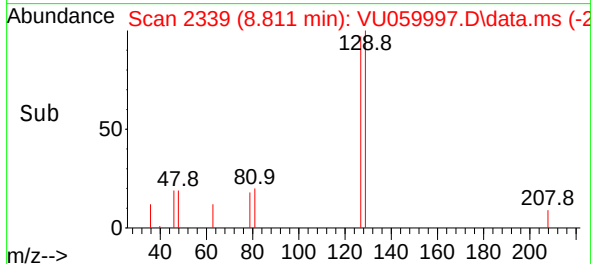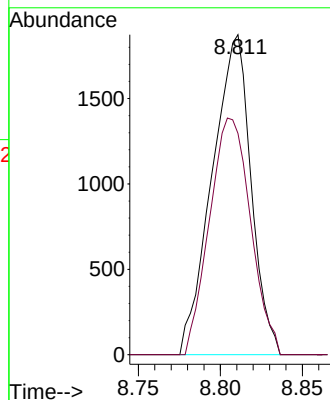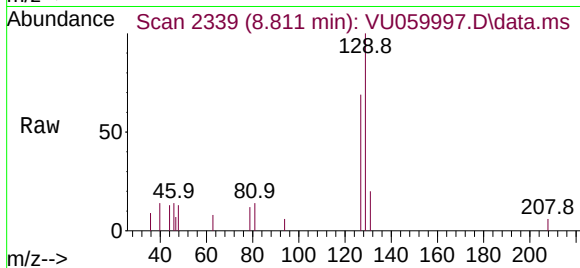

#60

1,2,3-Trichloropropane

Concen: 5.395 ug/L

RT: 11.807 min Scan# 3271

Delta R.T. 0.987 min

Lab File: VU059997.D

Acq: 17 Jul 2024 16:06

Tgt Ion: 75 Resp: 9487

Ion Ratio Lower Upper

75 100

77 29.7 25.5 38.3

110 1.8 30.7 46.1#

