

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU059989.D
 Acq On : 17 Jul 2024 13:00
 Operator : MD/SY
 Sample : P3260-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08F5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

Signal : TIC: VU059989.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	108	rBV	71311	82299	11.81%	1.455%
2	1.682	117	122	134	rVB	14226	17735	2.55%	0.314%
3	1.904	185	191	208	rVB	63969	88783	12.74%	1.570%
4	2.560	383	395	410	rBV	122918	201254	28.88%	3.558%
5	2.792	456	467	475	rBV5	1070	2331	0.33%	0.041%
6	2.965	517	521	524	rVB3	308	226	0.03%	0.004%
7	3.033	537	542	544	rBV2	1009	981	0.14%	0.017%
8	3.087	556	559	562	rVB2	195	106	0.02%	0.002%
9	3.132	569	573	574	rBV2	216	156	0.02%	0.003%
10	3.374	647	648	650	rBV	95	51	0.01%	0.001%
11	3.431	663	666	668	rBV	316	206	0.03%	0.004%
12	3.483	680	682	684	rVB2	135	56	0.01%	0.001%
13	3.502	684	688	691	rBV2	140	112	0.02%	0.002%
14	3.547	698	702	704	rBV2	191	149	0.02%	0.003%
15	3.679	741	743	745	rBV	218	128	0.02%	0.002%
16	3.747	760	764	766	rBV2	140	110	0.02%	0.002%
17	3.837	789	792	794	rBV	95	55	0.01%	0.001%
18	3.872	799	803	806	rBV2	240	207	0.03%	0.004%
19	3.910	812	815	817	rBV2	137	71	0.01%	0.001%
20	3.923	817	819	823	rBV2	175	136	0.02%	0.002%
21	3.994	836	841	843	rBV	213	169	0.02%	0.003%
22	4.062	860	862	864	rBV	137	84	0.01%	0.001%
23	4.139	882	886	891	rBV2	209	254	0.04%	0.004%
24	4.328	943	945	947	rBV	92	42	0.01%	0.001%
25	4.348	947	951	956	rVV2	255	256	0.04%	0.005%
26	4.377	956	960	964	rVB2	197	163	0.02%	0.003%
27	4.431	973	977	983	rBV	233	210	0.03%	0.004%
28	4.463	984	987	991	rVB2	209	127	0.02%	0.002%
29	4.486	991	994	997	rBV	217	146	0.02%	0.003%
30	4.618	1023	1035	1069	rBV	72380	197765	28.38%	3.496%
31	5.055	1157	1171	1196	rVB	128029	283251	40.65%	5.008%
32	5.209	1215	1219	1222	rBV2	129	126	0.02%	0.002%
33	5.258	1230	1234	1235	rBV	144	97	0.01%	0.002%
34	5.293	1242	1245	1249	rVB2	265	210	0.03%	0.004%
35	5.316	1249	1252	1255	rBV2	113	90	0.01%	0.002%
36	5.361	1263	1266	1270	rBV	226	175	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU059989.D
 Acq On : 17 Jul 2024 13:00
 Operator : MD/SY
 Sample : P3260-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08F5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	5.399	1275	1278	1283	rVV2	198	179	0.03%	0.003%
38	5.444	1290	1292	1295	rVB2	133	74	0.01%	0.001%
39	5.463	1295	1298	1300	rBV	151	85	0.01%	0.002%
40	5.579	1330	1334	1337	rBV	176	154	0.02%	0.003%
41	5.618	1345	1346	1355	rBV2	180	202	0.03%	0.004%
42	5.717	1357	1377	1407	rBV2	254240	696827	100.00%	12.320%
43	5.926	1439	1442	1446	rBV	229	174	0.02%	0.003%
44	6.074	1485	1488	1493	rVB2	282	195	0.03%	0.003%
45	6.113	1493	1500	1501	rBV2	222	163	0.02%	0.003%
46	6.168	1512	1517	1520	rBV	226	252	0.04%	0.004%
47	6.242	1527	1540	1563	rBV	263494	507210	72.79%	8.967%
48	6.451	1603	1605	1611	rVB3	582	437	0.06%	0.008%
49	6.528	1620	1629	1630	rBV3	1572	1667	0.24%	0.029%
50	6.576	1641	1644	1648	rBV	108	124	0.02%	0.002%
51	6.605	1651	1653	1655	rVV	190	81	0.01%	0.001%
52	6.682	1661	1677	1700	rBV	161711	322197	46.24%	5.696%
53	6.814	1716	1718	1720	rVB2	475	148	0.02%	0.003%
54	6.827	1720	1722	1725	rBV2	353	174	0.02%	0.003%
55	6.907	1744	1747	1749	rBV	112	76	0.01%	0.001%
56	6.962	1760	1764	1766	rBV2	175	120	0.02%	0.002%
57	7.049	1786	1791	1793	rBV	301	338	0.05%	0.006%
58	7.100	1803	1807	1808	rBV	276	180	0.03%	0.003%
59	7.142	1812	1820	1822	rBV	329	423	0.06%	0.007%
60	7.290	1863	1866	1868	rBV2	130	77	0.01%	0.001%
61	7.441	1911	1913	1915	rBV	58	33	0.00%	0.001%
62	7.476	1919	1924	1926	rBV2	141	135	0.02%	0.002%
63	7.560	1938	1950	1976	rBV	80230	145282	20.85%	2.569%
64	7.756	2009	2011	2013	rBV	195	95	0.01%	0.002%
65	7.798	2021	2024	2025	rBV2	241	140	0.02%	0.002%
66	7.891	2041	2053	2069	rBV	285501	505973	72.61%	8.945%
67	8.174	2131	2141	2163	rBV	56276	96986	13.92%	1.715%
68	8.290	2175	2177	2180	rBV	290	175	0.03%	0.003%
69	8.332	2188	2190	2191	rVB	215	49	0.01%	0.001%
70	8.360	2196	2199	2202	rVV	312	187	0.03%	0.003%
71	8.467	2219	2232	2244	rBV2	9422	16308	2.34%	0.288%
72	8.631	2272	2283	2315	rBV	194728	382902	54.95%	6.770%
73	8.881	2358	2361	2363	rBV3	262	192	0.03%	0.003%
74	8.952	2380	2383	2386	rBV	185	101	0.01%	0.002%
75	8.968	2386	2388	2391	rVB	150	67	0.01%	0.001%
76	8.987	2391	2394	2399	rBV2	313	276	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU059989.D
 Acq On : 17 Jul 2024 13:00
 Operator : MD/SY
 Sample : P3260-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08F5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	9.042	2408	2411	2413	rBV	129	92	0.01%	0.002%
78	9.412	2514	2526	2551	rBV	382893	641320	92.03%	11.338%
79	9.569	2571	2575	2586	rVB5	1257	1827	0.26%	0.032%
80	9.695	2608	2614	2621	rBV4	1043	1713	0.25%	0.030%
81	9.939	2687	2690	2694	rBV2	121	93	0.01%	0.002%
82	10.010	2709	2712	2714	rBV2	302	188	0.03%	0.003%
83	10.277	2792	2795	2798	rBV2	281	190	0.03%	0.003%
84	10.319	2803	2808	2811	rBV2	192	183	0.03%	0.003%
85	10.364	2820	2822	2823	rBV	308	75	0.01%	0.001%
86	10.483	2854	2859	2867	rVB3	829	1054	0.15%	0.019%
87	10.560	2879	2883	2885	rBV2	224	173	0.02%	0.003%
88	10.656	2910	2913	2917	rBV	232	162	0.02%	0.003%
89	10.749	2930	2942	2961	rBV	269088	437083	62.72%	7.727%
90	10.888	2976	2985	2998	rVB3	11332	18387	2.64%	0.325%
91	11.807	3259	3271	3295	rBV	324376	524298	75.24%	9.269%
92	12.029	3337	3340	3344	rBV2	308	265	0.04%	0.005%
93	12.187	3377	3389	3409	rBV	275200	461243	66.19%	8.155%
94	12.717	3552	3554	3556	rBV	361	226	0.03%	0.004%
95	12.769	3564	3570	3580	rVB2	5229	7811	1.12%	0.138%
96	13.862	3904	3910	3917	rVB4	833	1097	0.16%	0.019%




Sum of corrected areas: 5656255

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU059989.D
Acq On : 17 Jul 2024 13:00
Operator : MD/SY
Sample : P3260-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

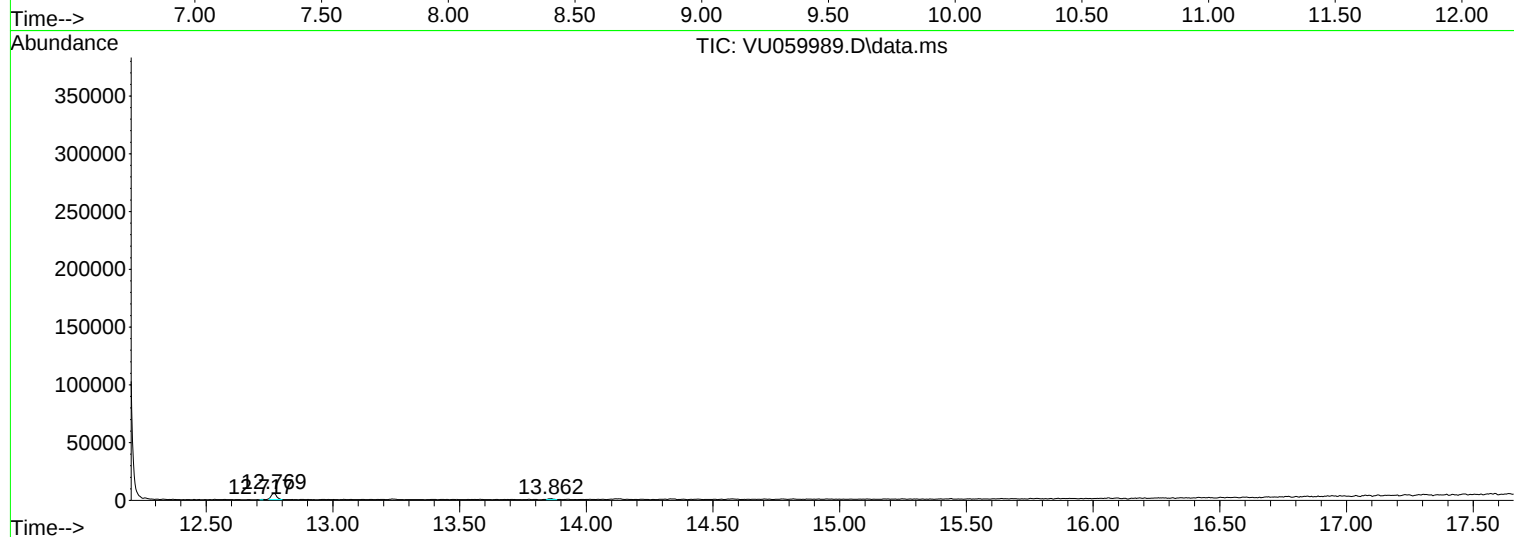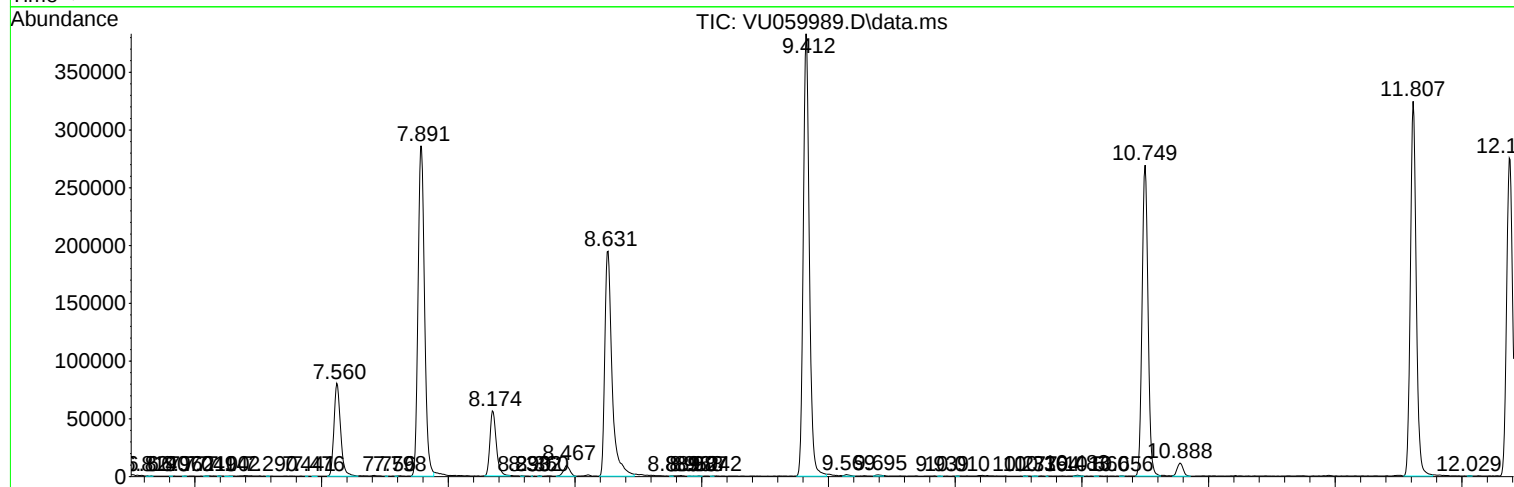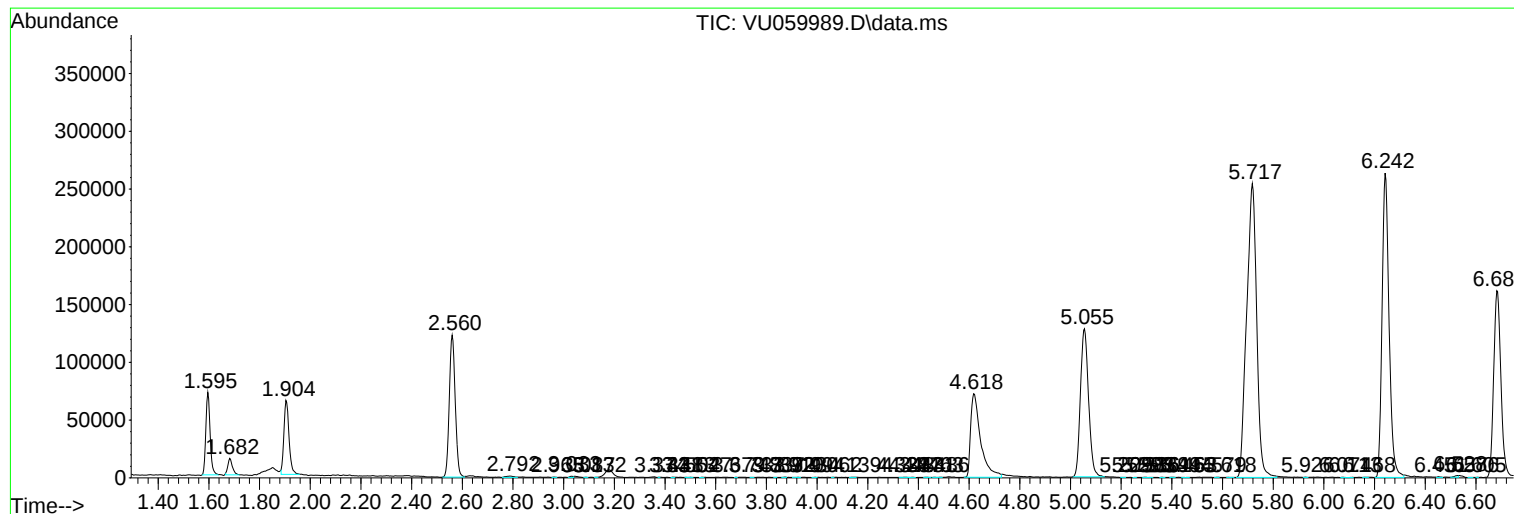

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU059989.D
Acq On : 17 Jul 2024 13:00
Operator : MD/SY
Sample : P3260-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU059989.D
Acq On : 17 Jul 2024 13:00
Operator : MD/SY
Sample : P3260-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------