

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU059997.D
 Acq On : 17 Jul 2024 16:06
 Operator : MD/SY
 Sample : P3260-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08G0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU059997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	110	rBV	68846	82633	1.93%	0.844%
2	1.904	184	191	209	rVB	58919	85007	1.99%	0.868%
3	2.560	383	395	409	rBV	119226	194542	4.55%	1.987%
4	2.779	452	463	479	rBV5	1551	3804	0.09%	0.039%
5	2.840	480	482	484	rBV2	196	103	0.00%	0.001%
6	3.042	537	545	555	rBV5	1150	1927	0.05%	0.020%
7	3.120	565	569	574	rBV2	235	303	0.01%	0.003%
8	3.178	576	587	599	rVV2	3088	6491	0.15%	0.066%
9	3.242	604	607	614	rVB2	255	322	0.01%	0.003%
10	3.277	614	618	621	rBV2	158	137	0.00%	0.001%
11	3.348	634	640	649	rBV2	538	939	0.02%	0.010%
12	3.438	665	668	673	rBV2	210	215	0.01%	0.002%
13	3.496	684	686	689	rVB	182	99	0.00%	0.001%
14	3.840	790	793	796	rBV2	141	93	0.00%	0.001%
15	3.856	796	798	800	rBV	203	113	0.00%	0.001%
16	3.907	811	814	819	rBV2	185	151	0.00%	0.002%
17	4.081	865	868	874	rVB2	336	274	0.01%	0.003%
18	4.113	875	878	881	rVB	238	145	0.00%	0.001%
19	4.139	883	886	888	rBV2	133	75	0.00%	0.001%
20	4.155	888	891	894	rBV	248	155	0.00%	0.002%
21	4.358	951	954	956	rBV	186	123	0.00%	0.001%
22	4.454	979	984	987	rBV2	119	131	0.00%	0.001%
23	4.499	994	998	1006	rBV2	131	188	0.00%	0.002%
24	4.618	1025	1035	1070	rBV	70722	189733	4.43%	1.938%
25	4.968	1141	1144	1151	rVB2	370	419	0.01%	0.004%
26	5.001	1151	1154	1156	rBV2	355	261	0.01%	0.003%
27	5.055	1156	1171	1197	rVV	126108	283498	6.63%	2.896%
28	5.229	1222	1225	1230	rBV2	396	337	0.01%	0.003%
29	5.251	1230	1232	1234	rVV	166	52	0.00%	0.001%
30	5.319	1250	1253	1255	rBV2	176	105	0.00%	0.001%
31	5.370	1266	1269	1271	rBV2	118	77	0.00%	0.001%
32	5.390	1271	1275	1277	rBV2	145	113	0.00%	0.001%
33	5.441	1289	1291	1292	rBV	105	47	0.00%	0.000%
34	5.496	1306	1308	1310	rBV	70	43	0.00%	0.000%
35	5.718	1358	1377	1410	rBV2	242421	665969	15.56%	6.803%
36	5.933	1440	1444	1448	rBV	200	190	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU059997.D
 Acq On : 17 Jul 2024 16:06
 Operator : MD/SY
 Sample : P3260-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08G0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	5.952	1448	1450	1452	rBV2	259	174	0.00%	0.002%
38	6.010	1465	1468	1471	rVB3	248	101	0.00%	0.001%
39	6.049	1475	1480	1483	rBV2	370	320	0.01%	0.003%
40	6.068	1483	1486	1488	rBV2	151	89	0.00%	0.001%
41	6.116	1498	1501	1505	rBV	173	142	0.00%	0.001%
42	6.168	1512	1517	1520	rBV2	356	284	0.01%	0.003%
43	6.187	1520	1523	1526	rBV2	81	52	0.00%	0.001%
44	6.242	1526	1540	1561	rBV	248727	476955	11.15%	4.872%
45	6.470	1606	1611	1615	rBV3	284	403	0.01%	0.004%
46	6.537	1621	1632	1651	rBV2	40623	79423	1.86%	0.811%
47	6.634	1660	1662	1664	rBV	154	76	0.00%	0.001%
48	6.682	1664	1677	1701	rBV	154621	307860	7.19%	3.145%
49	6.811	1715	1717	1721	rVB	499	222	0.01%	0.002%
50	6.955	1759	1762	1764	rBV2	117	57	0.00%	0.001%
51	6.972	1764	1767	1771	rBV2	257	146	0.00%	0.001%
52	7.017	1777	1781	1783	rBV	265	221	0.01%	0.002%
53	7.103	1798	1808	1822	rVB3	1540	2778	0.06%	0.028%
54	7.168	1825	1828	1831	rBV2	108	82	0.00%	0.001%
55	7.187	1831	1834	1836	rBV	373	303	0.01%	0.003%
56	7.280	1857	1863	1866	rVB2	124	116	0.00%	0.001%
57	7.300	1866	1869	1871	rBV	193	130	0.00%	0.001%
58	7.328	1875	1878	1885	rVV2	146	150	0.00%	0.002%
59	7.399	1897	1900	1902	rBV	81	53	0.00%	0.001%
60	7.476	1921	1924	1926	rBV2	125	81	0.00%	0.001%
61	7.492	1926	1929	1933	rVB2	240	166	0.00%	0.002%
62	7.560	1933	1950	1972	rBV	78486	139955	3.27%	1.430%
63	7.714	1993	1998	2000	rBV3	327	292	0.01%	0.003%
64	7.785	2018	2020	2021	rBV3	191	62	0.00%	0.001%
65	7.843	2036	2038	2041	rBV2	189	109	0.00%	0.001%
66	7.894	2041	2054	2072	rBV	271678	481299	11.25%	4.917%
67	8.126	2123	2126	2128	rBV2	277	176	0.00%	0.002%
68	8.174	2131	2141	2163	rVV	51292	90056	2.10%	0.920%
69	8.425	2216	2219	2223	rBV2	222	203	0.00%	0.002%
70	8.547	2243	2257	2273	rBV	2552965	4278886	100.00%	43.712%
71	8.627	2274	2282	2317	rVB	201405	395914	9.25%	4.045%
72	8.888	2359	2363	2366	rBV3	418	426	0.01%	0.004%
73	8.997	2394	2397	2401	rVB2	309	204	0.00%	0.002%
74	9.023	2402	2405	2407	rBV	116	82	0.00%	0.001%
75	9.107	2428	2431	2432	rBV	177	78	0.00%	0.001%
76	9.412	2514	2526	2548	rBV	365263	616012	14.40%	6.293%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU059997.D
 Acq On : 17 Jul 2024 16:06
 Operator : MD/SY
 Sample : P3260-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08G0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	9.634	2593	2595	2602	rBV2	151	97	0.00%	0.001%
78	9.695	2607	2614	2619	rBV3	607	873	0.02%	0.009%
79	9.750	2626	2631	2634	rBV2	398	391	0.01%	0.004%
80	9.846	2657	2661	2663	rBV2	175	139	0.00%	0.001%
81	10.287	2791	2798	2808	rVB3	3953	6038	0.14%	0.062%
82	10.328	2808	2811	2814	rBV	223	186	0.00%	0.002%
83	10.402	2830	2834	2837	rBV2	260	224	0.01%	0.002%
84	10.595	2892	2894	2897	rVB	313	159	0.00%	0.002%
85	10.750	2930	2942	2971	rBV	255229	413083	9.65%	4.220%
86	10.888	2979	2985	2997	rVB2	2908	4125	0.10%	0.042%
87	11.605	3205	3208	3211	rBV	271	174	0.00%	0.002%
88	11.807	3259	3271	3292	rBV	314895	513720	12.01%	5.248%
89	12.010	3331	3334	3337	rBV2	270	227	0.01%	0.002%
90	12.187	3376	3389	3418	rBV	271195	456341	10.66%	4.662%




Sum of corrected areas: 9788729

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU059997.D
Acq On : 17 Jul 2024 16:06
Operator : MD/SY
Sample : P3260-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08G0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

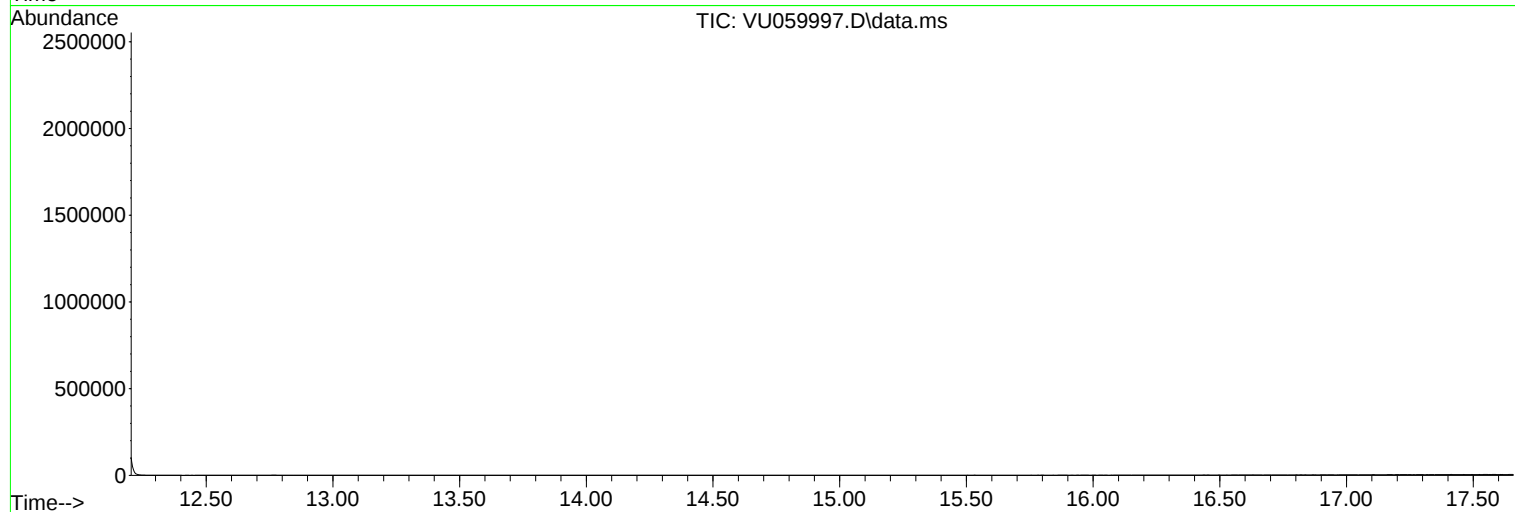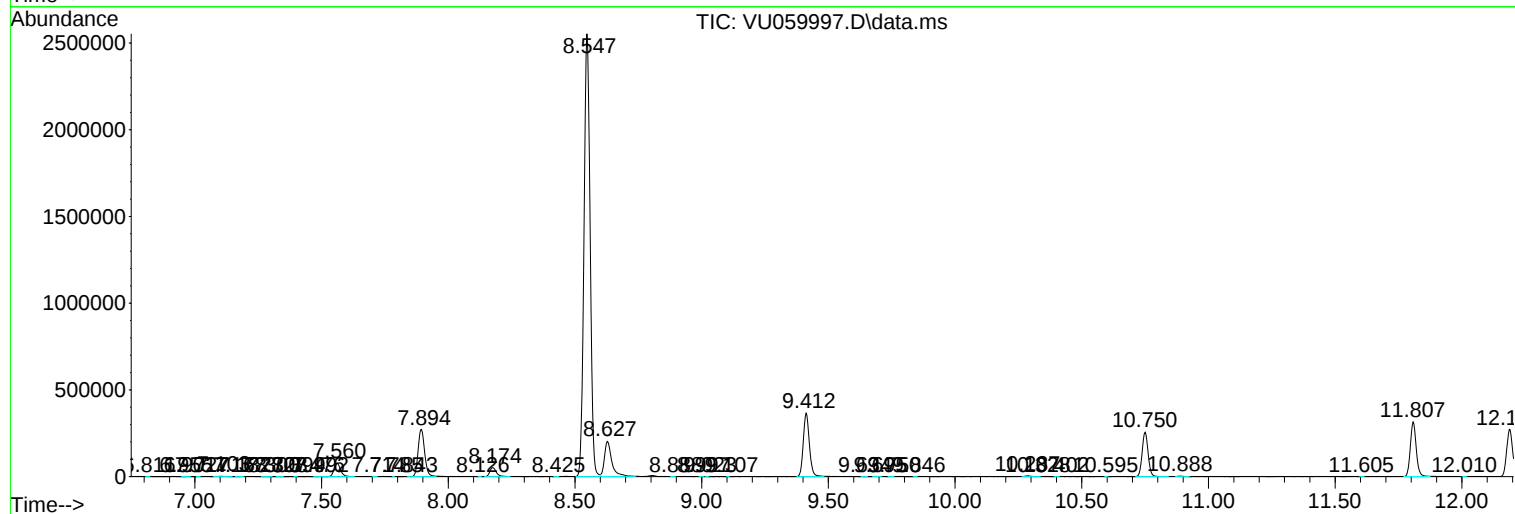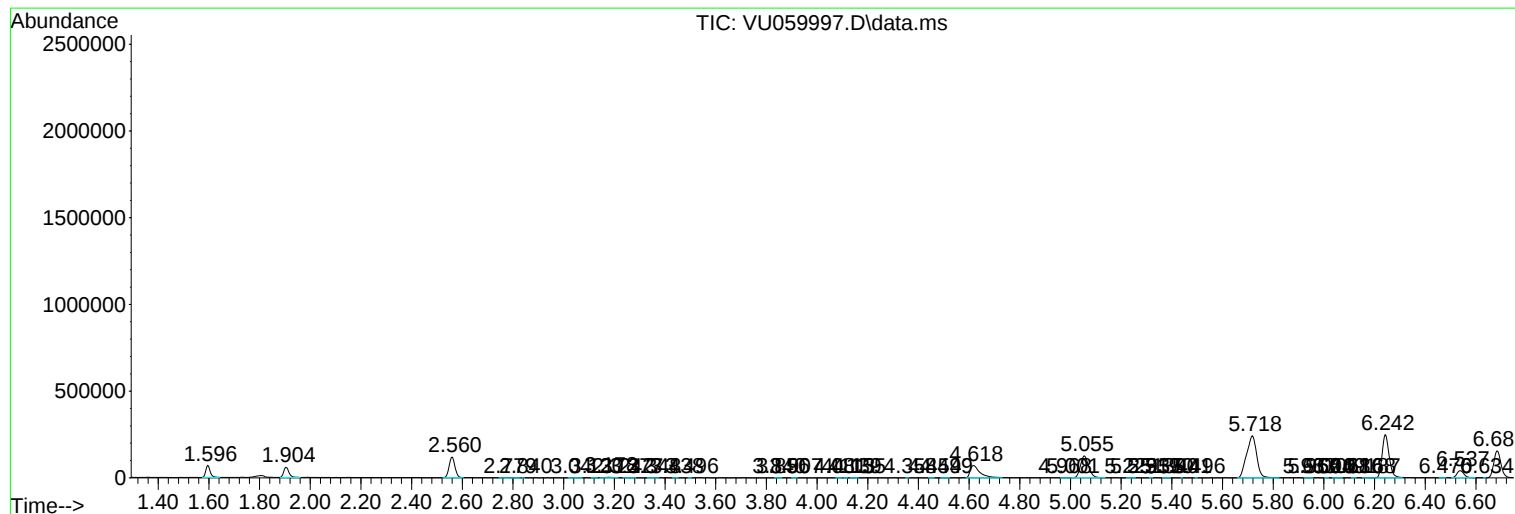

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU059997.D
Acq On : 17 Jul 2024 16:06
Operator : MD/SY
Sample : P3260-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08G0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU059997.D
Acq On : 17 Jul 2024 16:06
Operator : MD/SY
Sample : P3260-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08G0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------