

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU060001.D
 Acq On : 17 Jul 2024 18:05
 Operator : MD/SY
 Sample : P3277-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1ZQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

Signal : TIC: VU060001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	111	rVB	74796	90204	13.22%	1.621%
2	1.904	183	191	209	rVB	60932	86850	12.73%	1.561%
3	2.506	376	378	382	rVB	410	251	0.04%	0.005%
4	2.557	383	394	409	rBV	127478	209304	30.68%	3.761%
5	2.718	441	444	446	rVB	209	116	0.02%	0.002%
6	2.920	505	507	510	rVB	249	102	0.01%	0.002%
7	2.969	515	522	525	rBV2	243	356	0.05%	0.006%
8	3.078	553	556	559	rBV	137	108	0.02%	0.002%
9	3.178	573	587	601	rVB2	4448	10146	1.49%	0.182%
10	3.393	648	654	656	rBV	175	159	0.02%	0.003%
11	3.631	723	728	730	rBV2	134	108	0.02%	0.002%
12	3.756	761	767	772	rVB	259	285	0.04%	0.005%
13	3.782	772	775	777	rBV2	122	89	0.01%	0.002%
14	3.824	786	788	792	rBV	106	78	0.01%	0.001%
15	3.846	792	795	797	rVB2	144	83	0.01%	0.001%
16	3.862	797	800	802	rBV2	224	151	0.02%	0.003%
17	3.927	816	820	825	rBV	394	452	0.07%	0.008%
18	4.255	919	922	924	rBV2	160	103	0.02%	0.002%
19	4.383	957	962	968	rVB	271	253	0.04%	0.005%
20	4.444	978	981	985	rBV2	167	146	0.02%	0.003%
21	4.615	1023	1034	1067	rBV	74727	195884	28.72%	3.520%
22	4.940	1132	1135	1138	rBV	295	234	0.03%	0.004%
23	5.055	1156	1171	1194	rBV	126339	280599	41.14%	5.042%
24	5.229	1221	1225	1230	rBV2	508	379	0.06%	0.007%
25	5.293	1242	1245	1251	rBV2	154	127	0.02%	0.002%
26	5.374	1264	1270	1273	rBV2	290	237	0.03%	0.004%
27	5.390	1273	1275	1277	rBV	136	87	0.01%	0.002%
28	5.425	1282	1286	1290	rBV2	198	209	0.03%	0.004%
29	5.493	1303	1307	1310	rBV2	189	176	0.03%	0.003%
30	5.541	1319	1322	1323	rBV	228	113	0.02%	0.002%
31	5.602	1338	1341	1344	rVB	242	144	0.02%	0.003%
32	5.621	1344	1347	1349	rBV	174	103	0.02%	0.002%
33	5.718	1358	1377	1401	rBV2	248933	682128	100.00%	12.256%
34	5.917	1436	1439	1445	rBV3	235	304	0.04%	0.005%
35	5.978	1456	1458	1464	rBV2	234	181	0.03%	0.003%
36	6.017	1466	1470	1472	rBV2	111	86	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU060001.D
 Acq On : 17 Jul 2024 18:05
 Operator : MD/SY
 Sample : P3277-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1ZQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	6.046	1476	1479	1480	rBV	112	68	0.01%	0.001%
38	6.129	1501	1505	1512	rVB2	139	121	0.02%	0.002%
39	6.200	1521	1527	1528	rBV	201	163	0.02%	0.003%
40	6.242	1528	1540	1565	rBV	253883	487785	71.51%	8.765%
41	6.493	1612	1618	1621	rBV2	326	466	0.07%	0.008%
42	6.534	1622	1631	1640	rVB8	2494	4992	0.73%	0.090%
43	6.682	1663	1677	1699	rBV2	162075	318053	46.63%	5.715%
44	6.891	1739	1742	1744	rBV	162	78	0.01%	0.001%
45	6.943	1755	1758	1761	rBV	200	127	0.02%	0.002%
46	7.078	1797	1800	1802	rBV	177	109	0.02%	0.002%
47	7.107	1807	1809	1817	rVB2	374	277	0.04%	0.005%
48	7.203	1830	1839	1845	rBV2	846	1198	0.18%	0.022%
49	7.354	1881	1886	1888	rBV	209	192	0.03%	0.003%
50	7.412	1902	1904	1907	rVB2	136	69	0.01%	0.001%
51	7.435	1908	1911	1914	rVV2	155	91	0.01%	0.002%
52	7.518	1933	1937	1939	rBV2	166	131	0.02%	0.002%
53	7.560	1939	1950	1972	rVV2	80101	141465	20.74%	2.542%
54	7.705	1992	1995	1998	rBV3	332	282	0.04%	0.005%
55	7.737	2003	2005	2008	rBV2	204	140	0.02%	0.003%
56	7.782	2017	2019	2021	rBV2	173	103	0.02%	0.002%
57	7.891	2039	2053	2086	rBV	279608	500486	73.37%	8.993%
58	8.174	2130	2141	2166	rBV	53916	94669	13.88%	1.701%
59	8.296	2177	2179	2182	rVB	307	155	0.02%	0.003%
60	8.325	2182	2188	2193	rBV2	202	250	0.04%	0.004%
61	8.364	2198	2200	2202	rBV	186	112	0.02%	0.002%
62	8.431	2218	2221	2224	rVB2	263	147	0.02%	0.003%
63	8.476	2224	2235	2239	rBV3	758	1210	0.18%	0.022%
64	8.509	2242	2245	2248	rBV	194	137	0.02%	0.002%
65	8.550	2248	2258	2266	rVB4	5754	8273	1.21%	0.149%
66	8.589	2266	2270	2272	rBV2	126	84	0.01%	0.002%
67	8.628	2272	2282	2308	rBV	196778	376441	55.19%	6.764%
68	8.910	2367	2370	2374	rBV3	326	258	0.04%	0.005%
69	9.174	2449	2452	2453	rBV2	116	72	0.01%	0.001%
70	9.283	2483	2486	2490	rBV2	207	189	0.03%	0.003%
71	9.412	2514	2526	2565	rBV	368324	622931	91.32%	11.193%
72	9.611	2585	2588	2590	rBV2	290	147	0.02%	0.003%
73	9.692	2607	2613	2625	rVB4	1388	2415	0.35%	0.043%
74	9.756	2629	2633	2634	rBV	133	90	0.01%	0.002%
75	9.830	2652	2656	2660	rBV	284	295	0.04%	0.005%
76	9.991	2704	2706	2709	rVB2	135	73	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU060001.D
 Acq On : 17 Jul 2024 18:05
 Operator : MD/SY
 Sample : P3277-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1ZQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	10.007	2709	2711	2713	rBV2	139	83	0.01%	0.001%
78	10.158	2756	2758	2760	rBV	126	78	0.01%	0.001%
79	10.309	2803	2805	2807	rBV	109	71	0.01%	0.001%
80	10.589	2890	2892	2894	rBV	141	71	0.01%	0.001%
81	10.750	2930	2942	2962	rBV	263936	427341	62.65%	7.678%
82	10.885	2980	2984	2994	rVB2	1047	1520	0.22%	0.027%
83	11.152	3065	3067	3069	rBV	145	90	0.01%	0.002%
84	11.589	3199	3203	3205	rBV2	220	170	0.02%	0.003%
85	11.624	3211	3214	3216	rBV	152	90	0.01%	0.002%
86	11.692	3232	3235	3237	rBV2	170	111	0.02%	0.002%
87	11.743	3245	3251	3259	rBV5	1657	2502	0.37%	0.045%
88	11.807	3259	3271	3297	rVV	319149	518059	75.95%	9.308%
89	12.068	3344	3352	3364	rBV7	5434	13164	1.93%	0.237%
90	12.187	3378	3389	3413	rVB	282245	467182	68.49%	8.394%
91	12.319	3428	3430	3432	rBV2	318	151	0.02%	0.003%
92	12.489	3480	3483	3487	rVB2	308	224	0.03%	0.004%
93	12.705	3547	3550	3553	rBV	362	212	0.03%	0.004%
94	12.733	3557	3559	3562	rBV	289	193	0.03%	0.003%
95	13.225	3705	3712	3726	rVB6	1465	2378	0.35%	0.043%
96	13.315	3737	3740	3746	rBV2	323	335	0.05%	0.006%
97	13.852	3901	3907	3915	rVB4	2619	3593	0.53%	0.065%
98	14.190	4010	4012	4014	rBV	317	173	0.03%	0.003%
99	14.331	4052	4056	4064	rVB3	2330	2782	0.41%	0.050%
100	14.508	4109	4111	4114	rBV2	330	197	0.03%	0.004%




Sum of corrected areas: 5565449

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU060001.D
Acq On : 17 Jul 2024 18:05
Operator : MD/SY
Sample : P3277-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1ZQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

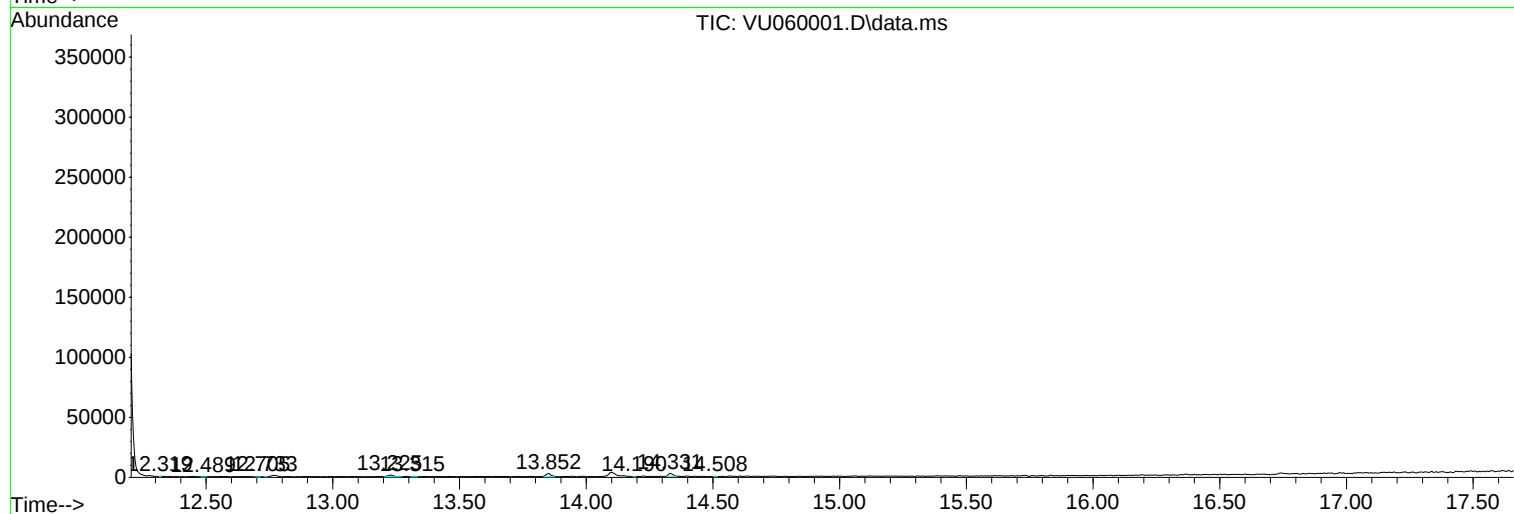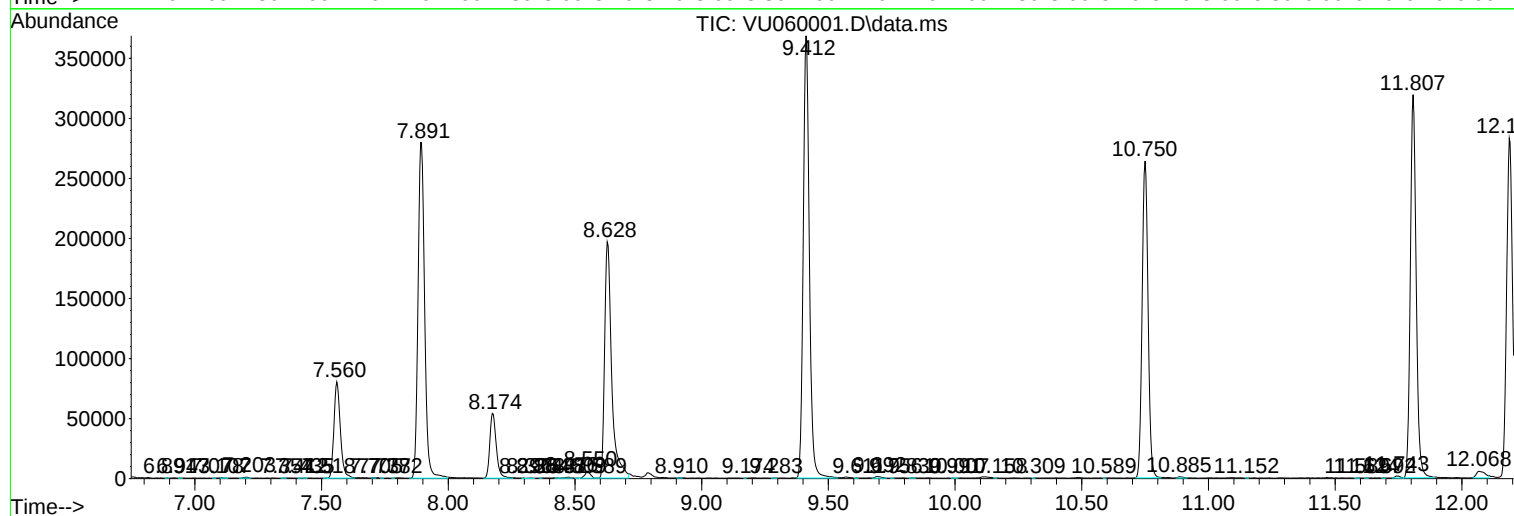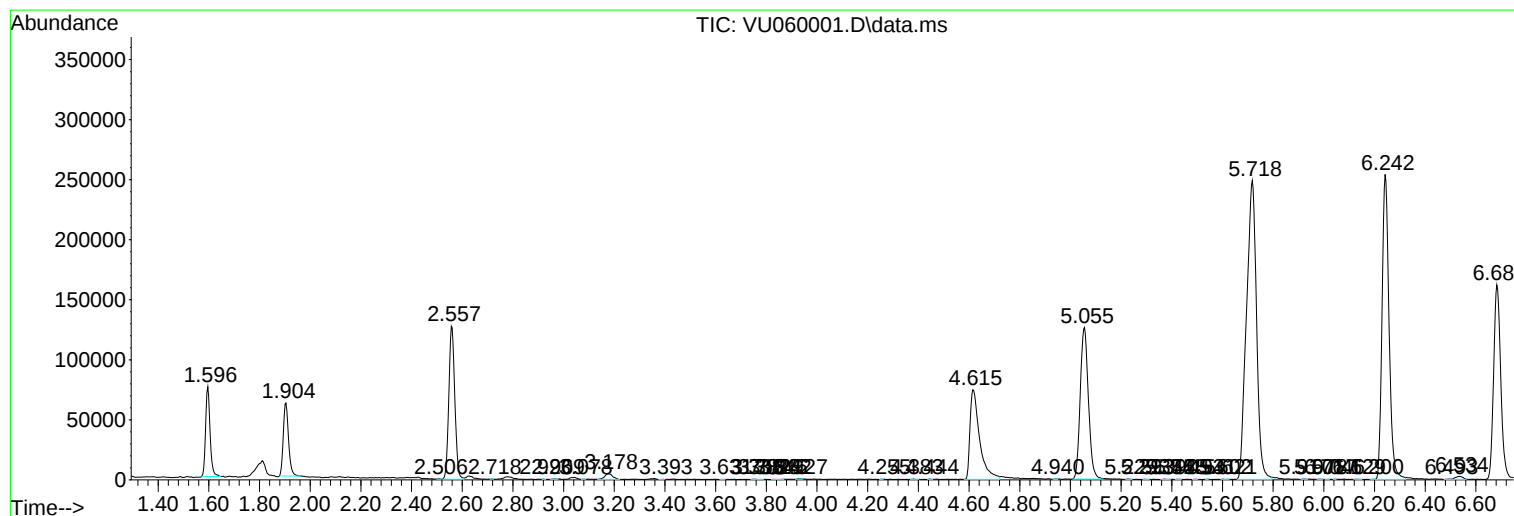

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU060001.D
Acq On : 17 Jul 2024 18:05
Operator : MD/SY
Sample : P3277-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1ZQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU060001.D
Acq On : 17 Jul 2024 18:05
Operator : MD/SY
Sample : P3277-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1ZQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------