

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU060002.D
 Acq On : 17 Jul 2024 18:29
 Operator : MD/SY
 Sample : P3277-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1ZQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU060002.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.515	66	70	74	rBV2	1555	1480	0.22%	0.027%
2	1.596	87	95	111	rBV	75803	93556	13.76%	1.682%
3	1.904	183	191	210	rVB	62441	89540	13.17%	1.609%
4	2.390	340	342	344	rBV2	476	217	0.03%	0.004%
5	2.560	382	395	409	rBV	127357	208850	30.72%	3.754%
6	2.628	410	416	431	rVB3	2400	4543	0.67%	0.082%
7	2.782	457	464	474	rVB3	1142	1822	0.27%	0.033%
8	2.846	481	484	490	rBV3	366	340	0.05%	0.006%
9	2.917	503	506	511	rBV2	157	160	0.02%	0.003%
10	3.039	536	544	545	rBV3	1220	1388	0.20%	0.025%
11	3.181	575	588	600	rBV2	2674	5780	0.85%	0.104%
12	3.345	636	639	650	rVB2	297	379	0.06%	0.007%
13	3.695	745	748	752	rVB	277	188	0.03%	0.003%
14	3.801	777	781	783	rBV	247	196	0.03%	0.004%
15	4.165	888	894	897	rVV	246	293	0.04%	0.005%
16	4.190	899	902	905	rVV2	211	163	0.02%	0.003%
17	4.210	905	908	914	rVB2	172	167	0.02%	0.003%
18	4.296	931	935	936	rBV	269	208	0.03%	0.004%
19	4.451	978	983	988	rVB2	185	188	0.03%	0.003%
20	4.618	1025	1035	1067	rBV	73930	194882	28.66%	3.503%
21	4.830	1097	1101	1104	rBV3	394	328	0.05%	0.006%
22	4.923	1127	1130	1134	rVB2	395	309	0.05%	0.006%
23	5.052	1155	1170	1197	rBV	126940	281282	41.37%	5.056%
24	5.229	1220	1225	1231	rVB3	297	328	0.05%	0.006%
25	5.287	1240	1243	1245	rBV	361	195	0.03%	0.004%
26	5.457	1289	1296	1303	rBV2	209	295	0.04%	0.005%
27	5.509	1305	1312	1315	rVV2	199	218	0.03%	0.004%
28	5.544	1321	1323	1330	rVB2	213	183	0.03%	0.003%
29	5.718	1358	1377	1408	rBV2	247794	679904	100.00%	12.220%
30	5.901	1431	1434	1440	rVB2	190	191	0.03%	0.003%
31	6.242	1527	1540	1560	rBV	252984	490745	72.18%	8.821%
32	6.476	1609	1613	1617	rBV2	415	370	0.05%	0.007%
33	6.534	1623	1631	1640	rVB7	1909	3777	0.56%	0.068%
34	6.682	1663	1677	1707	rBV	161407	318083	46.78%	5.717%
35	6.820	1718	1720	1724	rVB2	379	285	0.04%	0.005%
36	6.856	1729	1731	1734	rBV2	280	179	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU060002.D
 Acq On : 17 Jul 2024 18:29
 Operator : MD/SY
 Sample : P3277-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1ZQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	6.946	1754	1759	1763	rBV2	137	162	0.02%	0.003%
38	7.107	1805	1809	1812	rBV2	174	166	0.02%	0.003%
39	7.181	1829	1832	1834	rBV	306	216	0.03%	0.004%
40	7.283	1861	1864	1870	rVB2	249	224	0.03%	0.004%
41	7.512	1932	1935	1938	rVB2	280	178	0.03%	0.003%
42	7.560	1938	1950	1969	rBV	77665	138523	20.37%	2.490%
43	7.795	2019	2023	2025	rBV2	280	277	0.04%	0.005%
44	7.894	2040	2054	2071	rBV	280630	490004	72.07%	8.807%
45	8.174	2130	2141	2164	rBV	52874	92029	13.54%	1.654%
46	8.309	2180	2183	2189	rVB2	208	213	0.03%	0.004%
47	8.467	2225	2232	2241	rBV2	1131	1711	0.25%	0.031%
48	8.550	2250	2258	2266	rVB5	4063	5872	0.86%	0.106%
49	8.627	2272	2282	2315	rBV2	196892	387553	57.00%	6.966%
50	8.791	2325	2333	2345	rVB5	4016	6670	0.98%	0.120%
51	8.869	2355	2357	2360	rVB	582	297	0.04%	0.005%
52	9.007	2397	2400	2403	rVV2	234	165	0.02%	0.003%
53	9.094	2422	2427	2429	rBV2	181	167	0.02%	0.003%
54	9.209	2458	2463	2466	rBV2	262	300	0.04%	0.005%
55	9.264	2474	2480	2484	rBV2	319	404	0.06%	0.007%
56	9.412	2513	2526	2561	rBV	370881	622081	91.50%	11.181%
57	9.570	2569	2575	2583	rVB4	841	1162	0.17%	0.021%
58	9.605	2583	2586	2588	rBV	252	163	0.02%	0.003%
59	9.621	2588	2591	2596	rVB2	264	241	0.04%	0.004%
60	9.698	2609	2615	2626	rVB3	1317	1932	0.28%	0.035%
61	9.782	2637	2641	2647	rVB2	226	214	0.03%	0.004%
62	9.836	2655	2658	2663	rBV2	275	276	0.04%	0.005%
63	9.904	2675	2679	2683	rBV2	227	242	0.04%	0.004%
64	9.988	2702	2705	2709	rBV2	259	240	0.04%	0.004%
65	10.103	2735	2741	2742	rBV2	503	469	0.07%	0.008%
66	10.222	2774	2778	2788	rVV2	178	329	0.05%	0.006%
67	10.267	2789	2792	2798	rVB2	262	193	0.03%	0.003%
68	10.325	2807	2810	2817	rVB2	266	231	0.03%	0.004%
69	10.479	2855	2858	2862	rVB3	355	301	0.04%	0.005%
70	10.750	2929	2942	2962	rBV	263661	426188	62.68%	7.660%
71	10.888	2977	2985	2994	rVB2	2060	3066	0.45%	0.055%
72	11.094	3046	3049	3055	rVV3	411	437	0.06%	0.008%
73	11.502	3173	3176	3183	rBV2	209	162	0.02%	0.003%
74	11.634	3212	3217	3221	rBV	162	185	0.03%	0.003%
75	11.743	3247	3251	3256	rBV3	947	942	0.14%	0.017%
76	11.807	3259	3271	3292	rBV	315916	515778	75.86%	9.271%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU060002.D
 Acq On : 17 Jul 2024 18:29
 Operator : MD/SY
 Sample : P3277-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1ZQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	11.991	3325	3328	3335	rVB2	372	449	0.07%	0.008%
78	12.071	3345	3353	3368	rBV5	4119	10474	1.54%	0.188%
79	12.187	3376	3389	3412	rBV	278368	460653	67.75%	8.280%
80	12.553	3500	3503	3508	rVB	380	299	0.04%	0.005%
81	12.650	3529	3533	3536	rBV	202	211	0.03%	0.004%
82	12.769	3561	3570	3577	rBV2	1435	2139	0.31%	0.038%
83	12.910	3609	3614	3617	rBV2	550	441	0.06%	0.008%
84	12.949	3623	3626	3631	rVB2	339	285	0.04%	0.005%
85	13.232	3708	3714	3721	rVB3	774	1146	0.17%	0.021%
86	13.775	3880	3883	3887	rBB	304	201	0.03%	0.004%
87	13.849	3901	3906	3907	rBV3	581	509	0.07%	0.009%
88	14.113	3979	3988	3990	rVV2	942	1298	0.19%	0.023%
89	14.328	4047	4055	4056	rBV4	681	739	0.11%	0.013%
90	14.425	4082	4085	4088	rBV2	491	331	0.05%	0.006%
91	14.447	4089	4092	4096	rVB	636	383	0.06%	0.007%
92	14.470	4096	4099	4104	rBV2	238	275	0.04%	0.005%
93	14.643	4148	4153	4159	rBV3	381	482	0.07%	0.009%
94	14.672	4159	4162	4163	rBV	289	177	0.03%	0.003%
95	14.827	4207	4210	4215	rBV2	455	475	0.07%	0.009%
96	15.023	4267	4271	4274	rBV3	452	366	0.05%	0.007%
97	15.277	4348	4350	4352	rBV	431	224	0.03%	0.004%
98	15.473	4407	4411	4414	rVB4	370	348	0.05%	0.006%
99	16.026	4581	4583	4586	rBV3	502	285	0.04%	0.005%
100	16.171	4625	4628	4629	rBV	760	483	0.07%	0.009%




Sum of corrected areas: 5563648

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU060002.D
Acq On : 17 Jul 2024 18:29
Operator : MD/SY
Sample : P3277-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1ZQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

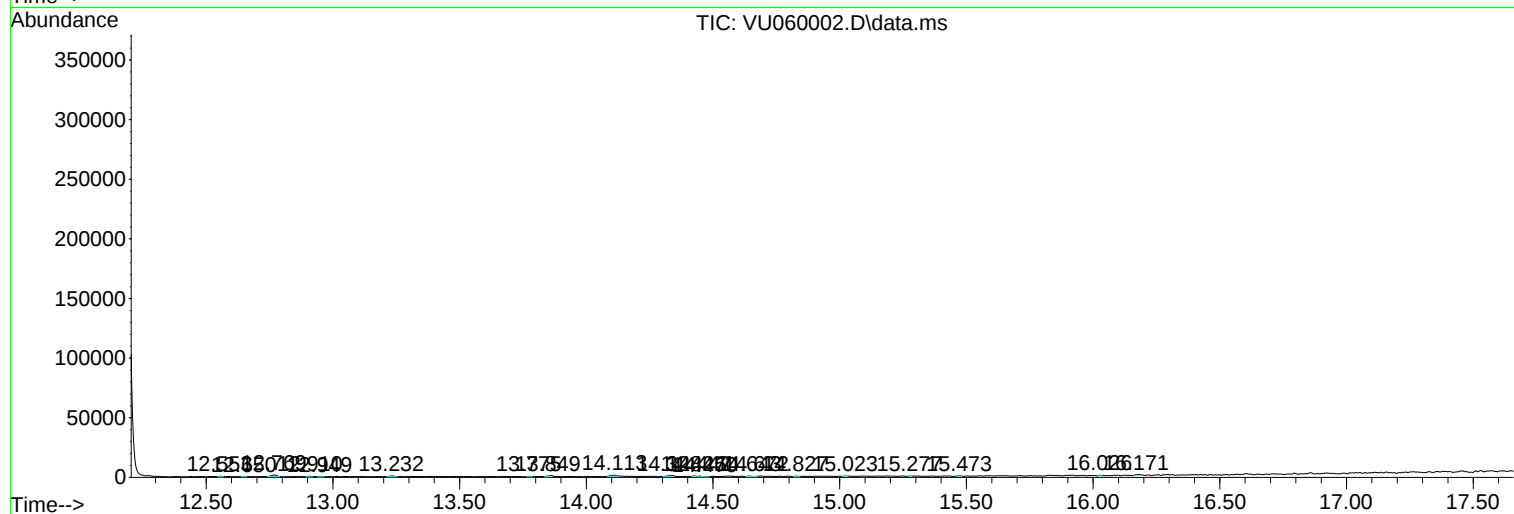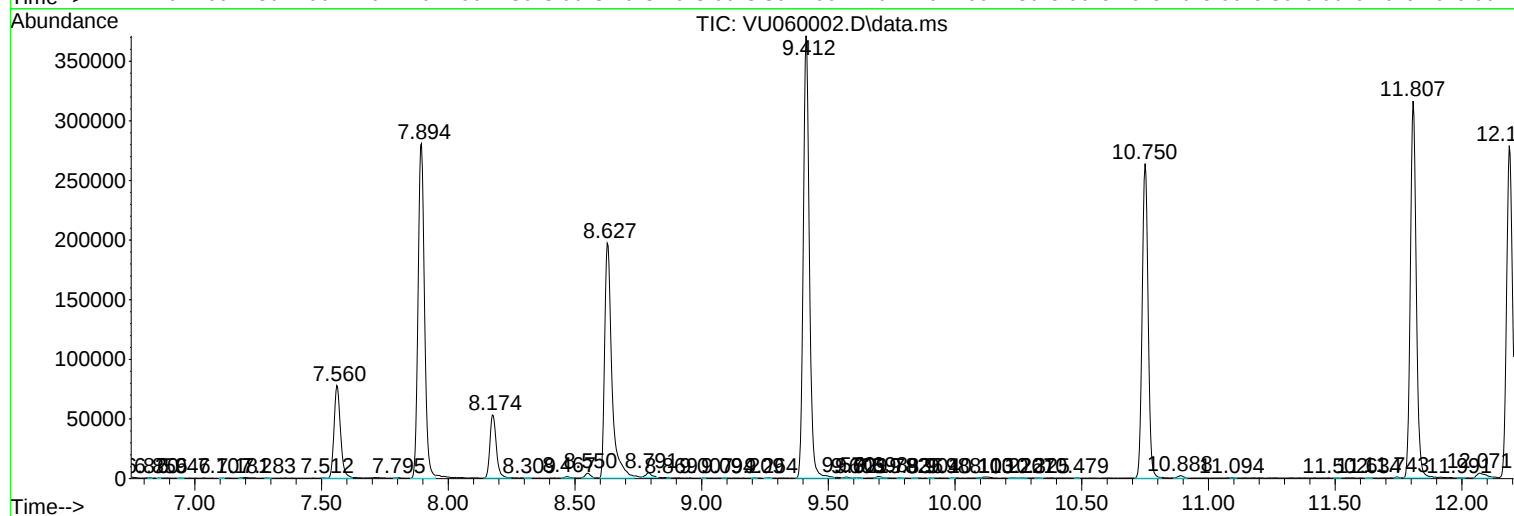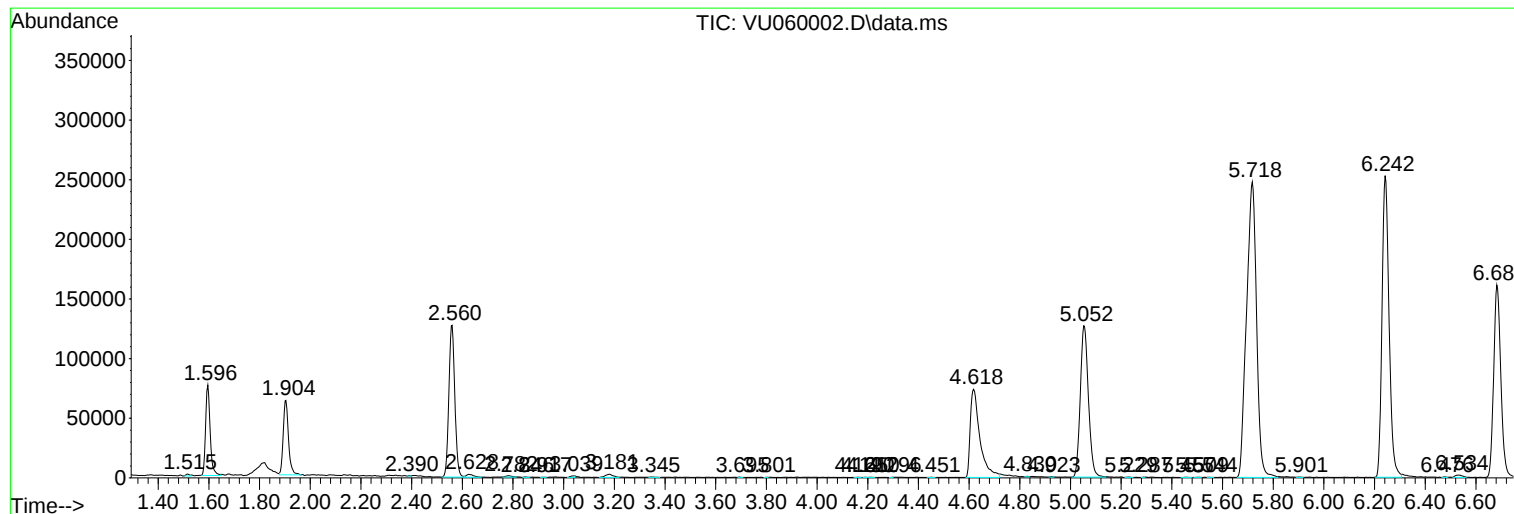

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU060002.D
Acq On : 17 Jul 2024 18:29
Operator : MD/SY
Sample : P3277-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1ZQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU060002.D
Acq On : 17 Jul 2024 18:29
Operator : MD/SY
Sample : P3277-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1ZQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------