

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU060004.D
 Acq On : 17 Jul 2024 19:17
 Operator : MD/SY
 Sample : P3264-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4DA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

Signal : TIC: VU060004.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	113	rVB	72733	87565	13.38%	1.646%
2	1.904	183	191	208	rVB	59854	83234	12.72%	1.565%
3	2.374	335	337	339	rBV	508	196	0.03%	0.004%
4	2.490	369	373	376	rBV	227	150	0.02%	0.003%
5	2.560	383	395	411	rBV	119490	198305	30.31%	3.728%
6	2.715	439	443	445	rBV	278	213	0.03%	0.004%
7	2.782	459	464	467	rBV3	448	445	0.07%	0.008%
8	2.901	497	501	505	rBV2	179	176	0.03%	0.003%
9	2.924	505	508	511	rVB2	211	139	0.02%	0.003%
10	2.946	512	515	521	rBV2	156	163	0.02%	0.003%
11	3.039	537	544	553	rVB5	1108	2058	0.31%	0.039%
12	3.133	565	573	578	rBV5	1469	2459	0.38%	0.046%
13	3.184	579	589	599	rVV3	2949	6412	0.98%	0.121%
14	3.223	599	601	607	rVB2	242	158	0.02%	0.003%
15	3.293	621	623	630	rVB2	167	185	0.03%	0.003%
16	3.338	634	637	640	rVB2	236	147	0.02%	0.003%
17	3.361	640	644	645	rBV	393	297	0.05%	0.006%
18	3.467	674	677	681	rBV2	255	188	0.03%	0.004%
19	3.493	682	685	688	rBV	198	134	0.02%	0.003%
20	3.615	718	723	733	rBV2	278	448	0.07%	0.008%
21	3.940	822	824	829	rVB	245	174	0.03%	0.003%
22	4.081	865	868	869	rBV	256	151	0.02%	0.003%
23	4.097	870	873	876	rVB2	354	254	0.04%	0.005%
24	4.123	876	881	883	rBV2	260	222	0.03%	0.004%
25	4.161	889	893	896	rBV2	420	355	0.05%	0.007%
26	4.277	924	929	934	rBV2	203	286	0.04%	0.005%
27	4.387	960	963	969	rVV2	194	197	0.03%	0.004%
28	4.618	1025	1035	1077	rBV	71280	187806	28.70%	3.530%
29	5.055	1155	1171	1191	rBV	123741	275484	42.10%	5.179%
30	5.216	1219	1221	1225	rVB2	296	157	0.02%	0.003%
31	5.718	1356	1377	1400	rBV2	238737	654301	100.00%	12.300%
32	6.242	1528	1540	1563	rBV	247463	476306	72.80%	8.954%
33	6.528	1622	1629	1639	rBV5	1927	3470	0.53%	0.065%
34	6.682	1663	1677	1699	rBV	152851	301967	46.15%	5.676%
35	6.856	1728	1731	1733	rBV	230	175	0.03%	0.003%
36	6.869	1733	1735	1742	rVB	302	216	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU060004.D
 Acq On : 17 Jul 2024 19:17
 Operator : MD/SY
 Sample : P3264-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4DA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	7.081	1798	1801	1803	rBV2	207	135	0.02%	0.003%
38	7.152	1814	1823	1825	rBV2	243	321	0.05%	0.006%
39	7.168	1825	1828	1833	rVV2	200	150	0.02%	0.003%
40	7.200	1833	1838	1846	rVV2	647	841	0.13%	0.016%
41	7.248	1849	1853	1855	rBV	194	162	0.02%	0.003%
42	7.496	1927	1930	1931	rBV2	316	143	0.02%	0.003%
43	7.560	1938	1950	1968	rBV2	74128	132155	20.20%	2.484%
44	7.702	1990	1994	1996	rBV3	391	314	0.05%	0.006%
45	7.779	2014	2018	2021	rVV2	220	181	0.03%	0.003%
46	7.830	2030	2034	2037	rBV2	180	153	0.02%	0.003%
47	7.891	2041	2053	2074	rBV	267915	473074	72.30%	8.893%
48	8.174	2131	2141	2164	rBV	51035	90319	13.80%	1.698%
49	8.258	2164	2167	2170	rVB2	309	194	0.03%	0.004%
50	8.290	2175	2177	2181	rVB2	363	250	0.04%	0.005%
51	8.464	2224	2231	2242	rVB3	649	1315	0.20%	0.025%
52	8.518	2242	2248	2250	rBV2	199	224	0.03%	0.004%
53	8.550	2250	2258	2266	rVB4	2779	4018	0.61%	0.076%
54	8.628	2271	2282	2313	rBV	182455	361379	55.23%	6.793%
55	8.830	2343	2345	2351	rVB3	372	313	0.05%	0.006%
56	8.923	2371	2374	2376	rVB	274	173	0.03%	0.003%
57	8.991	2392	2395	2397	rVB	310	164	0.03%	0.003%
58	9.049	2411	2413	2416	rVB	266	146	0.02%	0.003%
59	9.068	2416	2419	2421	rBV	207	136	0.02%	0.003%
60	9.206	2460	2462	2467	rVB	198	150	0.02%	0.003%
61	9.242	2467	2473	2476	rBV2	299	367	0.06%	0.007%
62	9.348	2502	2506	2511	rBV2	149	144	0.02%	0.003%
63	9.412	2513	2526	2567	rVV	355760	612254	93.57%	11.509%
64	9.695	2609	2614	2622	rBV3	1106	1553	0.24%	0.029%
65	9.746	2628	2630	2631	rBV	315	130	0.02%	0.002%
66	9.952	2689	2694	2696	rBV	178	175	0.03%	0.003%
67	10.209	2769	2774	2779	rBV	391	434	0.07%	0.008%
68	10.287	2795	2798	2803	rBV2	205	245	0.04%	0.005%
69	10.750	2930	2942	2964	rBV	249899	407907	62.34%	7.668%
70	10.840	2968	2970	2973	rVB2	191	129	0.02%	0.002%
71	10.885	2974	2984	2985	rBV3	1257	1274	0.19%	0.024%
72	11.235	3090	3093	3099	rBV2	274	241	0.04%	0.005%
73	11.389	3139	3141	3147	rBV2	218	167	0.03%	0.003%
74	11.418	3147	3150	3153	rVB	306	204	0.03%	0.004%
75	11.454	3154	3161	3163	rBV2	234	253	0.04%	0.005%
76	11.470	3163	3166	3173	rBV	262	247	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
 Data File : VU060004.D
 Acq On : 17 Jul 2024 19:17
 Operator : MD/SY
 Sample : P3264-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4DA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	11.643	3216	3220	3223	rBV	266	195	0.03%	0.004%
78	11.750	3249	3253	3256	rBV2	649	494	0.08%	0.009%
79	11.807	3259	3271	3290	rBV	308598	497091	75.97%	9.344%
80	12.071	3349	3353	3354	rBV3	544	335	0.05%	0.006%
81	12.187	3377	3389	3415	rBV	260724	436840	66.76%	8.212%
82	12.312	3426	3428	3432	rVB3	609	424	0.06%	0.008%
83	12.766	3562	3569	3577	rVB2	1065	1597	0.24%	0.030%
84	12.820	3583	3586	3590	rBV	322	213	0.03%	0.004%
85	12.901	3607	3611	3613	rBV3	864	645	0.10%	0.012%
86	13.049	3654	3657	3660	rBV	287	205	0.03%	0.004%
87	13.106	3672	3675	3680	rBV2	216	235	0.04%	0.004%
88	13.229	3710	3713	3719	rVB2	442	331	0.05%	0.006%
89	13.360	3750	3754	3755	rBV2	266	188	0.03%	0.004%
90	13.862	3907	3910	3913	rBV2	433	266	0.04%	0.005%
91	14.116	3985	3989	3992	rBV	374	418	0.06%	0.008%
92	14.213	4016	4019	4021	rBV	344	245	0.04%	0.005%
93	14.283	4039	4041	4046	rVB	366	237	0.04%	0.004%
94	14.463	4094	4097	4101	rBV2	369	230	0.04%	0.004%
95	15.171	4308	4317	4320	rBV2	536	804	0.12%	0.015%
96	15.685	4474	4477	4481	rBV2	512	329	0.05%	0.006%
97	15.814	4514	4517	4521	rBV2	645	526	0.08%	0.010%
98	15.836	4521	4524	4526	rBV2	386	267	0.04%	0.005%
99	15.868	4532	4534	4537	rBV3	476	291	0.04%	0.005%
100	16.319	4671	4674	4677	rBV2	867	527	0.08%	0.010%




Sum of corrected areas: 5319660

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU060004.D
Acq On : 17 Jul 2024 19:17
Operator : MD/SY
Sample : P3264-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4DA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

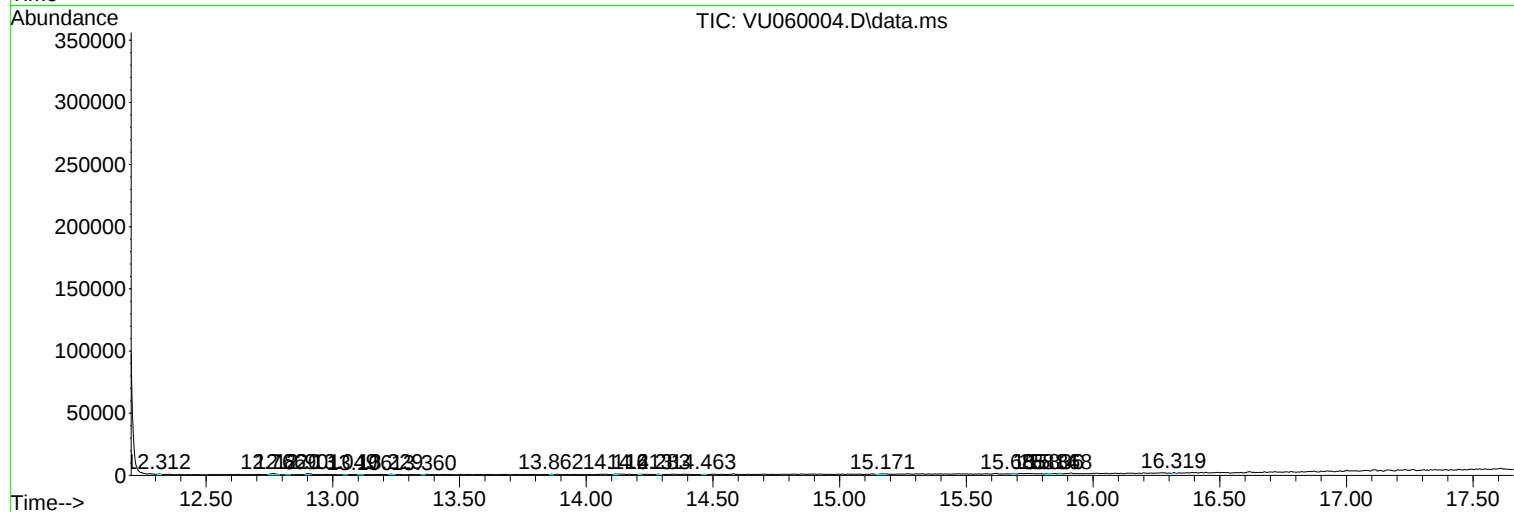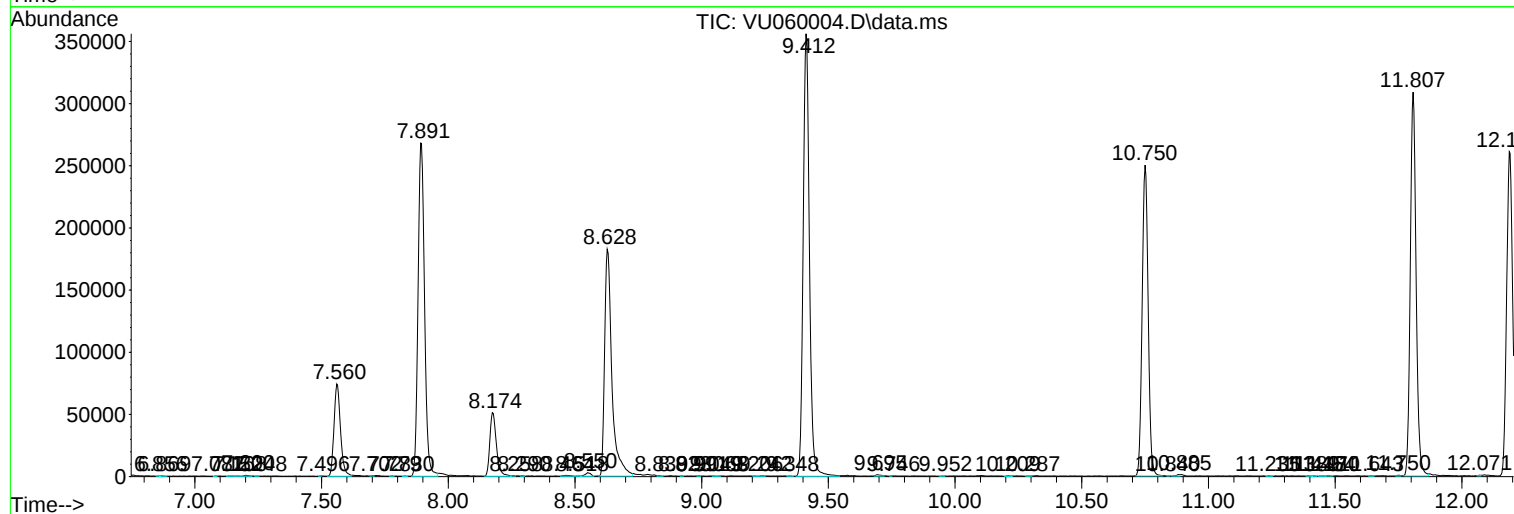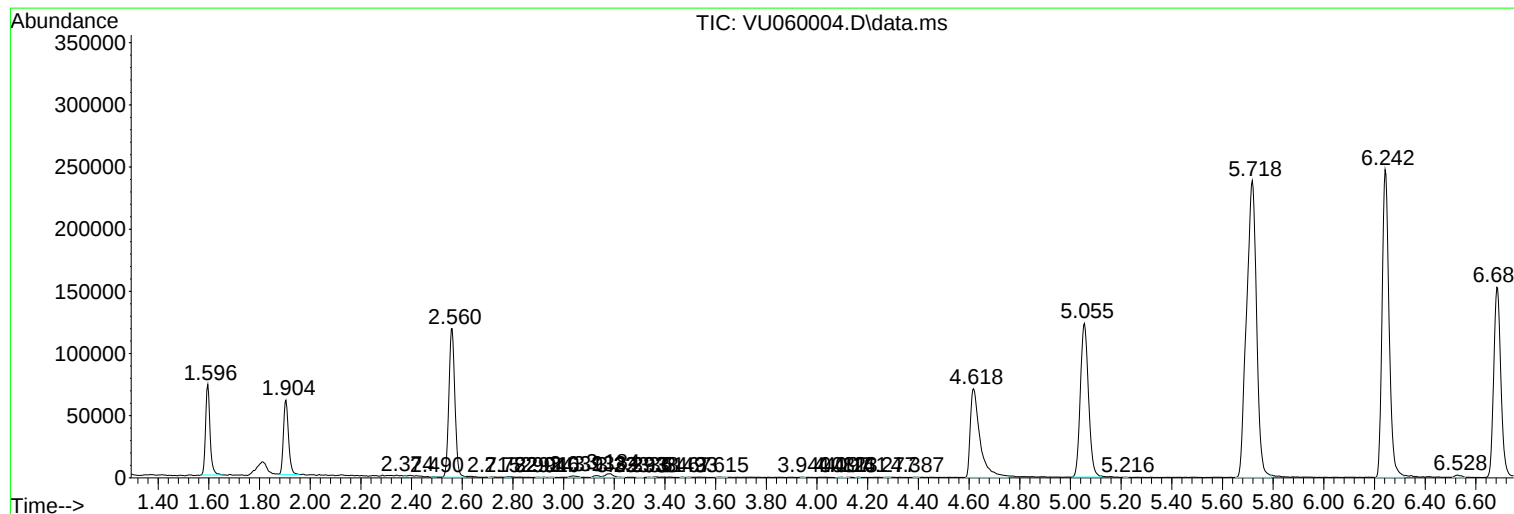

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU060004.D
Acq On : 17 Jul 2024 19:17
Operator : MD/SY
Sample : P3264-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4DA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU060004.D
Acq On : 17 Jul 2024 19:17
Operator : MD/SY
Sample : P3264-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4DA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------