
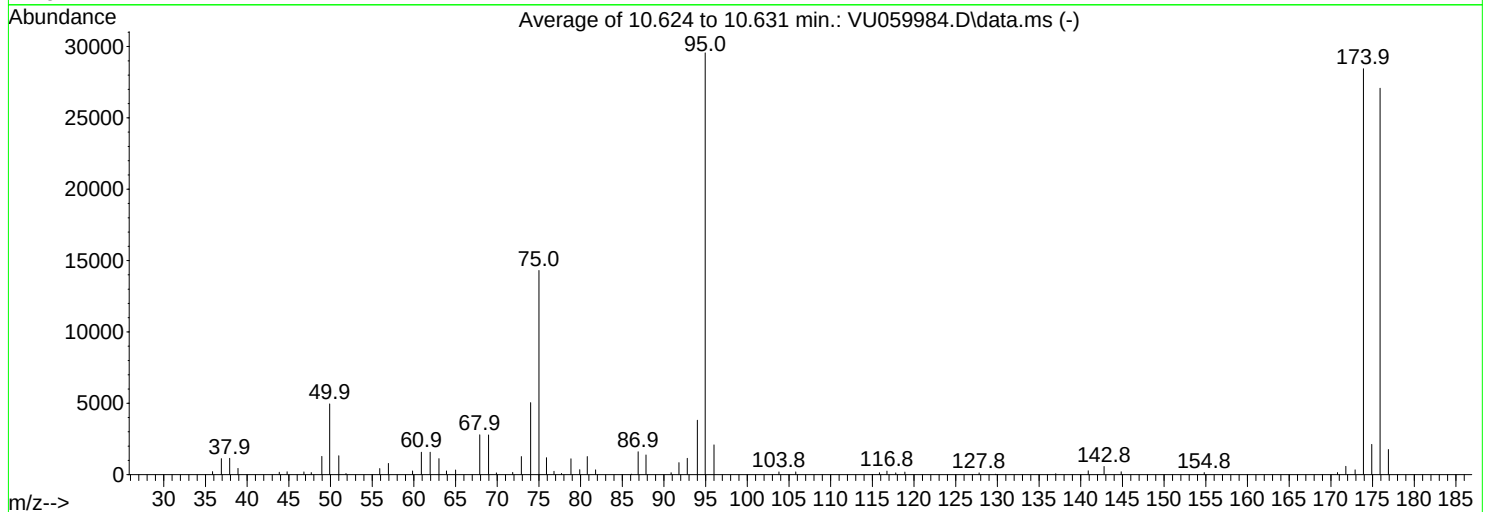


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071724\
Data File : VU059984.D
Acq On : 17 Jul 2024 09:52
Operator : MD/SY
Sample : BFB073
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB073

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Title : VOC Analysis
Last Update : Thu Jul 18 02:31:59 2024

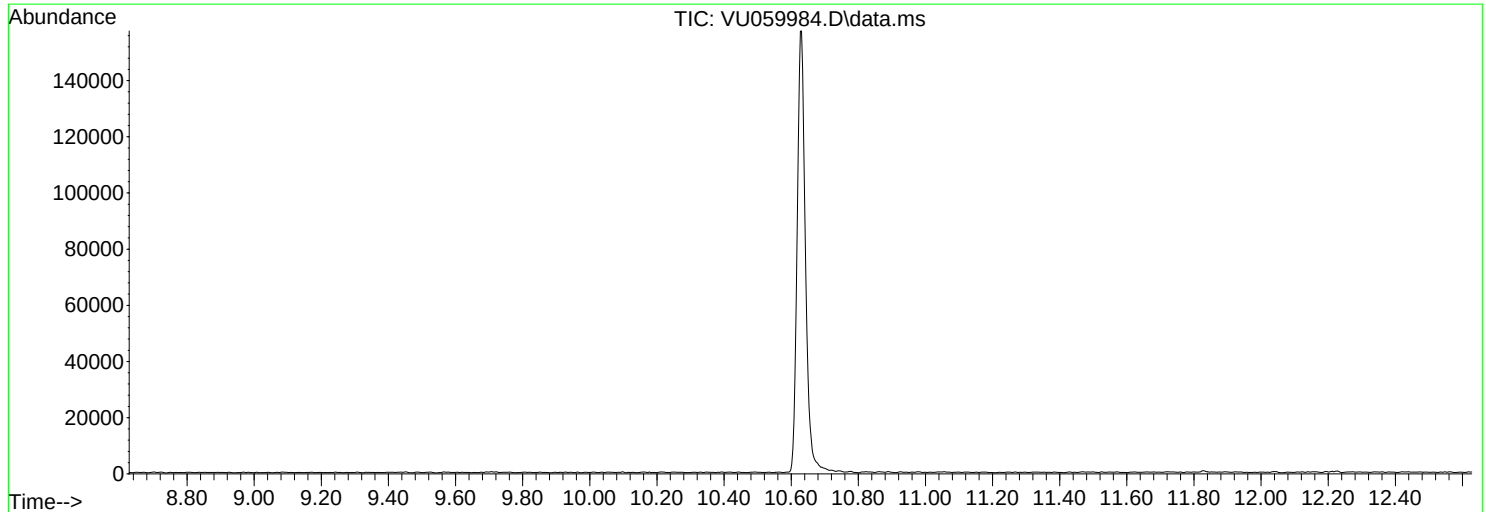

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	4961	PASS
75	95	30	80	48.4	14305	PASS
95	95	100	100	100.0	29557	PASS
96	95	5	9	7.0	2081	PASS
173	174	0.00	2	1.2	340	PASS
174	95	50	120	96.2	28440	PASS
175	174	5	9	7.5	2120	PASS
176	174	95	101	95.2	27072	PASS
177	176	5	9	6.5	1756	PASS

m/z	Abundance
39.80	310.0
43.90	331.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

m/z	Abundance
35.90	199.0
36.90	1205.0
37.90	1058.0
38.90	377.0
39.90	211.0
43.90	563.0
44.80	151.0
46.80	178.0
47.70	136.0
49.00	1149.0
49.90	4807.0
51.00	1285.0
51.80	119.0
55.90	375.0
56.90	844.0
59.80	245.0
60.90	1564.0
62.00	1414.0
63.00	1031.0
63.90	266.0
65.00	273.0
67.90	2606.0
68.90	2766.0
69.90	126.0
71.90	172.0
72.90	1221.0
74.00	4546.0
75.00	13774.0
75.90	1160.0
76.80	246.0
78.80	1119.0
79.90	297.0
80.80	1189.0
81.80	362.0
86.90	1438.0
87.90	1331.0
90.80	111.0
91.80	933.0
92.80	1051.0
94.00	3554.0
94.90	27992.0
96.00	2011.0
103.80	177.0
105.90	206.0
115.90	103.0
116.70	211.0
117.80	111.0
118.90	231.0
127.80	125.0
137.00	106.0
140.90	237.0
142.80	512.0
144.80	185.0
154.80	155.0
170.80	159.0
171.80	461.0
172.90	302.0
173.90	25904.0
174.90	2008.0
175.90	24672.0
176.90	1628.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

m/z	Abundance
35.90	238.0
36.90	1134.0
37.90	1196.0
38.90	416.0
39.90	229.0
43.90	491.0
44.80	218.0
46.80	208.0
47.70	151.0
48.90	1306.0
49.90	5072.0
51.00	1341.0
51.90	114.0
55.90	452.0
57.00	816.0
59.90	249.0
60.90	1634.0
62.00	1661.0
63.00	1170.0
63.90	254.0
65.00	325.0
67.90	2842.0
69.00	2886.0
69.90	116.0
71.90	166.0
72.90	1291.0
74.00	5201.0
75.00	14729.0
75.90	1249.0
76.80	244.0
77.70	121.0
78.80	1162.0
79.90	374.0
80.80	1319.0
81.80	360.0
86.90	1701.0
87.90	1393.0
90.80	149.0
91.80	872.0
92.80	1155.0
94.00	4021.0
94.90	30368.0
96.00	2153.0
103.80	209.0
105.80	184.0
115.80	122.0
116.80	256.0
117.80	128.0
118.90	174.0
127.80	131.0
137.00	101.0
140.90	285.0
142.80	584.0
144.80	213.0
154.80	172.0
170.80	158.0
171.80	596.0
172.90	333.0
173.90	29344.0
174.90	2210.0
175.90	27984.0
176.90	1823.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

m/z	Abundance
35.80	208.0
36.90	1017.0
37.90	1172.0
38.90	511.0
40.00	252.0
43.80	446.0
44.80	242.0
46.80	201.0
47.70	139.0
48.90	1391.0
49.90	5004.0
51.00	1356.0
55.90	461.0
56.90	696.0
59.90	290.0
60.90	1497.0
61.90	1624.0
63.00	1161.0
63.90	238.0
65.00	379.0
67.90	2942.0
69.00	2698.0
69.90	115.0
71.80	139.0
72.90	1291.0
74.00	5376.0
75.00	14411.0
75.90	1157.0
76.80	203.0
77.70	130.0
78.90	1039.0
79.90	369.0
80.80	1296.0
81.80	301.0
86.10	104.0
86.90	1678.0
87.80	1407.0
90.90	148.0
91.80	719.0
92.80	1219.0
94.00	3880.0
95.00	30312.0
96.00	2078.0
103.80	193.0
105.70	171.0
115.80	167.0
116.80	285.0
117.80	132.0
118.90	139.0
127.80	127.0
129.80	105.0
140.90	275.0
142.80	629.0
144.90	202.0
154.80	120.0
170.80	105.0
171.80	703.0
172.90	384.0
173.90	30072.0
174.90	2141.0
175.90	28560.0
176.90	1816.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073