

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063520.D
 Acq On : 17 Jul 2025 11:31
 Operator : MD/SY
 Sample : VU0717WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0717WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.030	534	541	544	rBV4	1886	2561	5.57%	1.672%
2	6.100	1483	1496	1517	rBV	22687	45210	98.36%	29.525%
3	7.898	2050	2055	2059	rBV2	554	526	1.14%	0.344%
4	9.422	2517	2529	2533	rBV4	1134	1548	3.37%	1.011%
5	10.631	2895	2905	2926	rBV	22362	39105	85.08%	25.538%
6	11.749	3246	3253	3259	rVB3	553	671	1.46%	0.438%
7	11.814	3263	3273	3289	rVB4	4622	8962	19.50%	5.853%
8	12.190	3380	3390	3406	rBV	26202	45964	100.00%	30.017%
9	13.856	3898	3908	3913	rBV3	1217	1830	3.98%	1.195%
10	14.097	3976	3983	3999	rBV4	1821	4007	8.72%	2.617%
11	14.328	4048	4055	4066	rBV4	1462	2209	4.81%	1.443%
12	17.392	5005	5008	5010	rVB2	944	534	1.16%	0.349%




Sum of corrected areas: 153127

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063520.D
Acq On : 17 Jul 2025 11:31
Operator : MD/SY
Sample : VU0717WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0717WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

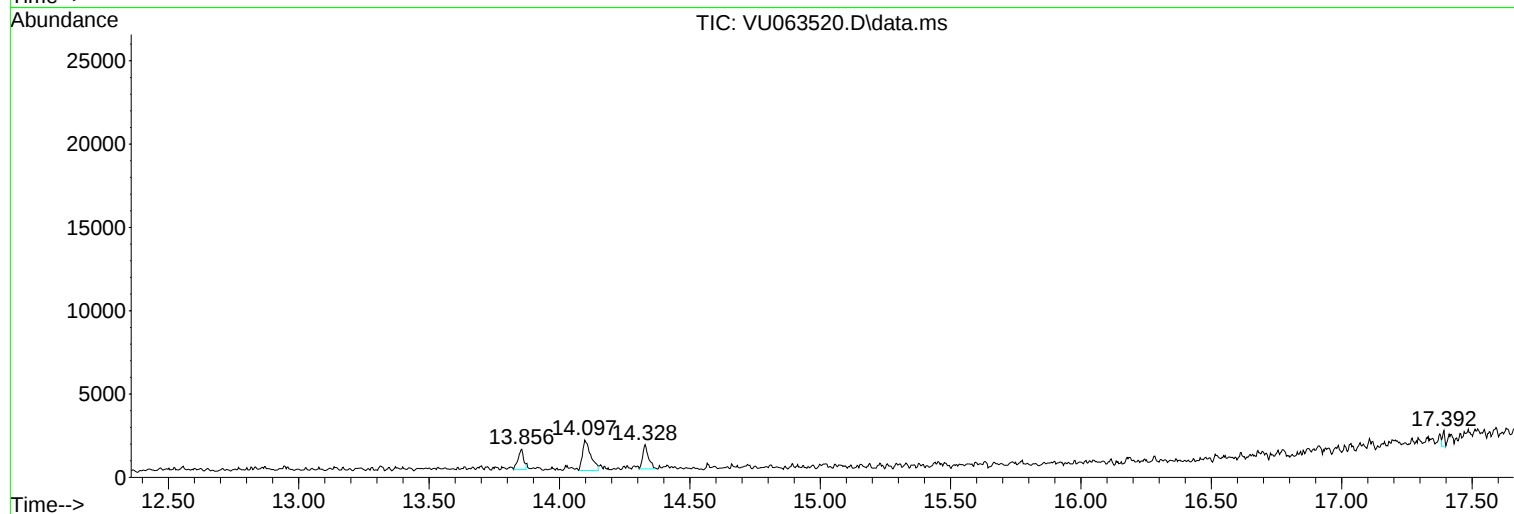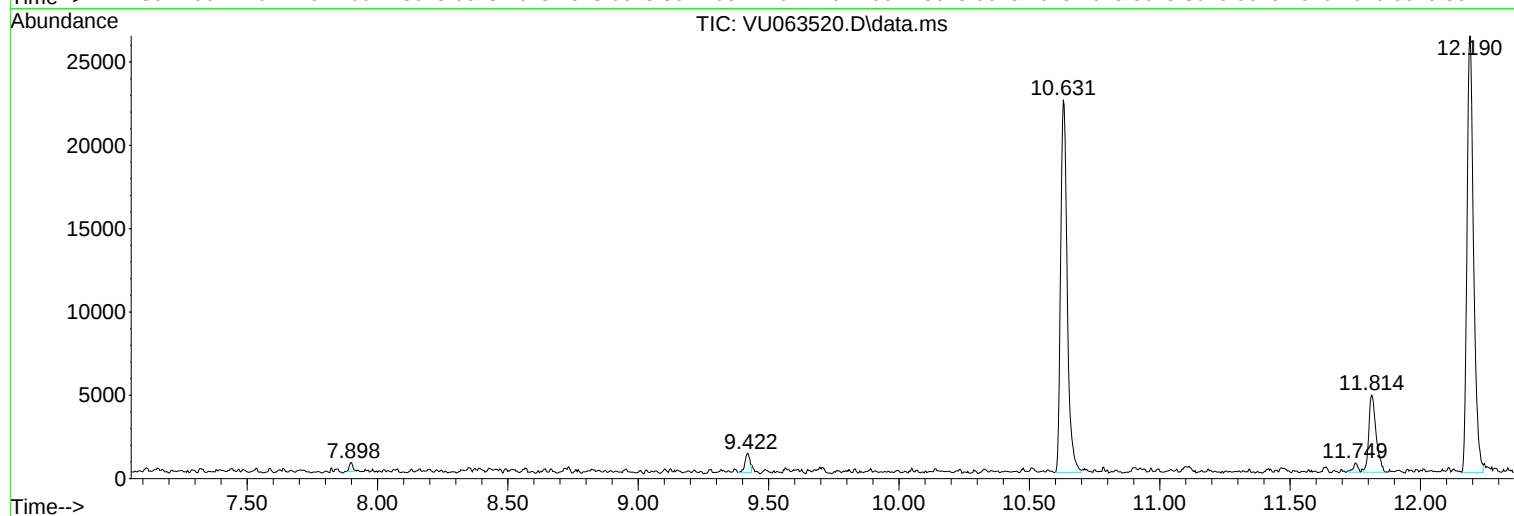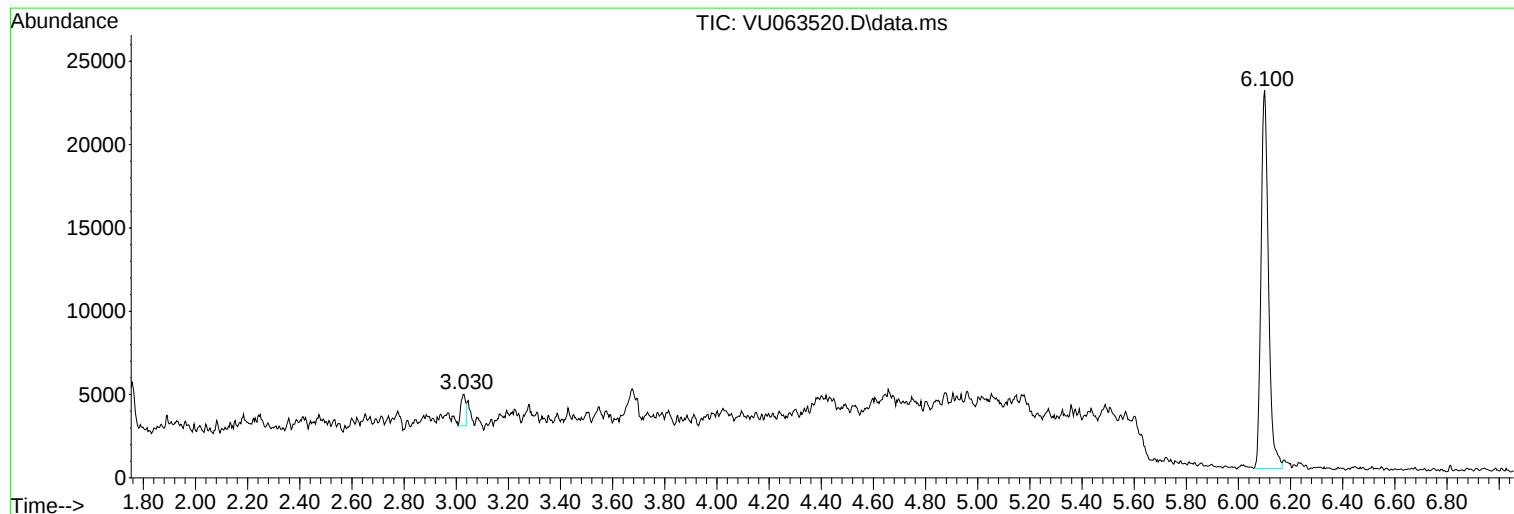

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063520.D
Acq On : 17 Jul 2025 11:31
Operator : MD/SY
Sample : VU0717WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0717WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063520.D
Acq On : 17 Jul 2025 11:31
Operator : MD/SY
Sample : VU0717WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0717WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------