

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063523.D
Acq On : 17 Jul 2025 14:16
Operator : MD/SY
Sample : Q2552-09
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-THM-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.634	408	418	429	rBV	10062	17430	1.91%	0.858%
2	5.071	1160	1176	1196	rBV	91496	205570	22.47%	10.115%
3	6.097	1483	1495	1515	rBV	20840	43686	4.78%	2.149%
4	7.097	1791	1806	1842	rBV	483502	914786	100.00%	45.010%
5	8.801	2322	2336	2369	rBV	380821	666428	72.85%	32.790%
6	10.283	2786	2797	2816	rBV	60658	104419	11.41%	5.138%
7	10.630	2896	2905	2925	rVB2	20460	34715	3.79%	1.708%
8	12.190	3380	3390	3408	rBV2	25770	45356	4.96%	2.232%




Sum of corrected areas: 2032390

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063523.D
Acq On : 17 Jul 2025 14:16
Operator : MD/SY
Sample : Q2552-09
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-THM-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

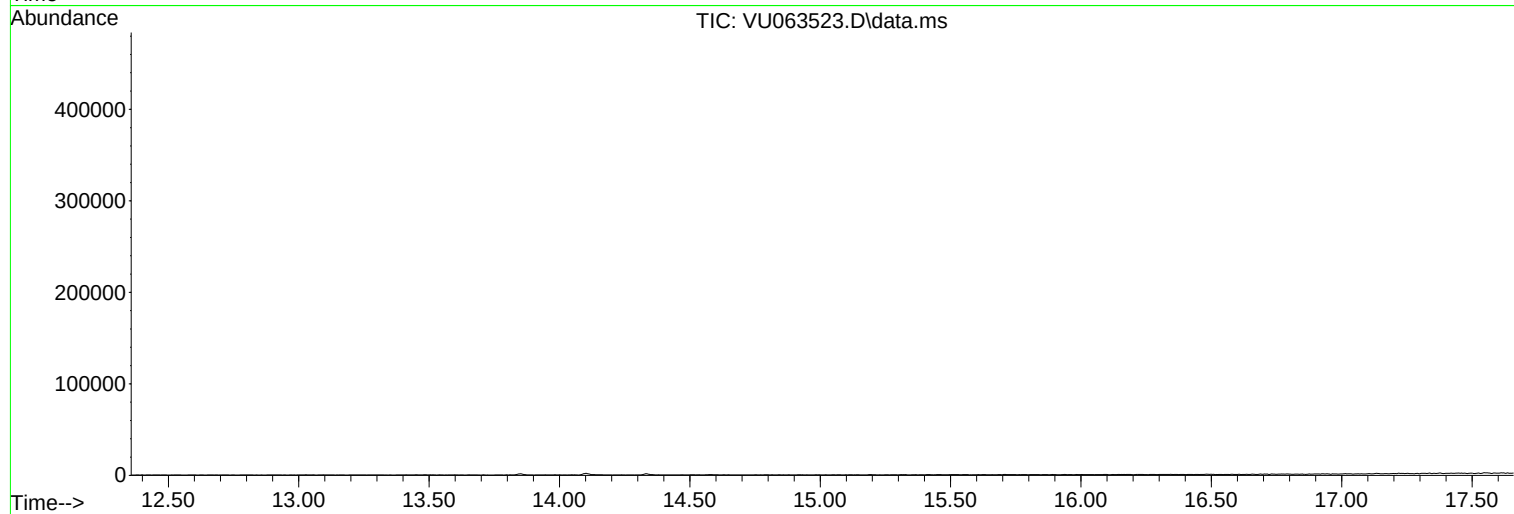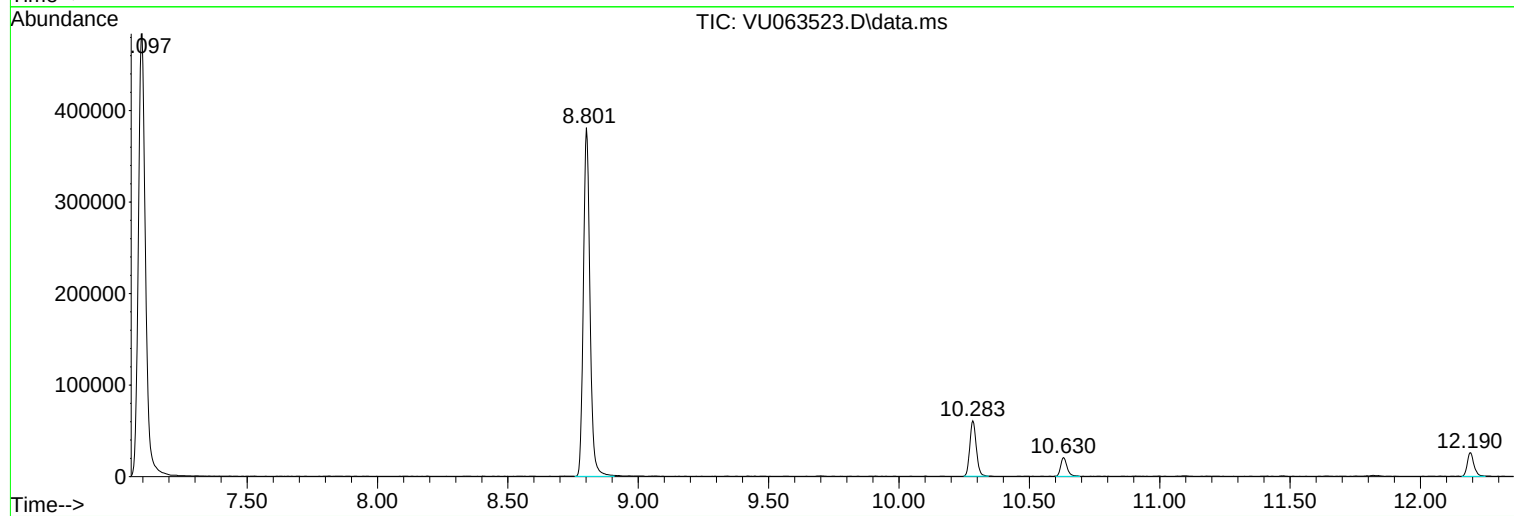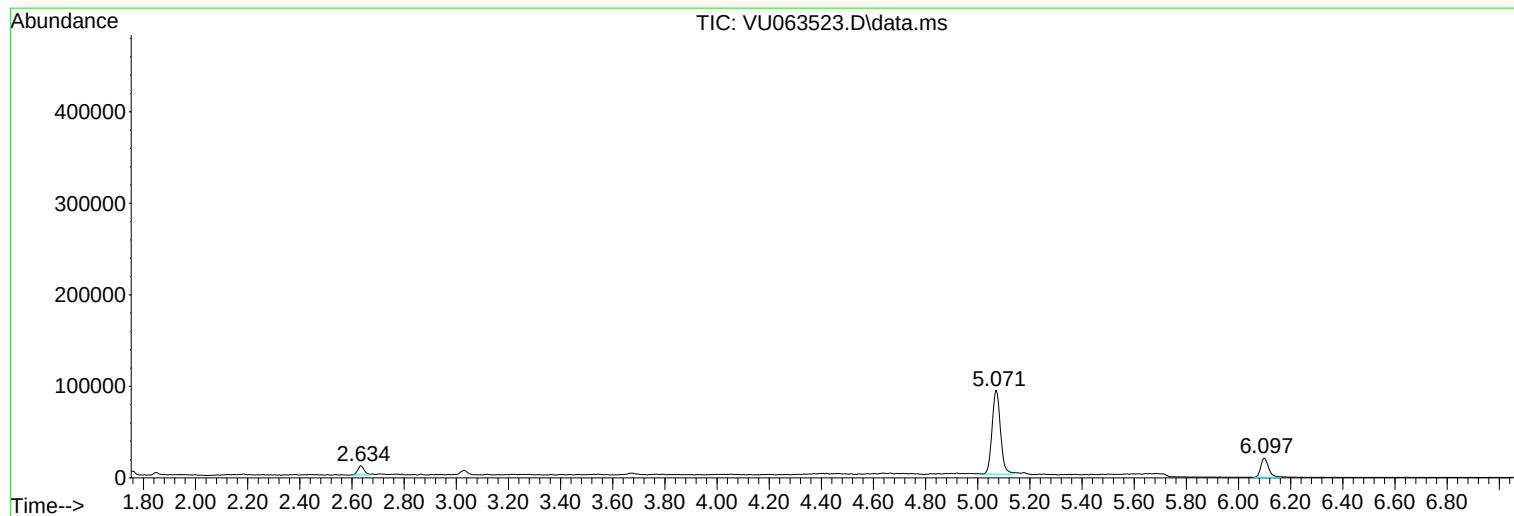

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063523.D
Acq On : 17 Jul 2025 14:16
Operator : MD/SY
Sample : Q2552-09
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-THM-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063523.D
Acq On : 17 Jul 2025 14:16
Operator : MD/SY
Sample : Q2552-09
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-THM-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------