

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063529.D
 Acq On : 17 Jul 2025 17:20
 Operator : MD/SY
 Sample : Q2552-07
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-RVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063529.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.567	386	397	411	rBV	146606	236318	21.95%	2.332%
2	3.030	528	541	566	rVB	195094	361390	33.56%	3.566%
3	3.332	621	635	664	rBV	278985	566636	52.62%	5.591%
4	4.647	1029	1044	1062	rBV	67342	155255	14.42%	1.532%
5	5.293	1229	1245	1275	rBV	254130	575806	53.47%	5.681%
6	5.496	1296	1308	1324	rBV	28000	59758	5.55%	0.590%
7	5.753	1373	1388	1430	rVB2	380193	1076821	100.00%	10.625%
8	6.097	1483	1495	1510	rBV	19339	39646	3.68%	0.391%
9	6.525	1615	1628	1661	rBV	212787	440735	40.93%	4.349%
10	6.779	1693	1707	1739	rBV	216083	432922	40.20%	4.272%
11	7.959	2063	2074	2109	rBV	65379	129509	12.03%	1.278%
12	8.393	2196	2209	2242	rBV	184113	335696	31.17%	3.312%
13	8.541	2242	2255	2287	rBV	340432	642108	59.63%	6.336%
14	9.438	2522	2534	2561	rBV	479762	879538	81.68%	8.678%
15	9.560	2561	2572	2599	rVV	599167	1036672	96.27%	10.229%
16	9.685	2599	2611	2657	rVB	464348	845811	78.55%	8.345%
17	10.094	2722	2738	2775	rBV	509817	936607	86.98%	9.241%
18	10.627	2895	2904	2922	rVB	21206	35575	3.30%	0.351%
19	11.830	3261	3278	3308	rBV	186078	313191	29.08%	3.090%
20	12.203	3377	3394	3416	rBV3	175506	330567	30.70%	3.262%
21	13.833	3888	3901	3923	rBV	421982	704475	65.42%	6.951%




Sum of corrected areas: 10135036

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063529.D
Acq On : 17 Jul 2025 17:20
Operator : MD/SY
Sample : Q2552-07
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

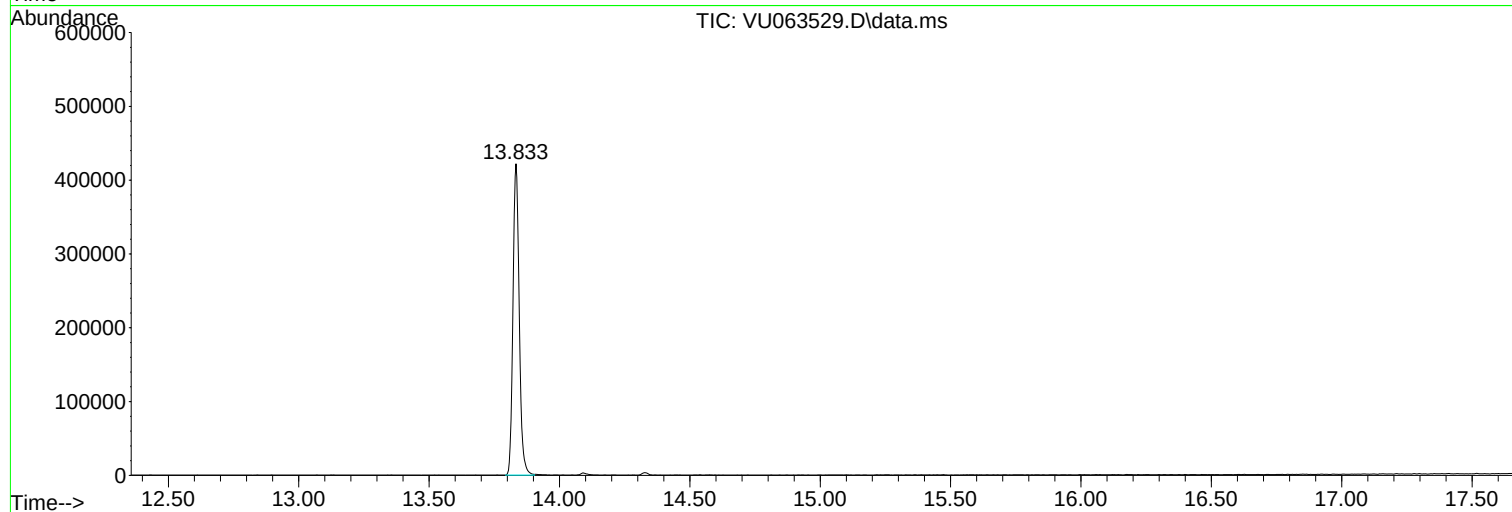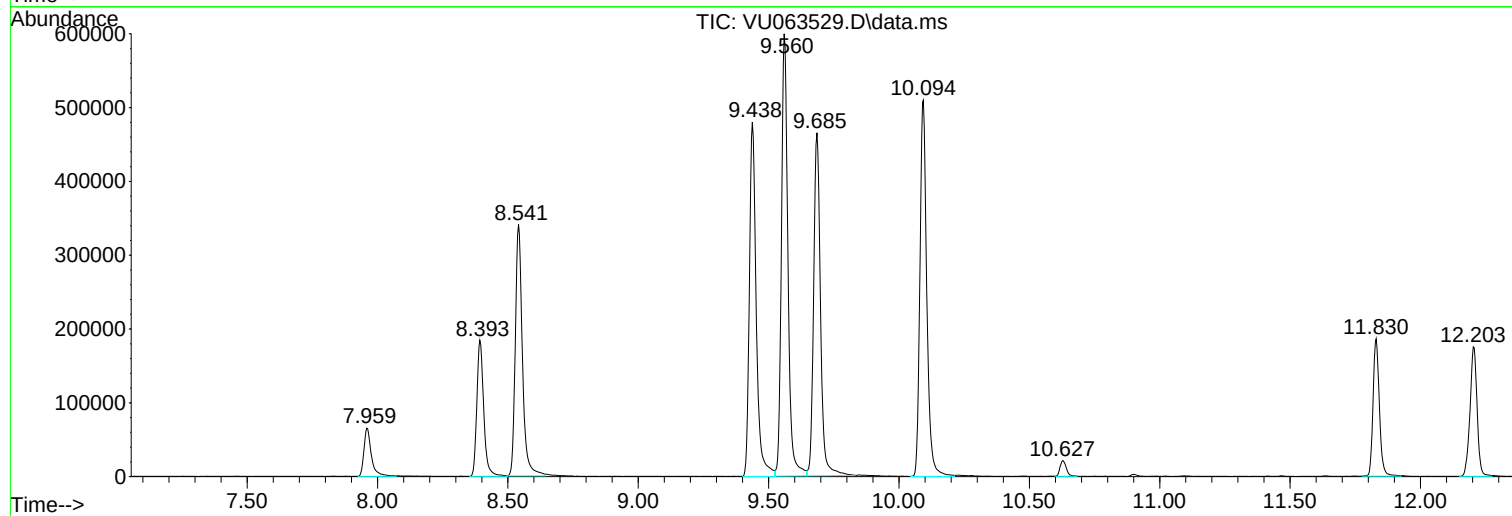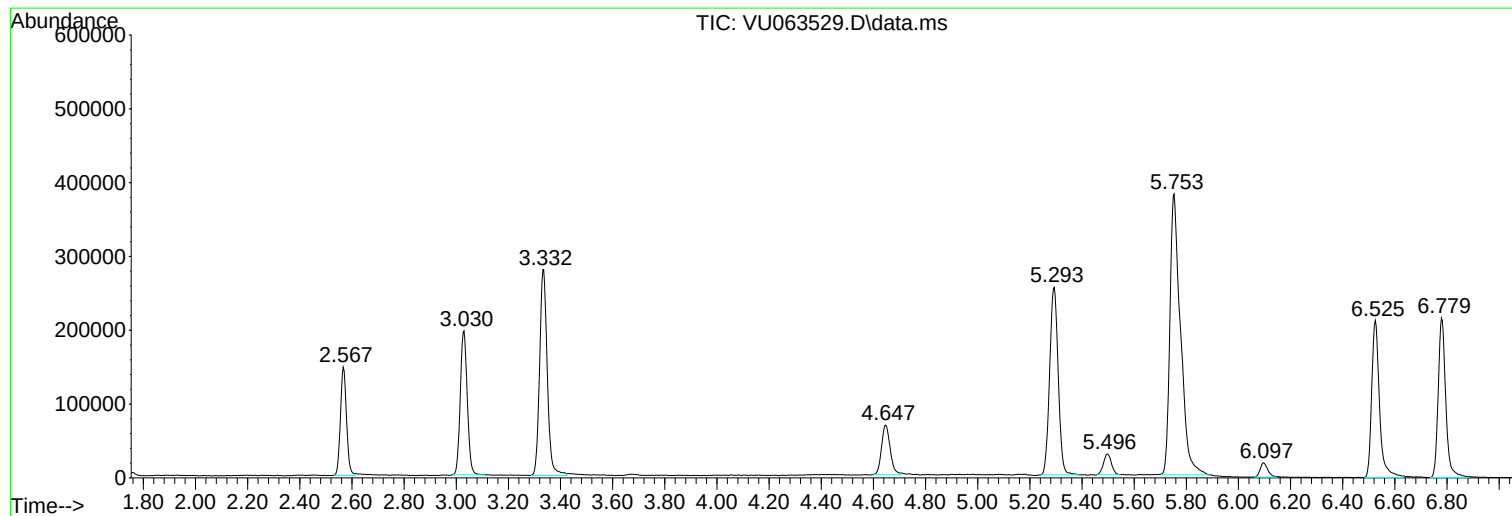

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063529.D
Acq On : 17 Jul 2025 17:20
Operator : MD/SY
Sample : Q2552-07
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063529.D
Acq On : 17 Jul 2025 17:20
Operator : MD/SY
Sample : Q2552-07
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------