


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071818\
 Data File : VU025484.D
 Acq On : 18 Jul 2018 09:03
 Operator : MD/SY
 Sample : BFB44
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
 Title : VOC Analysis
 Last Update : Thu Jul 19 01:07:14 2018

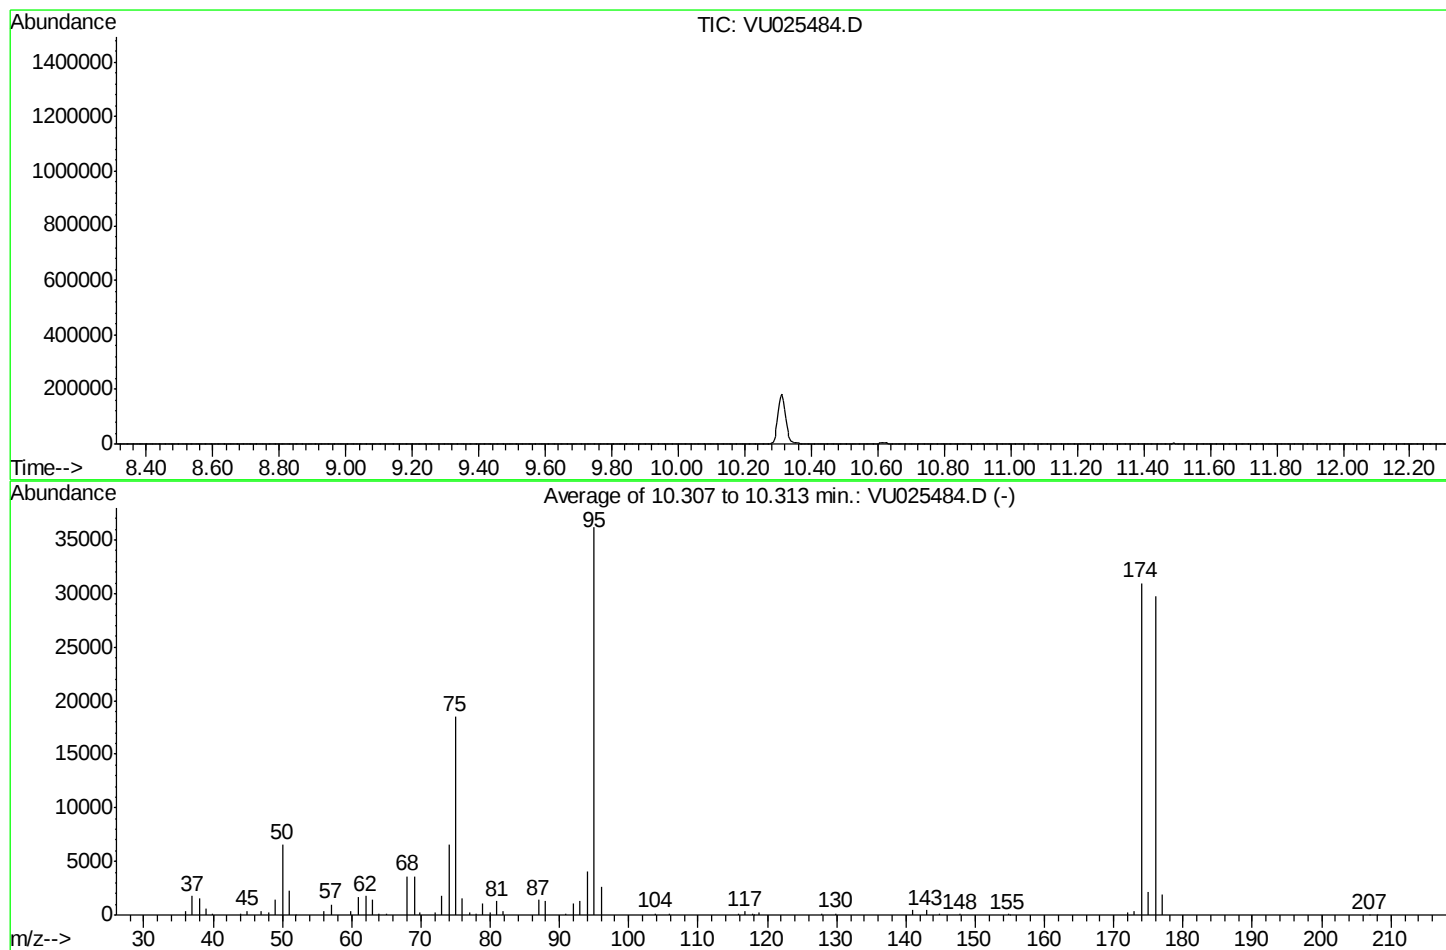

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	6533	PASS
75	95	30	80	51.1	18498	PASS
95	95	100	100	100.0	36178	PASS
96	95	5	9	7.4	2690	PASS
173	174	0.00	2	1.3	401	PASS
174	95	50	120	85.7	30997	PASS
175	174	5	9	7.1	2203	PASS
176	174	95	101	95.9	29714	PASS
177	176	5	9	6.6	1975	PASS

Scan 3011 (10.271 min): VU025484.D
BFB44

m/z	Abundance
43.90	379.0
207.00	600.0
208.00	128.0

m/z	Abundance
36.00	422.0
37.00	1696.0
38.00	1447.0
39.00	618.0
40.00	143.0
44.00	543.0
44.90	343.0
47.00	297.0
47.90	239.0
49.00	1425.0
50.00	6454.0
51.00	2446.0
56.10	418.0
57.00	925.0
59.90	311.0
61.00	1598.0
62.00	1835.0
63.10	1255.0
65.10	103.0
68.00	3515.0
69.00	3794.0
69.90	242.0
72.00	230.0
73.00	1675.0
74.00	6221.0
75.00	18584.0
76.00	1598.0
76.90	263.0
78.00	163.0
78.90	1123.0
80.00	314.0
80.90	1249.0
81.90	283.0
87.00	1414.0
88.00	1292.0
90.90	134.0
91.90	1109.0
93.00	1186.0
94.00	4195.0
95.00	35584.0
96.00	2598.0
103.90	183.0
105.90	142.0
115.80	158.0
116.80	340.0
117.80	143.0
118.10	108.0
118.80	214.0
127.90	146.0
129.90	159.0
141.00	446.0
142.90	433.0
144.90	128.0
154.70	114.0
172.00	214.0
173.00	374.0
174.00	28864.0
174.90	2066.0
176.00	28368.0
176.90	1798.0
207.00	714.0
208.00	102.0

m/z	Abundance
36.10	399.0
37.00	1814.0
38.00	1514.0
39.00	609.0
40.00	141.0
44.00	540.0
44.90	389.0
47.00	342.0
48.00	255.0
49.00	1552.0
50.00	6708.0
51.00	2421.0
56.10	380.0
57.00	989.0
59.90	346.0
61.00	1723.0
62.00	1799.0
63.10	1422.0
63.90	113.0
65.10	128.0
68.00	3763.0
69.00	3704.0
69.90	247.0
72.00	211.0
73.00	1789.0
74.00	6752.0
75.00	19048.0
76.00	1522.0
76.90	247.0
77.90	141.0
78.90	1155.0
79.90	302.0
80.90	1318.0
81.90	355.0
87.00	1477.0
88.00	1430.0
90.90	128.0
92.00	1181.0
93.00	1296.0
94.00	4237.0
95.00	37360.0
96.00	2779.0
103.90	163.0
105.90	150.0
115.80	166.0
116.80	353.0
117.80	147.0
118.90	221.0
127.90	160.0
129.90	146.0
140.90	482.0
142.90	482.0
144.90	136.0
147.80	120.0
154.80	104.0
172.00	204.0
173.00	401.0
174.00	32032.0
175.00	2188.0
176.00	30528.0
176.90	2040.0
207.00	661.0
208.00	166.0

m/z	Abundance
36.10	342.0
37.00	1721.0
38.00	1572.0
39.00	614.0
39.90	122.0
44.10	507.0
45.00	361.0
47.00	349.0
48.00	258.0
49.00	1483.0
50.00	6439.0
51.00	2083.0
52.00	103.0
56.00	345.0
57.00	1055.0
59.90	403.0
61.00	1694.0
62.00	1664.0
63.00	1509.0
63.90	151.0
65.00	134.0
68.00	3610.0
69.00	3294.0
69.90	230.0
72.00	158.0
73.10	1754.0
74.00	6688.0
75.00	17864.0
76.00	1432.0
77.00	248.0
77.80	116.0
78.90	1112.0
79.80	287.0
81.00	1256.0
81.90	427.0
87.00	1346.0
88.00	1410.0
90.90	130.0
92.00	1092.0
93.00	1327.0
94.00	3882.0
95.00	35592.0
96.00	2695.0
103.90	132.0
105.90	151.0
115.90	158.0
116.80	318.0
117.80	120.0
118.90	229.0
127.80	116.0
129.90	121.0
140.90	468.0
142.90	513.0
144.90	116.0
147.80	104.0
155.00	107.0
171.90	190.0
172.90	428.0
174.00	32096.0
175.00	2355.0
176.00	30248.0
176.90	2087.0
207.10	585.0
208.00	200.0