


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU071819\
 Data File : VU033302.D
 Acq On : 18 Jul 2019 08:24
 Operator : JC/SP
 Sample : BFB36
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB36

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis
 Last Update : Fri Jul 19 22:54:17 2019

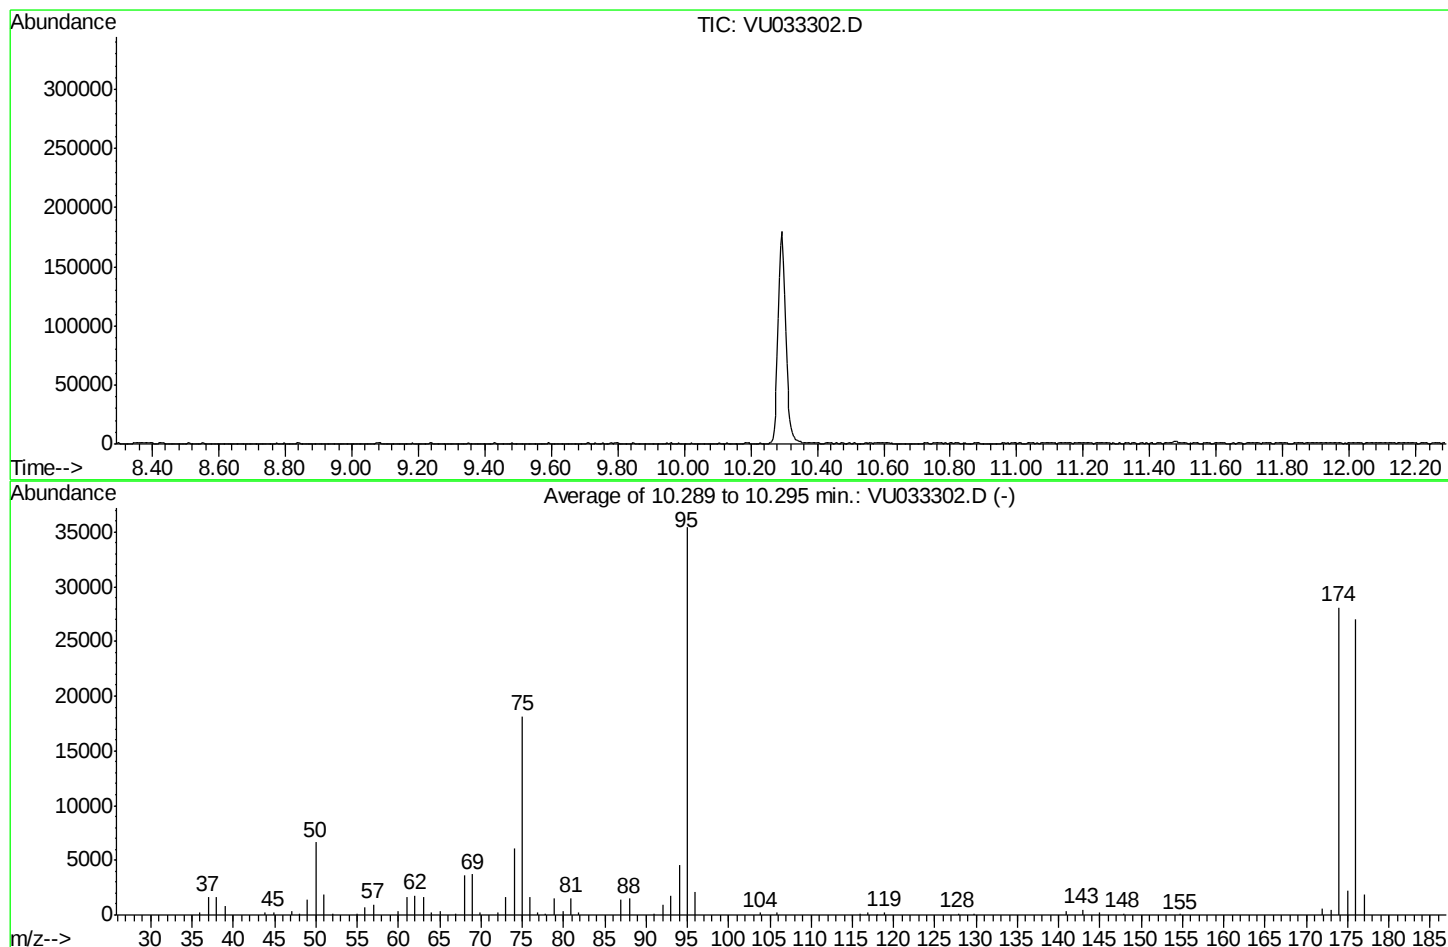

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	6616	PASS
75	95	30	80	51.3	18165	PASS
95	95	100	100	100.0	35426	PASS
96	95	5	9	5.9	2105	PASS
173	174	0.00	2	1.8	514	PASS
174	95	50	120	79.3	28104	PASS
175	174	5	9	8.0	2259	PASS
176	174	95	101	96.3	27058	PASS
177	176	5	9	7.1	1925	PASS

m/z	Abundance
39.90	238.0
43.90	320.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
35.90	253.0
37.00	1705.0
38.00	1616.0
39.00	810.0
40.00	166.0
44.00	524.0
44.90	293.0
47.10	317.0
48.10	177.0
49.00	1258.0
50.00	6701.0
51.00	1924.0
52.10	125.0
56.00	645.0
57.00	993.0
59.90	399.0
61.10	1563.0
62.00	1655.0
63.00	1612.0
63.90	294.0
65.00	315.0
66.90	124.0
68.00	3685.0
69.00	3742.0
69.90	312.0
71.90	193.0
73.00	1573.0
74.00	5864.0
75.00	17856.0
76.00	1733.0
76.90	243.0
77.90	175.0
78.90	1444.0
79.90	406.0
80.90	1451.0
81.90	222.0
87.00	1256.0
88.00	1384.0
91.00	108.0
92.00	1020.0
93.00	1772.0
94.00	4509.0
95.00	33992.0
96.00	2074.0
103.90	179.0
105.90	176.0
115.90	103.0
116.90	244.0
118.90	223.0
127.80	101.0
129.80	118.0
140.90	440.0
142.90	479.0
144.90	225.0
147.80	142.0
154.80	136.0
171.90	591.0
172.90	426.0
173.90	26240.0
174.90	2164.0
176.00	25440.0
176.90	1865.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
35.90	295.0
37.00	1720.0
38.00	1707.0
39.00	793.0
40.00	158.0
44.00	574.0
44.90	304.0
47.10	352.0
48.00	178.0
49.00	1424.0
50.00	6837.0
51.00	1953.0
52.00	158.0
55.00	103.0
56.00	727.0
57.00	992.0
59.90	375.0
61.00	1637.0
62.00	1866.0
63.00	1745.0
64.00	293.0
65.00	393.0
67.00	144.0
68.00	3754.0
69.00	3804.0
69.90	297.0
72.00	223.0
73.00	1757.0
74.00	6282.0
75.10	18816.0
76.00	1732.0
76.90	319.0
77.90	154.0
78.90	1592.0
79.90	374.0
80.90	1633.0
81.90	240.0
86.90	1375.0
88.00	1551.0
91.00	141.0
92.00	1026.0
93.00	1818.0
94.00	4695.0
95.00	36632.0
96.00	2107.0
103.90	243.0
105.90	192.0
116.00	138.0
116.90	227.0
119.00	272.0
127.90	122.0
129.80	121.0
140.90	412.0
142.90	517.0
144.90	215.0
147.80	140.0
154.70	138.0
171.90	603.0
173.00	522.0
174.00	29152.0
174.90	2345.0
176.00	27944.0
177.00	2002.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
35.90	314.0
37.00	1569.0
38.00	1656.0
39.10	759.0
40.00	189.0
43.90	567.0
44.90	285.0
47.10	291.0
48.00	177.0
49.00	1408.0
50.00	6311.0
51.00	1818.0
52.00	150.0
55.10	139.0
56.00	686.0
57.00	962.0
60.00	335.0
61.00	1693.0
62.00	1826.0
63.00	1742.0
64.00	246.0
65.00	434.0
67.00	134.0
68.00	3401.0
69.00	3608.0
70.00	247.0
72.10	245.0
73.00	1759.0
74.00	6006.0
75.10	17824.0
76.00	1588.0
76.90	275.0
77.80	129.0
78.90	1541.0
79.90	333.0
80.90	1614.0
81.80	263.0
86.90	1444.0
88.00	1543.0
91.00	128.0
92.00	915.0
93.00	1677.0
94.00	4507.0
95.00	35656.0
96.00	2136.0
103.90	270.0
105.90	175.0
116.00	127.0
116.90	245.0
117.90	126.0
118.90	262.0
127.80	143.0
129.80	118.0
140.90	367.0
142.90	488.0
144.90	162.0
147.90	113.0
171.90	629.0
173.00	595.0
174.00	28920.0
175.00	2269.0
176.00	27792.0
177.00	1909.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36