




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049773.D
 Acq On : 18 Jul 2022 20:23
 Operator : SY/MD
 Sample : N3700-15ME
 Misc : 5.75g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5B56ME

Manual IntegrationsAPPROVED

Quant Time: Jul 19 02:14:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 19 02:09:49 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/19/2022
 Supervised By :Mahesh Dadoda 07/19/2022

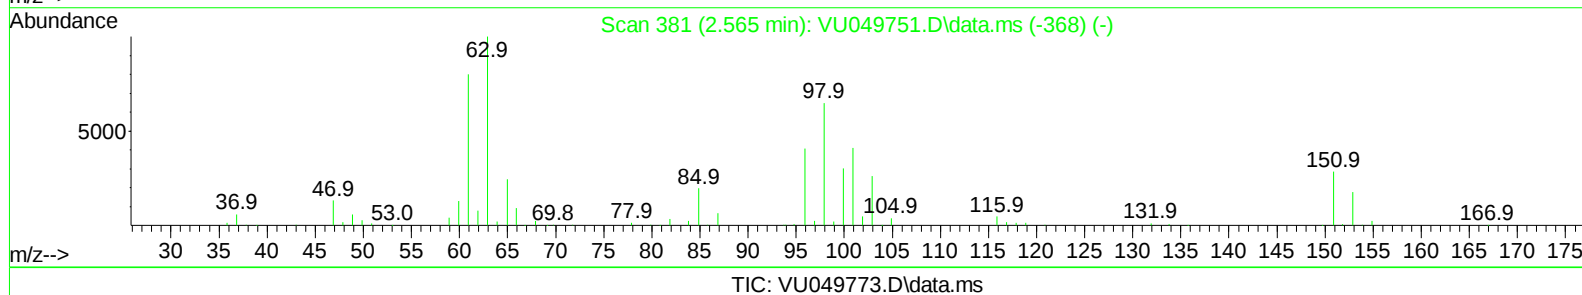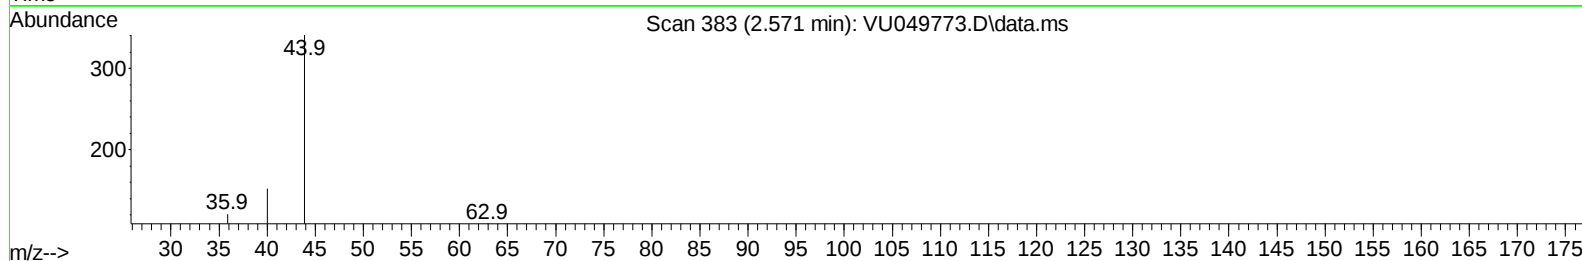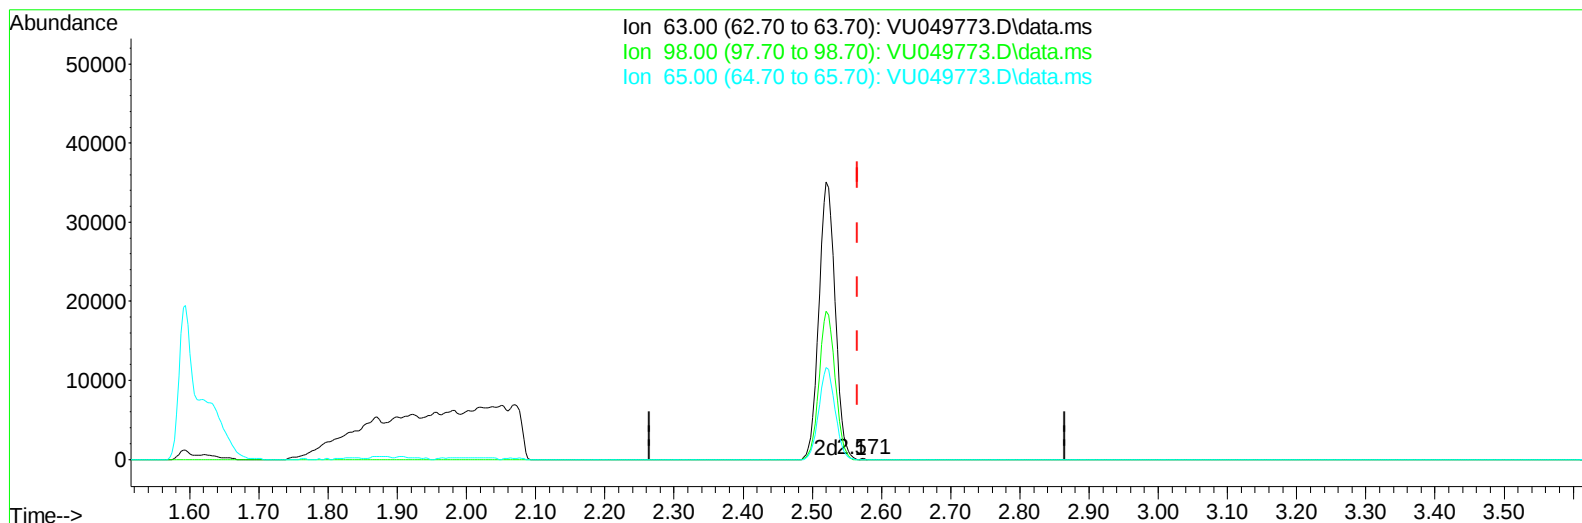

(11) 1,1-Dichloroethene-d2 (S)

2.571min (+ 0.006) 0.01 ug/L

response 41

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	69.30	0.00#
65.00	23.30	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049773.D
 Acq On : 18 Jul 2022 20:23
 Operator : SY/MD
 Sample : N3700-15ME
 Misc : 5.75g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5B56ME

Manual IntegrationsAPPROVED

Quant Time: Jul 19 02:14:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 19 02:09:49 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/19/2022
 Supervised By :Mahesh Dadoda 07/19/2022

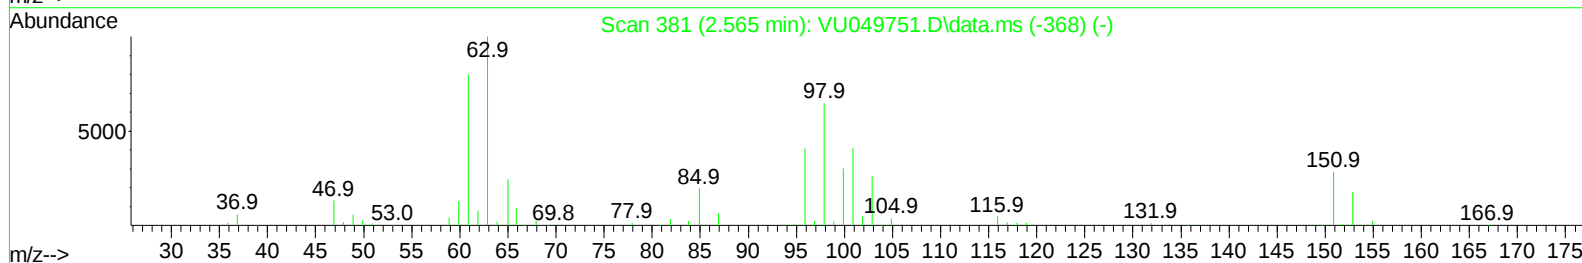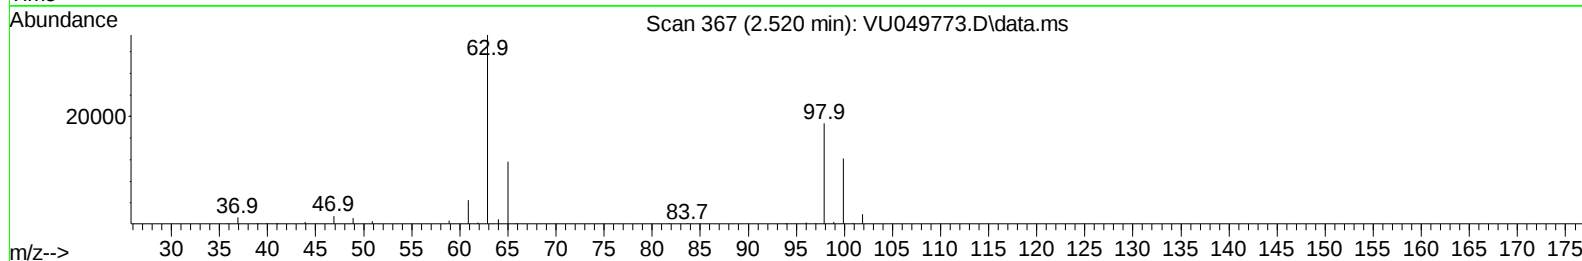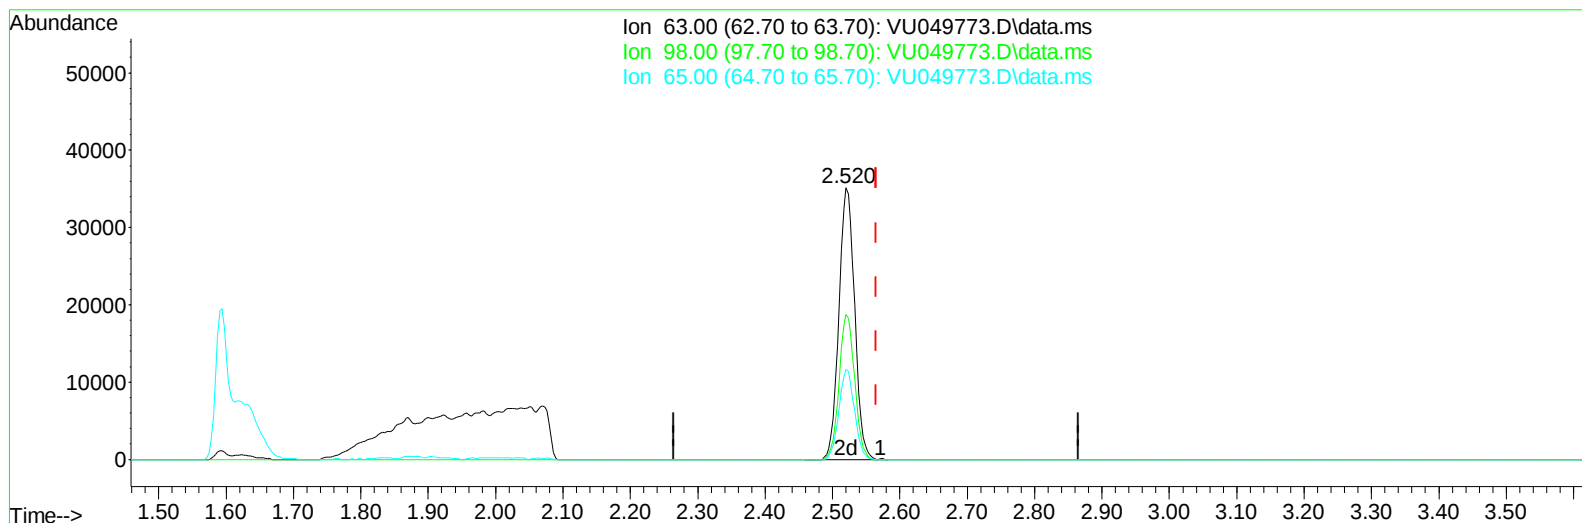

TIC: VU049773.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.520min (-0.045) 19.14 ug/L m

response 56984

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	69.30	0.00#
65.00	23.30	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049773.D
 Acq On : 18 Jul 2022 20:23
 Operator : SY/MD
 Sample : N3700-15ME
 Misc : 5.75g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5B56ME

Manual IntegrationsAPPROVED

Quant Time: Jul 19 02:14:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 19 02:09:49 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/19/2022
 Supervised By :Mahesh Dadoda 07/19/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	199815	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	192165	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	89888	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	26696	15.835	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery =	31.660%#		
7) Chloroethane-d5	1.870	69	20609	16.911	ug/L	-0.03
Spiked Amount 50.000	Range 70	- 130	Recovery =	33.820%#		
11) 1,1-Dichloroethene-d2	2.520	63	56984m	19.135	ug/L	-0.05
Spiked Amount 50.000	Range 60	- 125	Recovery =	38.280%#		
21) 2-Butanone-d5	4.636	46	161633	112.306	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery =	112.310%		
24) Chloroform-d	5.057	84	115218	38.585	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	77.180%		
26) 1,2-Dichloroethane-d4	5.697	65	84108	41.618	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	83.240%		
32) Benzene-d6	5.719	84	197270	33.791	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	67.580%#		
36) 1,2-Dichloropropane-d6	6.687	67	78683	40.070	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery =	80.140%		
41) Toluene-d8	7.896	98	160420	31.554	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery =	63.100%#		
43) trans-1,3-Dichloroprop...	8.182	79	30370	36.709	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery =	73.420%		
47) 2-Hexanone-d5	8.652	63	96997	109.813	ug/L	0.02
Spiked Amount 100.000	Range 45	- 130	Recovery =	109.810%		
56) 1,1,2,2-Tetrachloroeth...	10.761	84	137777	50.146	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery =	100.300%		
66) 1,2-Dichlorobenzene-d4	12.198	152	71267	42.051	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery =	84.100%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
Data File : VU049773.D
Acq On : 18 Jul 2022 20:23
Operator : SY/MD
Sample : N3700-15ME
Misc : 5.75g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5B56ME

Manual IntegrationsAPPROVED

Quant Time: Jul 19 02:14:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 19 02:09:49 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/19/2022
Supervised By :Mahesh Dadoda 07/19/2022

