

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049754.D
 Acq On : 18 Jul 2022 12:30
 Operator : SY/MD
 Sample : N3748-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	42	46	50	rBV2	1007	1068	0.15%	0.019%
2	1.597	72	80	91	rBV	64933	73208	10.22%	1.285%
3	1.899	165	174	191	rVB	55102	75627	10.55%	1.327%
4	2.494	357	359	365	rVB2	523	443	0.06%	0.008%
5	2.562	368	380	396	rVV	110357	174826	24.40%	3.068%
6	2.719	422	429	431	rBV2	263	306	0.04%	0.005%
7	2.755	436	440	443	rBV2	341	291	0.04%	0.005%
8	3.038	520	528	538	rBV4	706	945	0.13%	0.017%
9	3.115	548	552	556	rBV2	337	281	0.04%	0.005%
10	3.182	560	573	590	rBV	6001	13136	1.83%	0.231%
11	3.263	595	598	601	rBV2	214	142	0.02%	0.002%
12	3.407	639	643	648	rBV	134	161	0.02%	0.003%
13	3.462	657	660	664	rBV2	197	172	0.02%	0.003%
14	3.485	665	667	672	rVB	260	230	0.03%	0.004%
15	3.510	672	675	680	rBV2	201	161	0.02%	0.003%
16	3.546	680	686	689	rBV2	229	230	0.03%	0.004%
17	3.703	731	735	738	rBV2	192	147	0.02%	0.003%
18	3.886	790	792	799	rVB	186	148	0.02%	0.003%
19	4.366	936	941	944	rVB2	263	223	0.03%	0.004%
20	4.404	948	953	956	rVB	194	181	0.03%	0.003%
21	4.427	956	960	964	rBV2	261	275	0.04%	0.005%
22	4.565	999	1003	1008	rVB2	256	263	0.04%	0.005%
23	4.620	1008	1020	1059	rBV	105565	262124	36.58%	4.600%
24	4.835	1084	1087	1092	rBV	213	181	0.03%	0.003%
25	4.976	1128	1131	1134	rVB3	222	150	0.02%	0.003%
26	5.063	1142	1158	1182	rBV	138987	302886	42.27%	5.315%
27	5.208	1201	1203	1206	rVB	266	164	0.02%	0.003%
28	5.243	1206	1214	1216	rBV2	291	438	0.06%	0.008%
29	5.375	1250	1255	1260	rVV2	346	462	0.06%	0.008%
30	5.645	1335	1339	1342	rBV2	199	206	0.03%	0.004%
31	5.722	1342	1363	1389	rVV2	258280	716535	100.00%	12.574%
32	5.893	1412	1416	1419	rVB3	304	252	0.04%	0.004%
33	5.944	1427	1432	1433	rBV	306	184	0.03%	0.003%
34	6.041	1460	1462	1467	rVB2	311	201	0.03%	0.004%
35	6.070	1467	1471	1474	rBV2	246	173	0.02%	0.003%
36	6.099	1477	1480	1483	rVV2	163	143	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049754.D
 Acq On : 18 Jul 2022 12:30
 Operator : SY/MD
 Sample : N3748-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.247	1512	1526	1552	rBV	235920	446551	62.32%	7.836%
38	6.391	1567	1571	1574	rVB	424	369	0.05%	0.006%
39	6.433	1581	1584	1586	rVV2	257	159	0.02%	0.003%
40	6.484	1597	1600	1603	rVV2	287	191	0.03%	0.003%
41	6.526	1606	1613	1622	rVB3	1954	3171	0.44%	0.056%
42	6.594	1632	1634	1640	rVB2	336	247	0.03%	0.004%
43	6.629	1640	1645	1649	rBV2	136	160	0.02%	0.003%
44	6.690	1649	1664	1692	rBV	185501	359138	50.12%	6.302%
45	6.787	1692	1694	1699	rVB	269	154	0.02%	0.003%
46	6.819	1699	1704	1707	rBV3	392	345	0.05%	0.006%
47	7.015	1761	1765	1769	rVB2	193	150	0.02%	0.003%
48	7.041	1769	1773	1780	rBV2	117	177	0.02%	0.003%
49	7.185	1810	1818	1833	rVB3	1385	2140	0.30%	0.038%
50	7.398	1881	1884	1888	rBV	202	204	0.03%	0.004%
51	7.420	1888	1891	1895	rVV2	207	188	0.03%	0.003%
52	7.488	1908	1912	1915	rBV2	217	179	0.02%	0.003%
53	7.565	1923	1936	1958	rBV	92804	160216	22.36%	2.811%
54	7.668	1962	1968	1970	rBV2	241	273	0.04%	0.005%
55	7.687	1970	1974	1975	rBV2	674	416	0.06%	0.007%
56	7.799	2002	2009	2010	rBV	353	351	0.05%	0.006%
57	7.832	2015	2019	2021	rBV2	282	256	0.04%	0.004%
58	7.896	2025	2039	2060	rBV	287562	488200	68.13%	8.567%
59	8.179	2115	2127	2144	rBV	65325	106782	14.90%	1.874%
60	8.285	2157	2160	2166	rVB2	282	200	0.03%	0.004%
61	8.417	2197	2201	2208	rVB3	238	259	0.04%	0.005%
62	8.455	2208	2213	2217	rBV3	267	269	0.04%	0.005%
63	8.481	2217	2221	2223	rBV	362	260	0.04%	0.005%
64	8.542	2233	2240	2242	rBV2	208	231	0.03%	0.004%
65	8.558	2242	2245	2250	rVB	180	181	0.03%	0.003%
66	8.632	2256	2268	2300	rBV2	267723	531422	74.17%	9.325%
67	9.095	2409	2412	2415	rBV	270	192	0.03%	0.003%
68	9.246	2456	2459	2463	rVB2	302	189	0.03%	0.003%
69	9.417	2499	2512	2530	rBV	333319	551108	76.91%	9.671%
70	9.542	2549	2551	2554	rVB2	310	161	0.02%	0.003%
71	9.565	2555	2558	2562	rVB3	544	359	0.05%	0.006%
72	9.603	2568	2570	2573	rBV2	189	138	0.02%	0.002%
73	9.697	2590	2599	2602	rBV3	512	622	0.09%	0.011%
74	9.777	2618	2624	2625	rBV	297	274	0.04%	0.005%
75	9.880	2650	2656	2662	rVB2	427	661	0.09%	0.012%
76	9.915	2662	2667	2668	rBV	349	347	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049754.D
 Acq On : 18 Jul 2022 12:30
 Operator : SY/MD
 Sample : N3748-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	9.931	2669	2672	2675	rVV2	275	204	0.03%	0.004%
78	10.018	2695	2699	2703	rBV2	250	217	0.03%	0.004%
79	10.076	2714	2717	2721	rVB	344	280	0.04%	0.005%
80	10.102	2721	2725	2727	rBV2	383	339	0.05%	0.006%
81	10.188	2747	2752	2755	rBV	266	263	0.04%	0.005%
82	10.378	2808	2811	2816	rVB	174	174	0.02%	0.003%
83	10.455	2830	2835	2837	rBV	222	232	0.03%	0.004%
84	10.558	2864	2867	2872	rVB	264	207	0.03%	0.004%
85	10.703	2908	2912	2914	rBV2	311	269	0.04%	0.005%
86	10.754	2915	2928	2948	rVV	280768	445440	62.17%	7.816%
87	10.902	2971	2974	2980	rBV2	344	286	0.04%	0.005%
88	10.967	2992	2994	2999	rVB	233	136	0.02%	0.002%
89	11.812	3244	3257	3281	rBV	303731	484359	67.60%	8.499%
90	12.066	3333	3336	3339	rBV	220	163	0.02%	0.003%
91	12.192	3362	3375	3394	rBV	303313	480149	67.01%	8.426%
92	12.478	3461	3464	3466	rBV	253	177	0.02%	0.003%
93	12.574	3491	3494	3497	rBV2	317	195	0.03%	0.003%
94	12.770	3551	3555	3560	rBV3	410	390	0.05%	0.007%
95	12.848	3576	3579	3583	rBV	269	179	0.02%	0.003%
96	13.446	3762	3765	3769	rVB	337	254	0.04%	0.004%
97	14.063	3953	3957	3959	rBV	259	212	0.03%	0.004%
98	14.693	4150	4153	4157	rBV2	397	362	0.05%	0.006%
99	14.806	4184	4188	4191	rBV2	432	426	0.06%	0.007%
100	15.362	4358	4361	4363	rBV	478	372	0.05%	0.007%


Sum of corrected areas: 5698738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
Data File : VU049754.D
Acq On : 18 Jul 2022 12:30
Operator : SY/MD
Sample : N3748-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

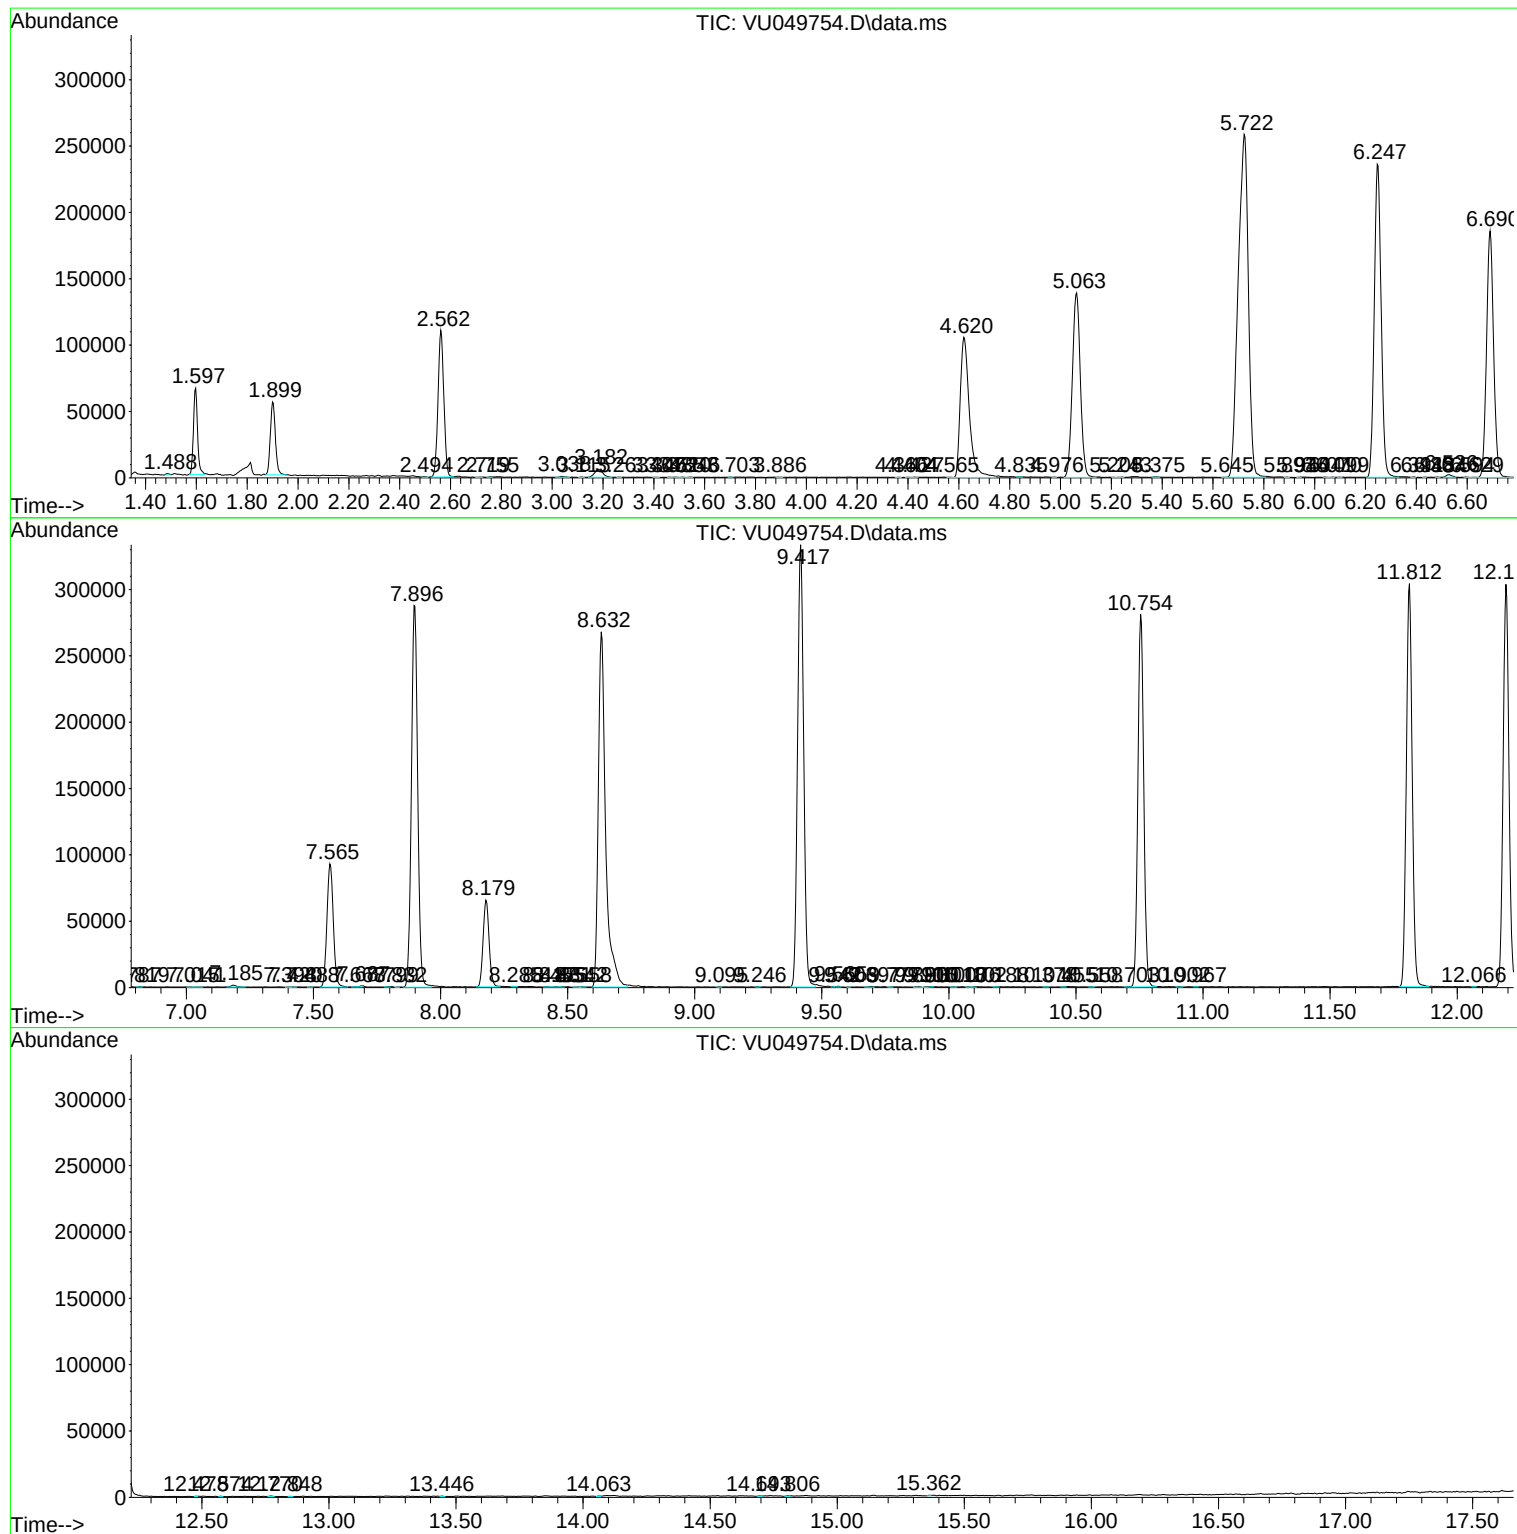

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
Data File : VU049754.D
Acq On : 18 Jul 2022 12:30
Operator : SY/MD
Sample : N3748-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
Data File : VU049754.D
Acq On : 18 Jul 2022 12:30
Operator : SY/MD
Sample : N3748-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc