

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049758.D
 Acq On : 18 Jul 2022 14:04
 Operator : SY/MD
 Sample : N3748-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH0E8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.517	51	55	59	rBV3	1825	1898	0.25%	0.033%
2	1.597	73	80	99	rVB	69252	77268	10.35%	1.333%
3	1.903	166	175	192	rVB	60093	80327	10.76%	1.386%
4	2.562	368	380	395	rBV	111775	179233	24.00%	3.092%
5	2.626	395	400	408	rVB3	1144	1533	0.21%	0.026%
6	2.761	439	442	446	rVB2	331	251	0.03%	0.004%
7	2.790	448	451	455	rBV2	423	386	0.05%	0.007%
8	2.945	496	499	505	rVB2	317	338	0.05%	0.006%
9	2.977	505	509	511	rBV	208	183	0.02%	0.003%
10	2.993	511	514	518	rVV2	339	310	0.04%	0.005%
11	3.044	524	530	536	rVV4	952	1298	0.17%	0.022%
12	3.076	536	540	548	rVV2	264	325	0.04%	0.006%
13	3.137	552	559	562	rVV2	244	356	0.05%	0.006%
14	3.186	562	574	588	rVV2	5361	11628	1.56%	0.201%
15	3.244	588	592	595	rVB2	238	170	0.02%	0.003%
16	3.350	618	625	627	rBV2	210	229	0.03%	0.004%
17	3.469	659	662	668	rVB2	223	209	0.03%	0.004%
18	3.559	686	690	692	rBV2	180	157	0.02%	0.003%
19	3.604	701	704	709	rVB2	229	179	0.02%	0.003%
20	3.671	722	725	732	rBV2	169	164	0.02%	0.003%
21	4.411	952	955	961	rBV2	192	171	0.02%	0.003%
22	4.507	977	985	987	rBV	268	386	0.05%	0.007%
23	4.620	1007	1020	1063	rBV	114129	280034	37.50%	4.830%
24	4.977	1128	1131	1135	rVB2	309	190	0.03%	0.003%
25	5.060	1141	1157	1175	rBV	143543	311280	41.68%	5.369%
26	5.295	1223	1230	1236	rVB4	615	1064	0.14%	0.018%
27	5.324	1236	1239	1244	rBV2	264	296	0.04%	0.005%
28	5.369	1251	1253	1258	rBV2	262	230	0.03%	0.004%
29	5.433	1270	1273	1277	rBV2	204	165	0.02%	0.003%
30	5.514	1295	1298	1302	rVB2	277	242	0.03%	0.004%
31	5.536	1302	1305	1307	rBV	231	190	0.03%	0.003%
32	5.723	1341	1363	1390	rBV2	270770	746844	100.00%	12.882%
33	5.925	1421	1426	1427	rBV	199	154	0.02%	0.003%
34	6.096	1477	1479	1483	rVB2	262	194	0.03%	0.003%
35	6.124	1483	1488	1491	rBV2	279	167	0.02%	0.003%
36	6.247	1512	1526	1547	rBV	241813	454800	60.90%	7.845%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049758.D
 Acq On : 18 Jul 2022 14:04
 Operator : SY/MD
 Sample : N3748-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH0E8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.420	1576	1580	1583	rVB2	347	177	0.02%	0.003%
38	6.530	1607	1614	1623	rBV5	1920	3684	0.49%	0.064%
39	6.591	1631	1633	1640	rVB2	353	325	0.04%	0.006%
40	6.690	1649	1664	1685	rVV	189879	371158	49.70%	6.402%
41	6.803	1695	1699	1704	rBV	324	378	0.05%	0.007%
42	6.903	1727	1730	1734	rVB2	218	180	0.02%	0.003%
43	6.957	1742	1747	1749	rBV	220	198	0.03%	0.003%
44	6.999	1758	1760	1767	rVB	285	243	0.03%	0.004%
45	7.038	1767	1772	1776	rBV2	380	422	0.06%	0.007%
46	7.060	1776	1779	1784	rBV2	277	307	0.04%	0.005%
47	7.182	1810	1817	1825	rBV6	1190	1984	0.27%	0.034%
48	7.218	1825	1828	1831	rVB2	310	198	0.03%	0.003%
49	7.285	1845	1849	1852	rBV	208	155	0.02%	0.003%
50	7.565	1923	1936	1957	rBV	95647	163940	21.95%	2.828%
51	7.684	1968	1973	1975	rBV3	637	595	0.08%	0.010%
52	7.787	2001	2005	2008	rBV2	418	292	0.04%	0.005%
53	7.896	2026	2039	2057	rBV	287819	492504	65.94%	8.495%
54	8.179	2115	2127	2144	rBV	64703	107853	14.44%	1.860%
55	8.388	2188	2192	2196	rBV2	357	330	0.04%	0.006%
56	8.459	2211	2214	2217	rBV2	267	181	0.02%	0.003%
57	8.507	2226	2229	2233	rBV	231	171	0.02%	0.003%
58	8.552	2237	2243	2251	rVB6	2416	3212	0.43%	0.055%
59	8.632	2255	2268	2296	rBV2	282824	555517	74.38%	9.582%
60	8.777	2310	2313	2314	rBV2	482	264	0.04%	0.005%
61	8.851	2331	2336	2339	rBV	269	230	0.03%	0.004%
62	8.906	2350	2353	2358	rVB2	271	213	0.03%	0.004%
63	9.044	2392	2396	2403	rBV2	232	314	0.04%	0.005%
64	9.198	2442	2444	2450	rVB	242	201	0.03%	0.003%
65	9.417	2499	2512	2531	rBV	336635	550041	73.65%	9.487%
66	9.619	2568	2575	2577	rBV	282	376	0.05%	0.006%
67	9.693	2595	2598	2603	rVB2	606	397	0.05%	0.007%
68	9.957	2677	2680	2685	rBV	237	175	0.02%	0.003%
69	10.571	2867	2871	2873	rBV2	385	268	0.04%	0.005%
70	10.706	2909	2913	2915	rBV2	238	207	0.03%	0.004%
71	10.754	2915	2928	2948	rVV	287874	460877	61.71%	7.950%
72	10.848	2954	2957	2960	rVB2	347	171	0.02%	0.003%
73	11.025	3009	3012	3017	rVB2	295	209	0.03%	0.004%
74	11.111	3034	3039	3043	rBV2	275	330	0.04%	0.006%
75	11.218	3069	3072	3076	rBV2	245	205	0.03%	0.004%
76	11.288	3092	3094	3098	rVB2	325	199	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049758.D
 Acq On : 18 Jul 2022 14:04
 Operator : SY/MD
 Sample : N3748-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH0E8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	11.314	3098	3102	3109	rBV	263	280	0.04%	0.005%
78	11.472	3149	3151	3154	rBV3	326	235	0.03%	0.004%
79	11.545	3171	3174	3179	rBV2	242	169	0.02%	0.003%
80	11.812	3245	3257	3275	rBV	281272	452724	60.62%	7.809%
81	12.063	3328	3335	3352	rVB4	2618	5162	0.69%	0.089%
82	12.192	3362	3375	3391	rBV	280694	461023	61.73%	7.952%
83	12.584	3488	3497	3500	rBV2	368	562	0.08%	0.010%
84	12.770	3551	3555	3559	rBV3	459	408	0.05%	0.007%
85	12.915	3597	3600	3602	rBV2	252	169	0.02%	0.003%
86	13.073	3647	3649	3652	rBV	259	166	0.02%	0.003%
87	13.471	3769	3773	3776	rBV2	373	268	0.04%	0.005%
88	13.581	3805	3807	3810	rVB	371	178	0.02%	0.003%
89	13.613	3814	3817	3821	rVB2	416	324	0.04%	0.006%
90	13.838	3884	3887	3891	rVB	477	311	0.04%	0.005%
91	13.857	3891	3893	3897	rBV	357	214	0.03%	0.004%
92	14.082	3961	3963	3965	rBV2	345	179	0.02%	0.003%
93	14.227	4006	4008	4012	rVB	379	263	0.04%	0.005%
94	14.262	4015	4019	4025	rBV2	482	489	0.07%	0.008%
95	14.372	4051	4053	4055	rBV	450	264	0.04%	0.005%
96	14.455	4077	4079	4082	rVB	536	291	0.04%	0.005%
97	14.574	4112	4116	4123	rVB4	869	834	0.11%	0.014%
98	14.658	4140	4142	4146	rVB2	344	180	0.02%	0.003%
99	14.992	4244	4246	4252	rBV2	463	564	0.08%	0.010%
100	16.529	4721	4724	4728	rBV2	921	769	0.10%	0.013%




Sum of corrected areas: 5797556

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
Data File : VU049758.D
Acq On : 18 Jul 2022 14:04
Operator : SY/MD
Sample : N3748-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH0E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

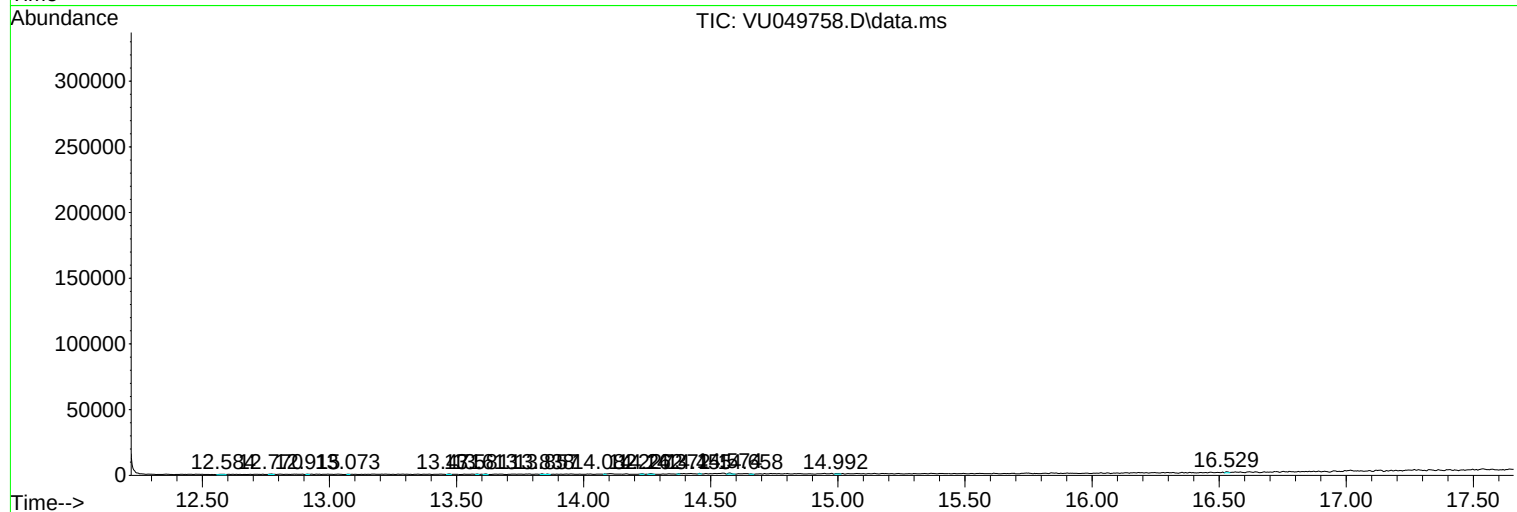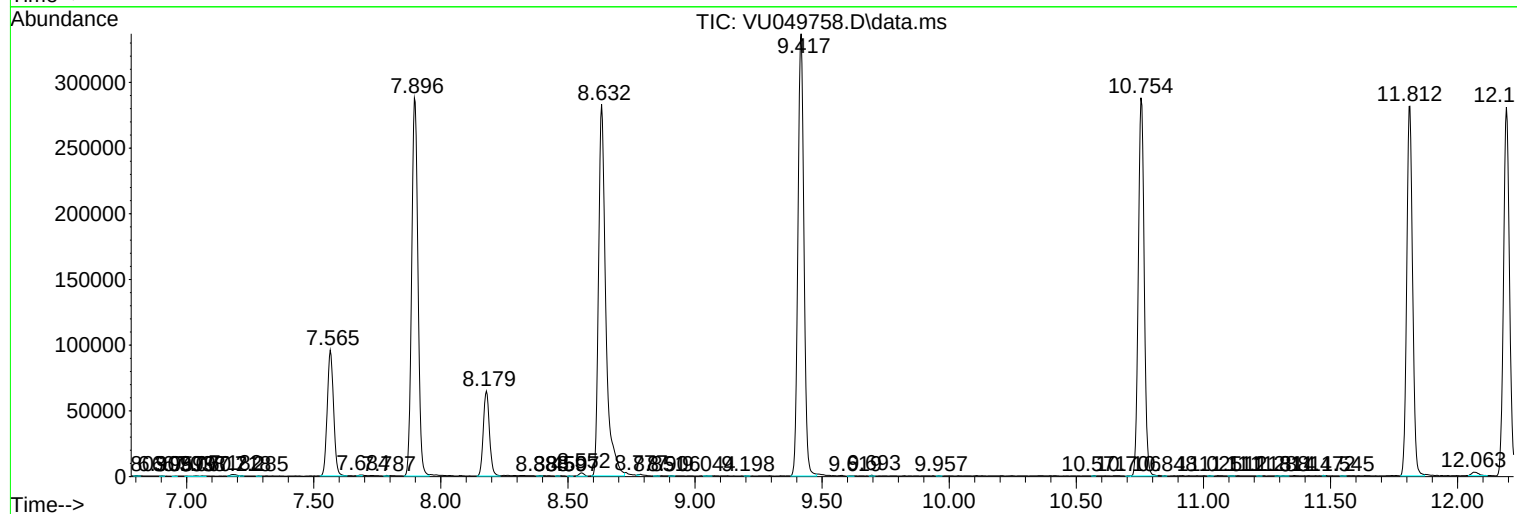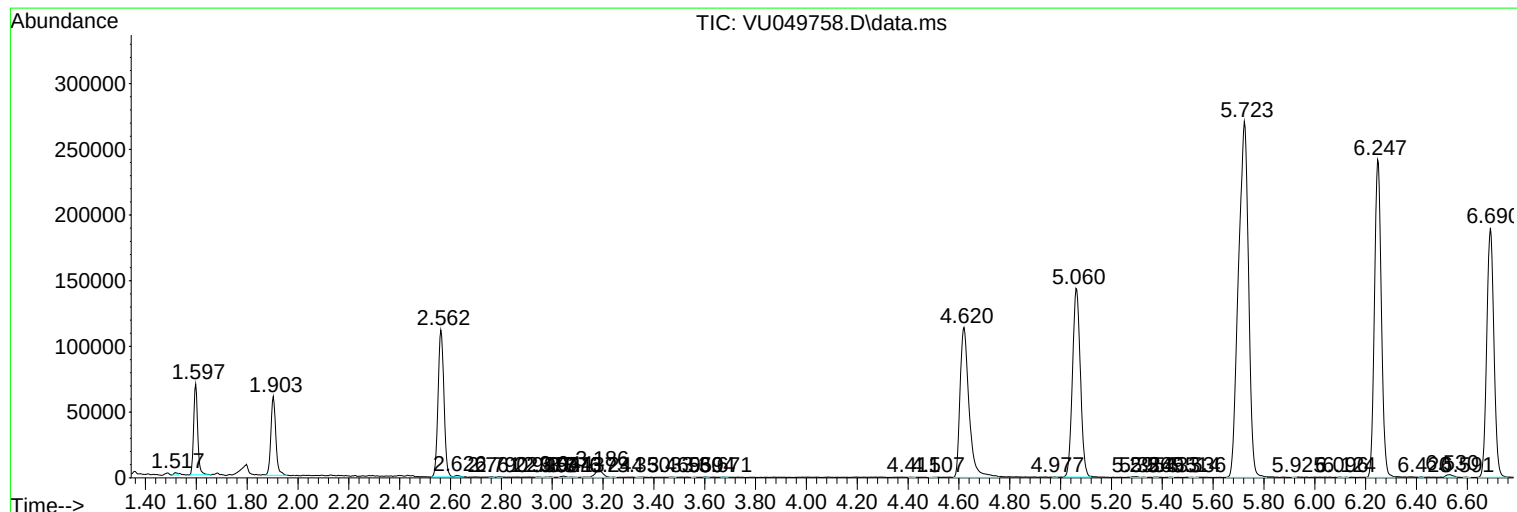

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
Data File : VU049758.D
Acq On : 18 Jul 2022 14:04
Operator : SY/MD
Sample : N3748-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH0E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
Data File : VU049758.D
Acq On : 18 Jul 2022 14:04
Operator : SY/MD
Sample : N3748-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH0E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------