

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049761.D
 Acq On : 18 Jul 2022 15:15
 Operator : SY/MD
 Sample : N3744-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.517	51	55	60	rBV2	1616	1916	0.22%	0.031%
2	1.597	72	80	99	rVB	120298	138067	16.09%	2.205%
3	1.900	165	174	193	rVB	87425	116802	13.61%	1.865%
4	2.562	367	380	393	rBV	162744	267150	31.14%	4.267%
5	2.781	444	448	454	rBV3	343	375	0.04%	0.006%
6	3.038	519	528	538	rVB2	3062	5232	0.61%	0.084%
7	3.183	563	573	578	rVB3	500	876	0.10%	0.014%
8	3.244	589	592	599	rVB	274	303	0.04%	0.005%
9	3.276	599	602	609	rBV2	256	284	0.03%	0.005%
10	3.330	615	619	621	rBV	213	186	0.02%	0.003%
11	3.472	657	663	666	rBV2	254	239	0.03%	0.004%
12	3.527	675	680	683	rBV2	399	462	0.05%	0.007%
13	3.575	691	695	700	rVB2	286	293	0.03%	0.005%
14	3.604	700	704	708	rBV2	265	233	0.03%	0.004%
15	4.009	820	830	834	rBV2	331	512	0.06%	0.008%
16	4.080	846	852	857	rBV	217	288	0.03%	0.005%
17	4.192	882	887	890	rBV2	243	226	0.03%	0.004%
18	4.260	906	908	911	rVB	236	141	0.02%	0.002%
19	4.395	946	950	954	rBV	181	150	0.02%	0.002%
20	4.620	1007	1020	1041	rBV	100597	239433	27.91%	3.824%
21	4.961	1121	1126	1129	rVB3	266	263	0.03%	0.004%
22	4.980	1129	1132	1134	rBV2	250	143	0.02%	0.002%
23	5.060	1141	1157	1180	rBV	155695	341544	39.81%	5.455%
24	5.144	1180	1183	1186	rVB2	485	318	0.04%	0.005%
25	5.166	1186	1190	1195	rVB2	284	257	0.03%	0.004%
26	5.237	1209	1212	1218	rBV2	169	207	0.02%	0.003%
27	5.272	1221	1223	1225	rBV2	233	149	0.02%	0.002%
28	5.369	1250	1253	1255	rBV	372	232	0.03%	0.004%
29	5.379	1255	1256	1259	rVV2	328	162	0.02%	0.003%
30	5.472	1280	1285	1291	rBV2	233	265	0.03%	0.004%
31	5.520	1295	1300	1303	rBV	137	149	0.02%	0.002%
32	5.629	1331	1334	1337	rVV	215	146	0.02%	0.002%
33	5.723	1342	1363	1385	rBV2	319328	857895	100.00%	13.701%
34	5.954	1429	1435	1441	rBV2	361	401	0.05%	0.006%
35	6.028	1453	1458	1462	rBV2	212	272	0.03%	0.004%
36	6.121	1485	1487	1492	rVB2	377	180	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049761.D
 Acq On : 18 Jul 2022 15:15
 Operator : SY/MD
 Sample : N3744-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.179	1501	1505	1509	rBV2	168	225	0.03%	0.004%
38	6.247	1512	1526	1548	rVV	250188	468217	54.58%	7.478%
39	6.353	1556	1559	1563	rVB3	220	171	0.02%	0.003%
40	6.485	1595	1600	1602	rBV	166	138	0.02%	0.002%
41	6.523	1607	1612	1620	rVV4	1404	1980	0.23%	0.032%
42	6.690	1646	1664	1684	rVV	206916	400728	46.71%	6.400%
43	6.771	1686	1689	1696	rVB3	804	691	0.08%	0.011%
44	6.809	1696	1701	1713	rBV2	573	914	0.11%	0.015%
45	6.935	1737	1740	1745	rVB	292	245	0.03%	0.004%
46	6.967	1745	1750	1752	rBV2	247	273	0.03%	0.004%
47	7.186	1808	1818	1830	rVB5	1177	1908	0.22%	0.030%
48	7.256	1838	1840	1843	rBV	205	150	0.02%	0.002%
49	7.411	1883	1888	1893	rBV2	199	276	0.03%	0.004%
50	7.456	1898	1902	1906	rBV	264	227	0.03%	0.004%
51	7.565	1923	1936	1957	rBV2	104476	183834	21.43%	2.936%
52	7.687	1968	1974	1983	rVB4	868	1038	0.12%	0.017%
53	7.771	1997	2000	2004	rBV2	217	146	0.02%	0.002%
54	7.825	2011	2017	2021	rBV2	308	322	0.04%	0.005%
55	7.896	2025	2039	2055	rBV	355776	611699	71.30%	9.769%
56	8.057	2085	2089	2093	rVB2	468	429	0.05%	0.007%
57	8.179	2116	2127	2143	rVV	71832	118620	13.83%	1.894%
58	8.395	2191	2194	2197	rVB	385	254	0.03%	0.004%
59	8.475	2217	2219	2223	rVB2	256	165	0.02%	0.003%
60	8.632	2252	2268	2302	rBV2	259225	512824	59.78%	8.190%
61	9.131	2419	2423	2427	rBV	243	196	0.02%	0.003%
62	9.288	2468	2472	2475	rBV	162	149	0.02%	0.002%
63	9.417	2499	2512	2529	rBV	348047	565863	65.96%	9.037%
64	9.517	2541	2543	2554	rVB4	996	960	0.11%	0.015%
65	9.694	2596	2598	2606	rVB2	235	210	0.02%	0.003%
66	9.761	2617	2619	2624	rVB2	239	197	0.02%	0.003%
67	9.787	2624	2627	2632	rBV2	239	230	0.03%	0.004%
68	10.189	2749	2752	2755	rBV2	268	212	0.02%	0.003%
69	10.340	2796	2799	2802	rBV	214	169	0.02%	0.003%
70	10.472	2837	2840	2842	rBV2	230	168	0.02%	0.003%
71	10.546	2860	2863	2866	rBV2	204	173	0.02%	0.003%
72	10.755	2915	2928	2949	rVB	274946	437220	50.96%	6.983%
73	10.941	2983	2986	2992	rBV2	269	307	0.04%	0.005%
74	11.012	3005	3008	3011	rBV2	200	148	0.02%	0.002%
75	11.076	3025	3028	3032	rBV	179	175	0.02%	0.003%
76	11.578	3182	3184	3189	rVB2	252	172	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049761.D
 Acq On : 18 Jul 2022 15:15
 Operator : SY/MD
 Sample : N3744-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	11.610	3190	3194	3198	rBV2	189	194	0.02%	0.003%
78	11.761	3238	3241	3243	rBV	251	179	0.02%	0.003%
79	11.812	3244	3257	3276	rVV	296672	472678	55.10%	7.549%
80	11.967	3303	3305	3310	rVB	256	170	0.02%	0.003%
81	12.070	3330	3337	3339	rBV3	1375	1647	0.19%	0.026%
82	12.192	3363	3375	3398	rBV	307883	494036	57.59%	7.890%
83	12.359	3423	3427	3429	rBV	383	287	0.03%	0.005%
84	12.398	3436	3439	3441	rBV	205	141	0.02%	0.002%
85	12.526	3473	3479	3482	rBV	457	578	0.07%	0.009%
86	12.652	3516	3518	3524	rVB2	303	244	0.03%	0.004%
87	12.700	3531	3533	3536	rBV	216	134	0.02%	0.002%
88	12.986	3620	3622	3627	rVB2	245	162	0.02%	0.003%
89	13.012	3627	3630	3631	rBV	259	142	0.02%	0.002%
90	13.359	3734	3738	3741	rBV2	248	204	0.02%	0.003%
91	13.867	3894	3896	3900	rVB	389	155	0.02%	0.002%
92	13.922	3911	3913	3916	rVB	420	226	0.03%	0.004%
93	13.941	3916	3919	3922	rBV2	314	212	0.02%	0.003%
94	13.996	3933	3936	3938	rBV2	270	159	0.02%	0.003%
95	14.131	3976	3978	3980	rBV	276	136	0.02%	0.002%
96	14.285	4023	4026	4032	rBV3	483	388	0.05%	0.006%
97	14.976	4238	4241	4243	rBV2	407	245	0.03%	0.004%
98	15.108	4279	4282	4285	rBV	423	274	0.03%	0.004%
99	15.275	4332	4334	4338	rBV2	494	325	0.04%	0.005%
100	16.668	4764	4767	4771	rBV4	1133	843	0.10%	0.013%




Sum of corrected areas: 6261533

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
Data File : VU049761.D
Acq On : 18 Jul 2022 15:15
Operator : SY/MD
Sample : N3744-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

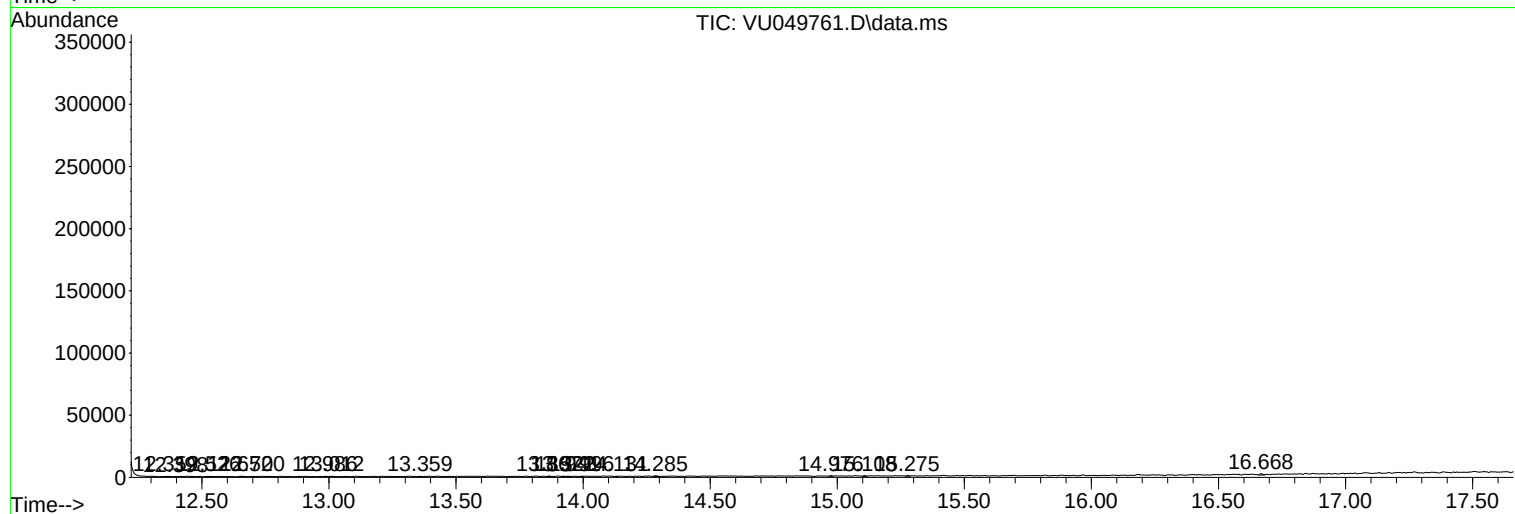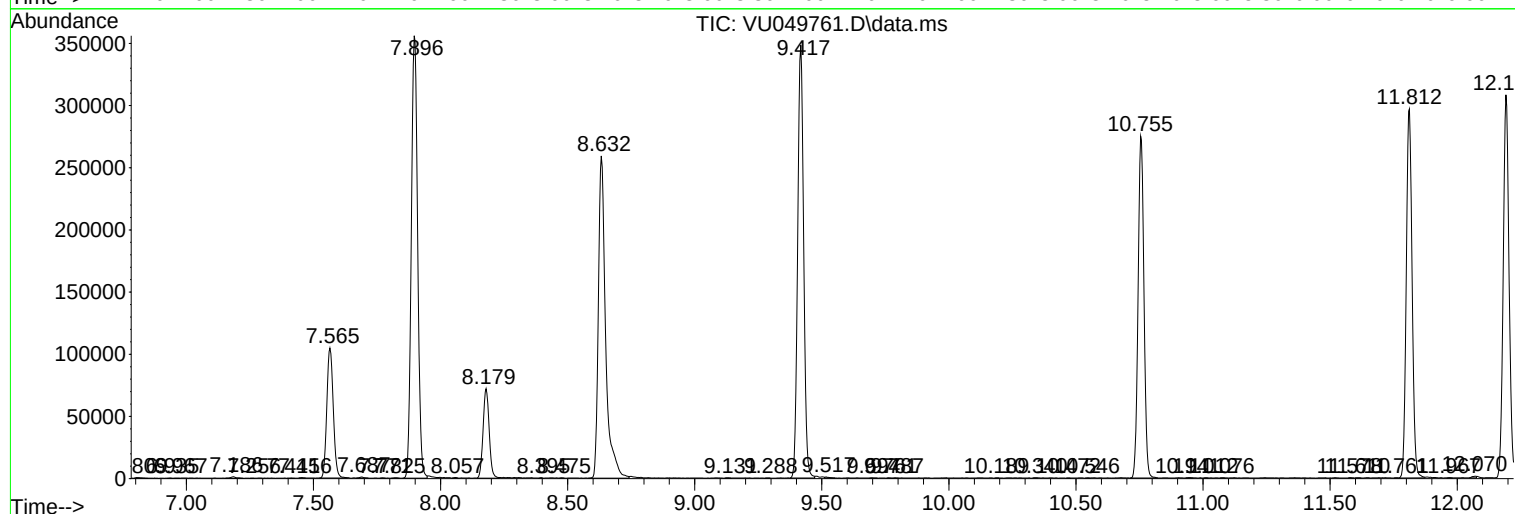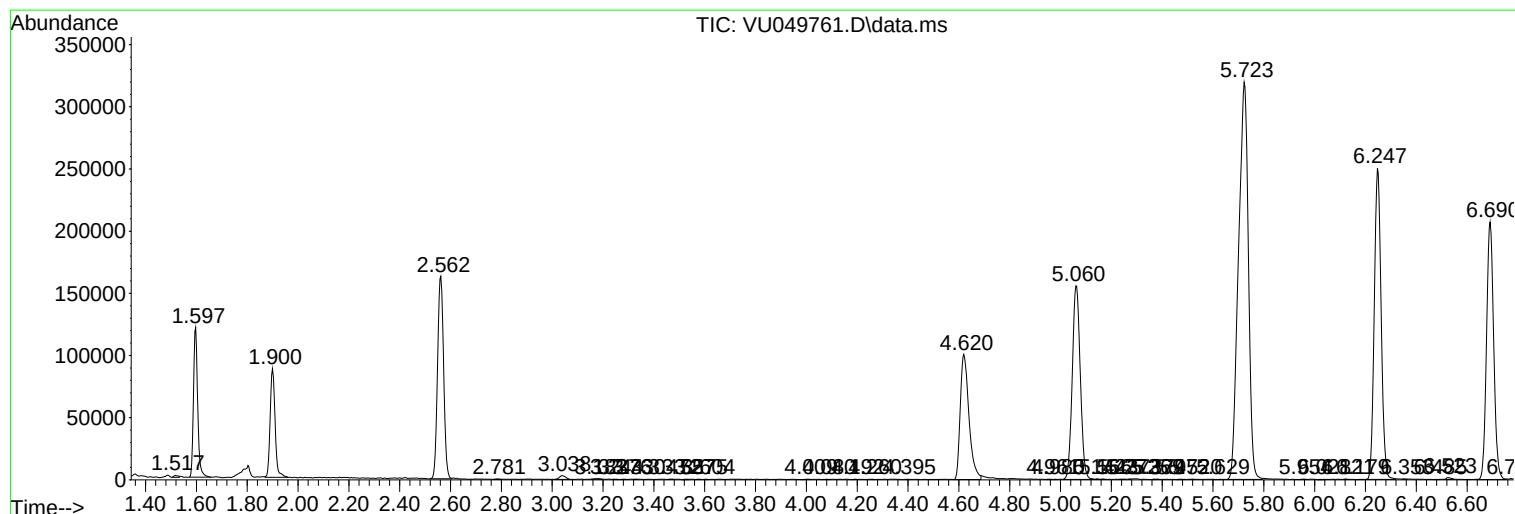

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
Data File : VU049761.D
Acq On : 18 Jul 2022 15:15
Operator : SY/MD
Sample : N3744-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
Data File : VU049761.D
Acq On : 18 Jul 2022 15:15
Operator : SY/MD
Sample : N3744-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------