

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049763.D
 Acq On : 18 Jul 2022 16:03
 Operator : SY/MD
 Sample : N3743-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.520	51	56	63	rBV2	1944	2526	0.30%	0.041%
2	1.597	71	80	97	rBV	112188	128942	15.30%	2.089%
3	1.900	166	174	194	rVB	80603	111340	13.21%	1.804%
4	2.202	266	268	271	rBV2	489	270	0.03%	0.004%
5	2.562	368	380	398	rBV	160755	257286	30.52%	4.169%
6	2.771	437	445	447	rBV3	583	684	0.08%	0.011%
7	2.851	466	470	472	rBV	291	251	0.03%	0.004%
8	3.041	520	529	539	rBV3	3057	5604	0.66%	0.091%
9	3.182	561	573	585	rVV	3830	7890	0.94%	0.128%
10	3.263	595	598	602	rBV	157	158	0.02%	0.003%
11	3.501	667	672	675	rBV	268	262	0.03%	0.004%
12	3.613	704	707	710	rBV	225	146	0.02%	0.002%
13	3.655	717	720	723	rBV	202	172	0.02%	0.003%
14	3.970	812	818	822	rBV2	418	563	0.07%	0.009%
15	4.012	826	831	833	rBV	422	357	0.04%	0.006%
16	4.253	902	906	910	rBV2	257	281	0.03%	0.005%
17	4.404	950	953	957	rBV2	195	154	0.02%	0.002%
18	4.620	1007	1020	1046	rBV2	103815	249881	29.65%	4.049%
19	4.935	1115	1118	1122	rVB3	289	199	0.02%	0.003%
20	4.964	1122	1127	1131	rBV3	273	288	0.03%	0.005%
21	4.983	1131	1133	1137	rVB2	210	172	0.02%	0.003%
22	5.060	1142	1157	1179	rVV	152786	331151	39.29%	5.366%
23	5.176	1191	1193	1196	rBV2	300	173	0.02%	0.003%
24	5.282	1219	1226	1227	rBV3	393	411	0.05%	0.007%
25	5.333	1240	1242	1248	rVB2	157	150	0.02%	0.002%
26	5.372	1249	1254	1256	rBV2	465	322	0.04%	0.005%
27	5.494	1289	1292	1296	rBV	195	184	0.02%	0.003%
28	5.597	1320	1324	1327	rBV	243	187	0.02%	0.003%
29	5.723	1342	1363	1382	rBV2	308912	842871	100.00%	13.659%
30	5.851	1400	1403	1408	rBV3	215	161	0.02%	0.003%
31	5.919	1420	1424	1427	rBV2	313	315	0.04%	0.005%
32	5.973	1438	1441	1444	rBV3	267	158	0.02%	0.003%
33	6.047	1461	1464	1467	rBV2	289	196	0.02%	0.003%
34	6.079	1471	1474	1478	rVB2	185	166	0.02%	0.003%
35	6.157	1493	1498	1500	rBV	237	243	0.03%	0.004%
36	6.247	1512	1526	1548	rBV	243163	456513	54.16%	7.398%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049763.D
 Acq On : 18 Jul 2022 16:03
 Operator : SY/MD
 Sample : N3743-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.385	1567	1569	1576	rVB3	301	285	0.03%	0.005%
38	6.488	1597	1601	1605	rVB2	240	200	0.02%	0.003%
39	6.530	1606	1614	1621	rBV6	1547	2353	0.28%	0.038%
40	6.597	1630	1635	1639	rBV2	243	242	0.03%	0.004%
41	6.690	1649	1664	1686	rBV	204306	395090	46.87%	6.402%
42	6.803	1696	1699	1700	rBV	279	182	0.02%	0.003%
43	6.813	1700	1702	1709	rVB2	631	527	0.06%	0.009%
44	6.848	1709	1713	1716	rBV	227	171	0.02%	0.003%
45	6.896	1724	1728	1731	rVB2	227	179	0.02%	0.003%
46	6.951	1740	1745	1749	rBV2	188	185	0.02%	0.003%
47	7.009	1759	1763	1765	rBV	199	170	0.02%	0.003%
48	7.121	1791	1798	1802	rBV2	200	298	0.04%	0.005%
49	7.182	1812	1817	1820	rBV2	1014	1029	0.12%	0.017%
50	7.446	1896	1899	1905	rBV2	149	187	0.02%	0.003%
51	7.565	1921	1936	1953	rBV	102721	178932	21.23%	2.900%
52	7.687	1970	1974	1982	rVB3	704	792	0.09%	0.013%
53	7.790	2003	2006	2015	rVB2	207	203	0.02%	0.003%
54	7.896	2025	2039	2065	rBV	347659	600723	71.27%	9.735%
55	8.179	2115	2127	2140	rBV2	70447	117075	13.89%	1.897%
56	8.346	2176	2179	2182	rVB2	293	198	0.02%	0.003%
57	8.632	2255	2268	2303	rBV2	265401	513078	60.87%	8.314%
58	8.751	2303	2305	2311	rVB3	446	471	0.06%	0.008%
59	8.925	2356	2359	2361	rBV	230	168	0.02%	0.003%
60	8.999	2379	2382	2385	rBV2	211	174	0.02%	0.003%
61	9.050	2393	2398	2402	rBV2	234	219	0.03%	0.004%
62	9.417	2496	2512	2536	rBV	332604	558544	66.27%	9.051%
63	9.546	2549	2552	2555	rBV	360	270	0.03%	0.004%
64	9.687	2593	2596	2598	rBV	210	153	0.02%	0.002%
65	9.944	2673	2676	2681	rVB	178	161	0.02%	0.003%
66	10.009	2694	2696	2699	rVB2	296	157	0.02%	0.003%
67	10.028	2699	2702	2704	rBV	233	153	0.02%	0.002%
68	10.224	2759	2763	2766	rBV2	238	199	0.02%	0.003%
69	10.369	2804	2808	2811	rBV2	228	177	0.02%	0.003%
70	10.414	2818	2822	2828	rBV	177	253	0.03%	0.004%
71	10.755	2915	2928	2947	rBV	270851	434079	51.50%	7.034%
72	10.899	2966	2973	2976	rBV2	190	245	0.03%	0.004%
73	10.973	2993	2996	3002	rVB	248	271	0.03%	0.004%
74	11.005	3003	3006	3008	rBV	197	144	0.02%	0.002%
75	11.041	3010	3017	3020	rVB2	197	209	0.02%	0.003%
76	11.144	3046	3049	3055	rBV	291	273	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
 Data File : VU049763.D
 Acq On : 18 Jul 2022 16:03
 Operator : SY/MD
 Sample : N3743-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	11.629	3193	3200	3203	rBV2	295	437	0.05%	0.007%
78	11.697	3219	3221	3226	rVB	298	223	0.03%	0.004%
79	11.812	3245	3257	3274	rBV	292680	467934	55.52%	7.583%
80	11.928	3291	3293	3296	rVB	325	154	0.02%	0.002%
81	11.941	3296	3297	3300	rBV	244	154	0.02%	0.002%
82	12.192	3363	3375	3395	rBV	299279	488307	57.93%	7.913%
83	12.369	3428	3430	3433	rBV	311	164	0.02%	0.003%
84	12.562	3486	3490	3491	rBV2	353	216	0.03%	0.004%
85	12.809	3563	3567	3571	rVB	314	239	0.03%	0.004%
86	12.877	3585	3588	3590	rBV	263	176	0.02%	0.003%
87	12.922	3599	3602	3604	rBV2	261	183	0.02%	0.003%
88	13.121	3660	3664	3668	rBV3	342	267	0.03%	0.004%
89	13.394	3745	3749	3753	rBV3	385	335	0.04%	0.005%
90	13.555	3797	3799	3805	rVB	376	248	0.03%	0.004%
91	13.848	3888	3890	3892	rBV2	249	145	0.02%	0.002%
92	14.024	3942	3945	3947	rBV2	283	159	0.02%	0.003%
93	14.121	3972	3975	3982	rVB3	505	478	0.06%	0.008%
94	14.304	4029	4032	4035	rBV2	384	266	0.03%	0.004%
95	14.417	4064	4067	4068	rBV	362	172	0.02%	0.003%
96	14.703	4153	4156	4161	rBV	409	328	0.04%	0.005%
97	14.735	4161	4166	4169	rVV3	330	341	0.04%	0.006%
98	14.751	4169	4171	4175	rVB2	410	194	0.02%	0.003%
99	16.291	4647	4650	4653	rVB2	823	466	0.06%	0.008%
100	16.311	4654	4656	4659	rVB2	697	394	0.05%	0.006%




Sum of corrected areas: 6171026

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
Data File : VU049763.D
Acq On : 18 Jul 2022 16:03
Operator : SY/MD
Sample : N3743-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

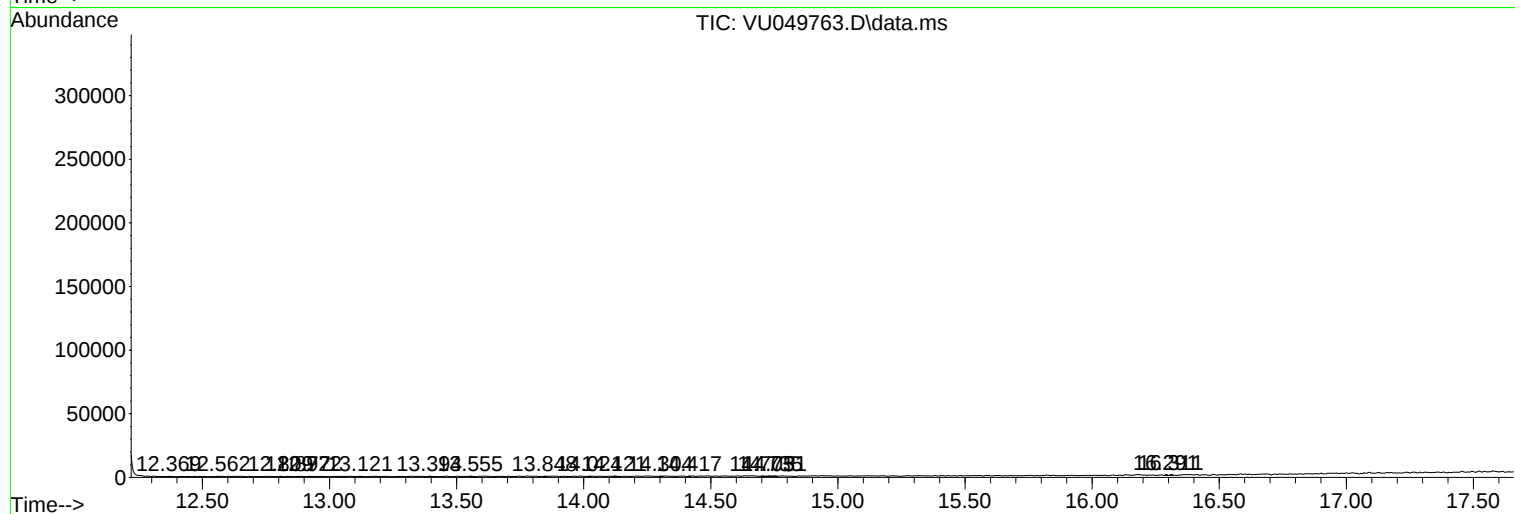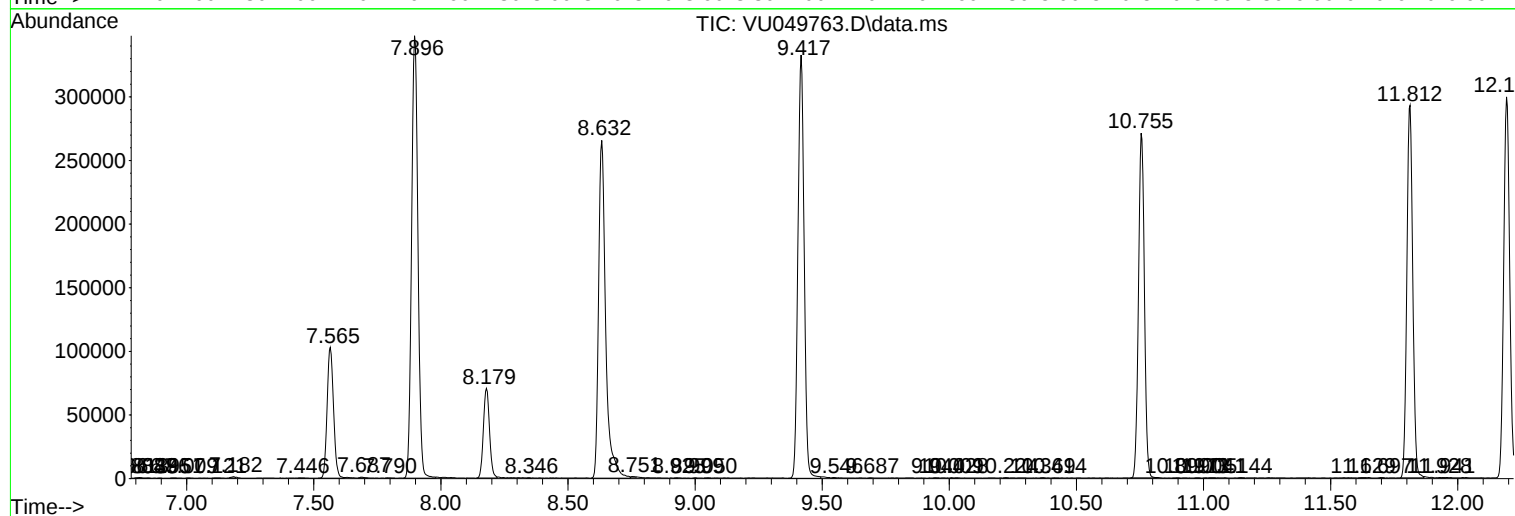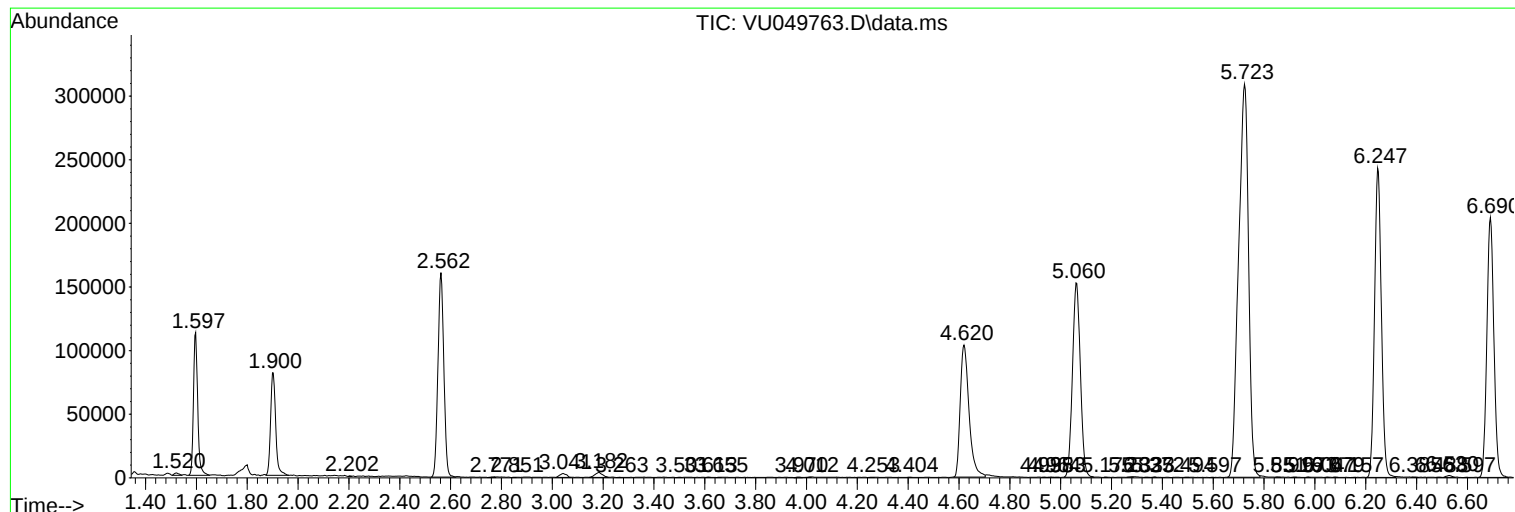

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
Data File : VU049763.D
Acq On : 18 Jul 2022 16:03
Operator : SY/MD
Sample : N3743-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
Data File : VU049763.D
Acq On : 18 Jul 2022 16:03
Operator : SY/MD
Sample : N3743-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------