
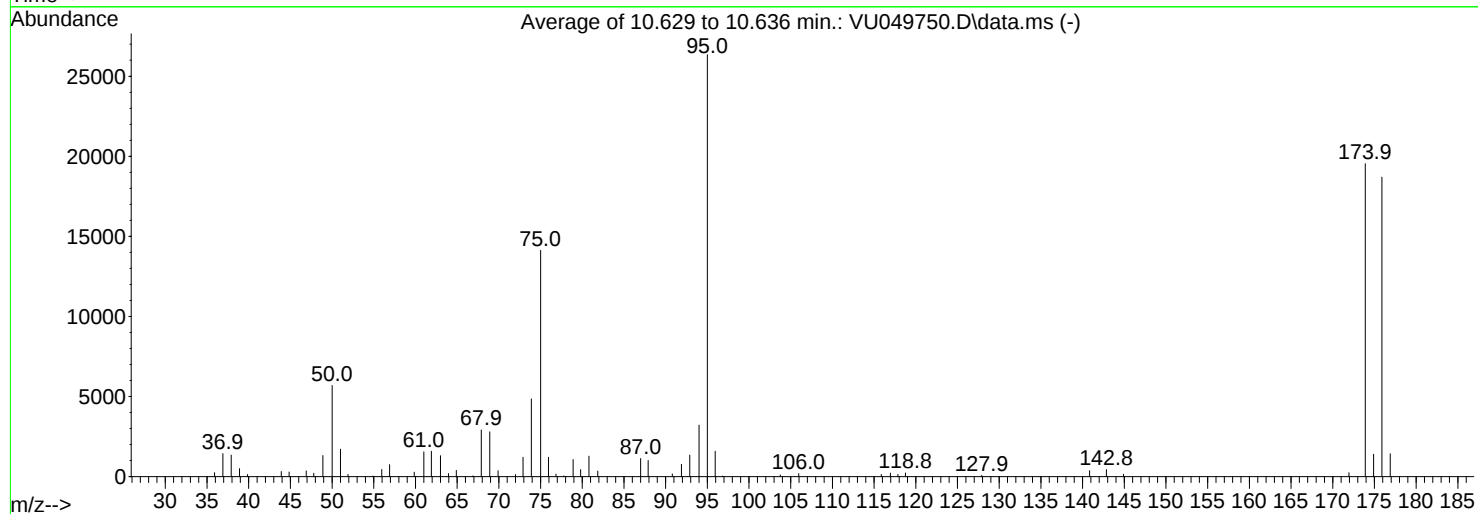


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071822\
Data File : VU049750.D
Acq On : 18 Jul 2022 09:56
Operator : SY/MD
Sample : BFB106
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB106

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Title : VOC Analysis
Last Update : Wed Jul 20 04:27:32 2022

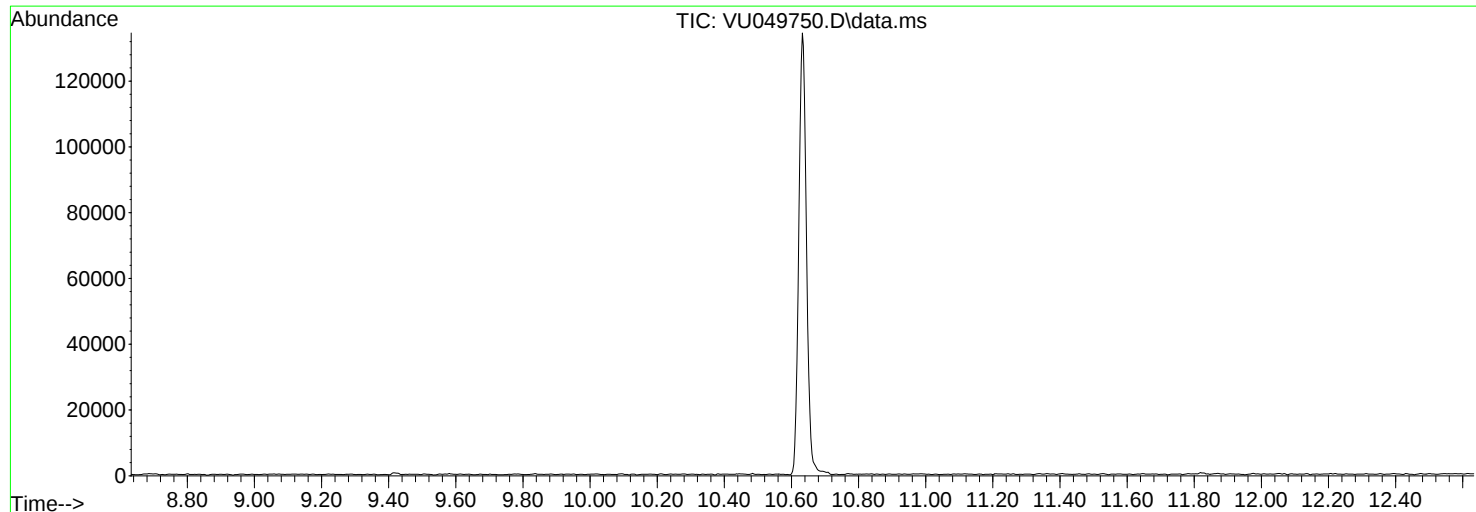

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	5687	PASS
75	95	30	80	53.6	14126	PASS
95	95	100	100	100.0	26341	PASS
96	95	5	9	6.0	1585	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.2	19541	PASS
175	174	5	9	7.2	1399	PASS
176	174	95	101	95.7	18701	PASS
177	176	5	9	7.6	1425	PASS

m/z	Abundance
39.80	105.0
44.00	210.0

Instrument :
MSVOA_U
ClientSampleId :
BFB106

m/z	Abundance
35.90	249.0
36.90	1483.0
37.90	1315.0
38.90	452.0
39.90	238.0
43.90	453.0
44.80	303.0
46.90	358.0
47.80	167.0
48.90	1286.0
50.00	5422.0
51.00	1741.0
51.90	122.0
55.90	433.0
56.90	745.0
59.90	219.0
61.00	1435.0
61.90	1587.0
63.00	1315.0
63.90	157.0
64.90	369.0
67.90	2830.0
68.90	2737.0
69.90	385.0
71.90	116.0
72.90	1152.0
73.90	4678.0
75.00	13932.0
76.00	1245.0
76.90	192.0
78.90	1046.0
79.80	412.0
80.80	1159.0
81.80	321.0
87.00	1104.0
87.90	901.0
90.80	209.0
91.90	739.0
92.90	1269.0
94.00	3129.0
95.00	25848.0
96.00	1568.0
106.00	155.0
115.90	149.0
117.00	194.0
117.90	100.0
118.70	193.0
140.90	339.0
142.90	403.0
144.90	131.0
172.00	199.0
173.90	18296.0
174.90	1359.0
175.90	17936.0
176.90	1338.0

Instrument :
MSVOA_U
ClientSampleId :
BFB106

m/z	Abundance
35.90	234.0
36.90	1461.0
37.90	1394.0
38.90	480.0
39.90	228.0
43.90	537.0
44.80	294.0
46.90	367.0
47.80	223.0
48.90	1364.0
50.00	5935.0
51.00	1780.0
51.90	145.0
56.00	441.0
56.90	768.0
59.80	281.0
61.00	1573.0
61.90	1661.0
63.00	1343.0
64.00	191.0
64.90	395.0
67.90	3002.0
68.90	2860.0
69.90	414.0
72.00	118.0
72.90	1206.0
73.90	5057.0
75.00	14510.0
75.90	1249.0
76.80	145.0
78.90	1080.0
79.80	437.0
80.80	1322.0
81.90	337.0
87.00	1191.0
87.90	1030.0
90.80	163.0
91.90	796.0
92.90	1358.0
94.00	3376.0
95.00	27320.0
96.00	1615.0
103.70	135.0
106.00	182.0
115.80	138.0
116.90	218.0
117.90	135.0
118.70	226.0
127.90	107.0
140.80	372.0
142.80	452.0
144.90	142.0
171.90	246.0
173.90	20136.0
174.90	1449.0
175.90	19512.0
176.90	1477.0

Instrument :
MSVOA_U
ClientSampleId :
BFB106

m/z	Abundance
35.90	248.0
36.90	1357.0
37.90	1328.0
38.90	551.0
39.90	214.0
43.90	585.0
44.90	259.0
46.90	330.0
47.80	241.0
48.90	1306.0
50.00	5704.0
51.00	1622.0
51.90	127.0
54.90	104.0
56.00	446.0
56.90	733.0
59.80	319.0
61.00	1620.0
61.90	1495.0
63.00	1258.0
64.00	194.0
64.90	386.0
66.90	123.0
67.90	2914.0
68.90	2770.0
69.90	307.0
72.10	146.0
72.90	1242.0
73.90	4830.0
75.00	13935.0
75.90	1123.0
76.90	143.0
77.80	127.0
78.90	1074.0
79.80	455.0
80.80	1342.0
81.90	365.0
87.00	1077.0
87.90	1083.0
90.70	114.0
91.90	746.0
92.90	1416.0
94.00	3142.0
95.00	25856.0
95.90	1572.0
96.80	105.0
103.80	170.0
105.90	207.0
115.80	120.0
116.90	221.0
117.80	161.0
118.80	257.0
127.90	115.0
140.80	385.0
142.80	438.0
144.90	168.0
171.90	280.0
173.90	20192.0
174.90	1390.0
175.90	18656.0
176.90	1459.0

Instrument :
MSVOA_U
ClientSampleId :
BFB106