

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
 Data File : VU054808.D
 Acq On : 18 Jul 2023 15:33
 Operator : MD/SY
 Sample : 03656-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH2W4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

Signal : TIC: VU054808.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	89	95	113	rBV	98761	136518	17.88%	2.107%
2	2.554	383	393	409	rVB	142742	229565	30.07%	3.542%
3	3.023	535	539	540	rBV4	992	691	0.09%	0.011%
4	3.078	554	556	561	rBV3	585	558	0.07%	0.009%
5	3.386	649	652	655	rBV4	960	697	0.09%	0.011%
6	3.499	684	687	691	rBV6	664	494	0.06%	0.008%
7	3.547	699	702	704	rBV2	521	410	0.05%	0.006%
8	3.653	733	735	740	rBV4	556	437	0.06%	0.007%
9	4.055	853	860	863	rBV2	679	761	0.10%	0.012%
10	4.116	876	879	882	rVB2	705	427	0.06%	0.007%
11	4.229	912	914	917	rVB	733	386	0.05%	0.006%
12	4.316	939	941	945	rVB2	734	387	0.05%	0.006%
13	4.415	969	972	975	rBV3	527	336	0.04%	0.005%
14	4.454	982	984	990	rVB3	481	434	0.06%	0.007%
15	4.483	990	993	995	rBV3	568	370	0.05%	0.006%
16	4.541	1007	1011	1014	rBV2	533	508	0.07%	0.008%
17	4.618	1023	1035	1060	rBV	82070	200444	26.25%	3.093%
18	4.891	1118	1120	1123	rVB4	612	317	0.04%	0.005%
19	4.914	1123	1127	1130	rBV5	623	476	0.06%	0.007%
20	4.971	1143	1145	1150	rBV3	549	506	0.07%	0.008%
21	5.055	1157	1171	1193	rBV	141835	309069	40.48%	4.769%
22	5.283	1238	1242	1246	rBV5	555	433	0.06%	0.007%
23	5.373	1268	1270	1276	rVV3	667	431	0.06%	0.007%
24	5.537	1315	1321	1326	rBV5	695	812	0.11%	0.013%
25	5.717	1357	1377	1398	rBV2	282380	763506	100.00%	11.782%
26	6.074	1486	1488	1493	rBV4	497	452	0.06%	0.007%
27	6.106	1495	1498	1500	rBV3	487	310	0.04%	0.005%
28	6.245	1528	1541	1561	rVV	263128	505663	66.23%	7.803%
29	6.450	1602	1605	1612	rBV3	439	559	0.07%	0.009%
30	6.685	1663	1678	1702	rBV2	186766	367029	48.07%	5.664%
31	6.894	1740	1743	1744	rBV3	706	445	0.06%	0.007%
32	7.016	1778	1781	1786	rBV4	517	472	0.06%	0.007%
33	7.045	1787	1790	1792	rVB2	596	284	0.04%	0.004%
34	7.071	1795	1798	1800	rBV2	456	296	0.04%	0.005%
35	7.087	1801	1803	1810	rVB4	782	654	0.09%	0.010%
36	7.119	1811	1813	1817	rVB3	643	430	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
 Data File : VU054808.D
 Acq On : 18 Jul 2023 15:33
 Operator : MD/SY
 Sample : 03656-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH2W4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

37	7.142	1817	1820	1822	rBV3	888	555	0.07%	0.009%
38	7.303	1867	1870	1875	rBV3	525	475	0.06%	0.007%
39	7.428	1906	1909	1912	rBV	439	359	0.05%	0.006%
40	7.473	1920	1923	1928	rBV4	673	510	0.07%	0.008%
41	7.563	1939	1951	1969	rBV	109121	193269	25.31%	2.982%
42	7.695	1985	1992	1999	rBV8	1900	3037	0.40%	0.047%
43	7.785	2017	2020	2021	rBV	524	302	0.04%	0.005%
44	7.894	2042	2054	2073	rBV	362865	632943	82.90%	9.767%
45	8.113	2118	2122	2127	rVB5	715	633	0.08%	0.010%
46	8.177	2131	2142	2157	rBV2	75433	128984	16.89%	1.990%
47	8.357	2194	2198	2199	rBV	594	334	0.04%	0.005%
48	8.434	2219	2222	2226	rVV3	635	455	0.06%	0.007%
49	8.550	2250	2258	2269	rVB4	18642	32176	4.21%	0.497%
50	8.630	2272	2283	2312	rBV	243038	455232	59.62%	7.025%
51	8.782	2327	2330	2331	rBV3	964	581	0.08%	0.009%
52	8.833	2343	2346	2347	rBV2	563	373	0.05%	0.006%
53	8.975	2387	2390	2394	rBV2	833	677	0.09%	0.010%
54	9.068	2416	2419	2422	rVB2	686	430	0.06%	0.007%
55	9.200	2455	2460	2461	rBV3	883	708	0.09%	0.011%
56	9.232	2468	2470	2474	rVB3	788	513	0.07%	0.008%
57	9.286	2484	2487	2490	rVB2	662	342	0.04%	0.005%
58	9.325	2497	2499	2504	rVB2	634	541	0.07%	0.008%
59	9.415	2514	2527	2552	rBV	385204	643416	84.27%	9.929%
60	9.540	2564	2566	2568	rVB2	767	361	0.05%	0.006%
61	9.563	2568	2573	2576	rBV4	580	598	0.08%	0.009%
62	9.624	2588	2592	2593	rBV2	606	340	0.04%	0.005%
63	9.698	2606	2615	2619	rBV6	1709	2812	0.37%	0.043%
64	9.746	2628	2630	2635	rVB2	846	479	0.06%	0.007%
65	9.843	2657	2660	2663	rBV	804	488	0.06%	0.008%
66	9.862	2663	2666	2669	rVV3	591	354	0.05%	0.005%
67	9.891	2672	2675	2677	rBV2	631	493	0.06%	0.008%
68	9.987	2702	2705	2710	rBV3	722	705	0.09%	0.011%
69	10.084	2731	2735	2737	rBV4	775	662	0.09%	0.010%
70	10.232	2777	2781	2782	rBV	613	339	0.04%	0.005%
71	10.264	2787	2791	2793	rBV2	532	425	0.06%	0.007%
72	10.338	2812	2814	2820	rBV4	908	823	0.11%	0.013%
73	10.364	2820	2822	2824	rVV2	473	297	0.04%	0.005%
74	10.396	2828	2832	2836	rBV2	480	466	0.06%	0.007%
75	10.489	2853	2861	2867	rBV6	1825	2873	0.38%	0.044%
76	10.692	2920	2924	2926	rBV2	736	506	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
 Data File : VU054808.D
 Acq On : 18 Jul 2023 15:33
 Operator : MD/SY
 Sample : 03656-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH2W4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

77	10.753	2931	2943	2961	rBV	321775	520967	68.23%	8.039%
78	10.904	2986	2990	2993	rBV3	560	637	0.08%	0.010%
79	11.061	3034	3039	3042	rBV2	515	530	0.07%	0.008%
80	11.161	3068	3070	3077	rBV4	502	415	0.05%	0.006%
81	11.344	3124	3127	3131	rVB3	730	586	0.08%	0.009%
82	11.380	3131	3138	3142	rBV6	1076	1361	0.18%	0.021%
83	11.515	3177	3180	3183	rBV2	675	376	0.05%	0.006%
84	11.618	3209	3212	3214	rBV2	500	312	0.04%	0.005%
85	11.743	3248	3251	3253	rBV3	771	638	0.08%	0.010%
86	11.810	3259	3272	3293	rBV	428202	684175	89.61%	10.558%
87	11.978	3321	3324	3325	rBV	695	466	0.06%	0.007%
88	12.074	3345	3354	3358	rBV7	2621	4222	0.55%	0.065%
89	12.190	3379	3390	3406	rBV	392736	624875	81.84%	9.643%
90	12.794	3575	3578	3581	rBV	472	349	0.05%	0.005%
91	12.849	3592	3595	3598	rBV5	539	421	0.06%	0.006%
92	12.891	3604	3608	3611	rBV3	857	790	0.10%	0.012%
93	12.990	3637	3639	3642	rVB2	557	318	0.04%	0.005%
94	13.119	3676	3679	3681	rBV2	708	446	0.06%	0.007%
95	13.289	3726	3732	3733	rBV2	560	570	0.07%	0.009%
96	13.299	3733	3735	3740	rVB3	1006	567	0.07%	0.009%
97	13.672	3848	3851	3853	rVV	689	387	0.05%	0.006%
98	13.846	3901	3905	3906	rBV2	739	501	0.07%	0.008%
99	13.904	3920	3923	3925	rBV2	596	428	0.06%	0.007%
100	14.074	3973	3976	3977	rBV2	1053	590	0.08%	0.009%




Sum of corrected areas: 6480360

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
Data File : VU054808.D
Acq On : 18 Jul 2023 15:33
Operator : MD/SY
Sample : 03656-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH2W4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

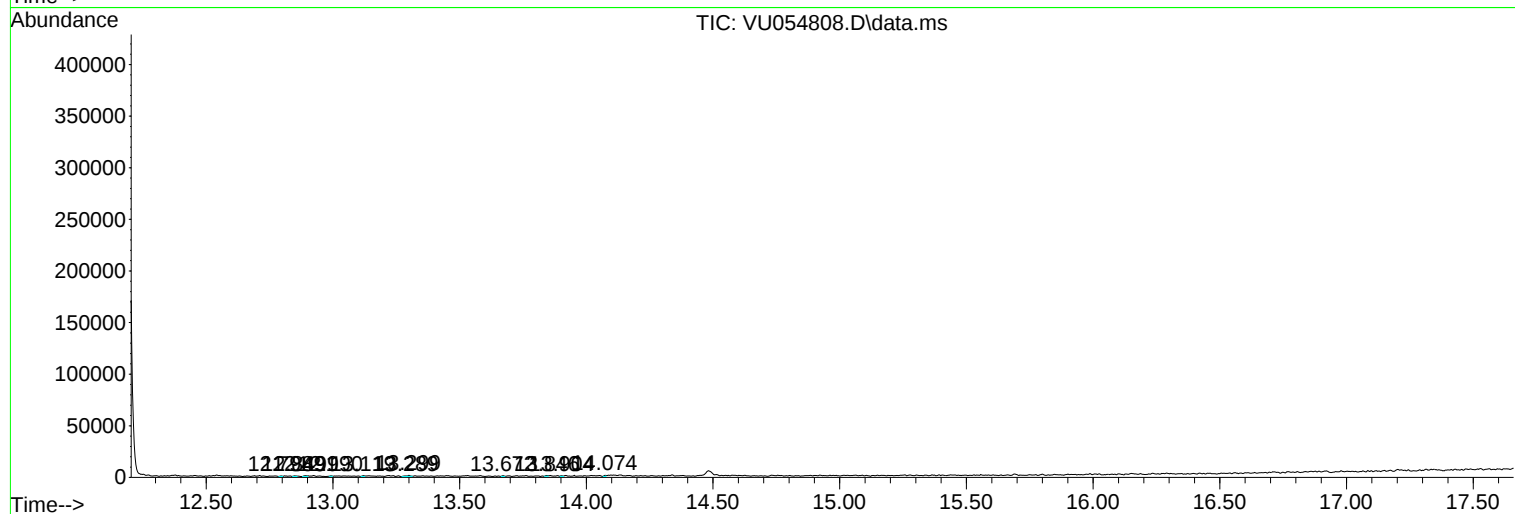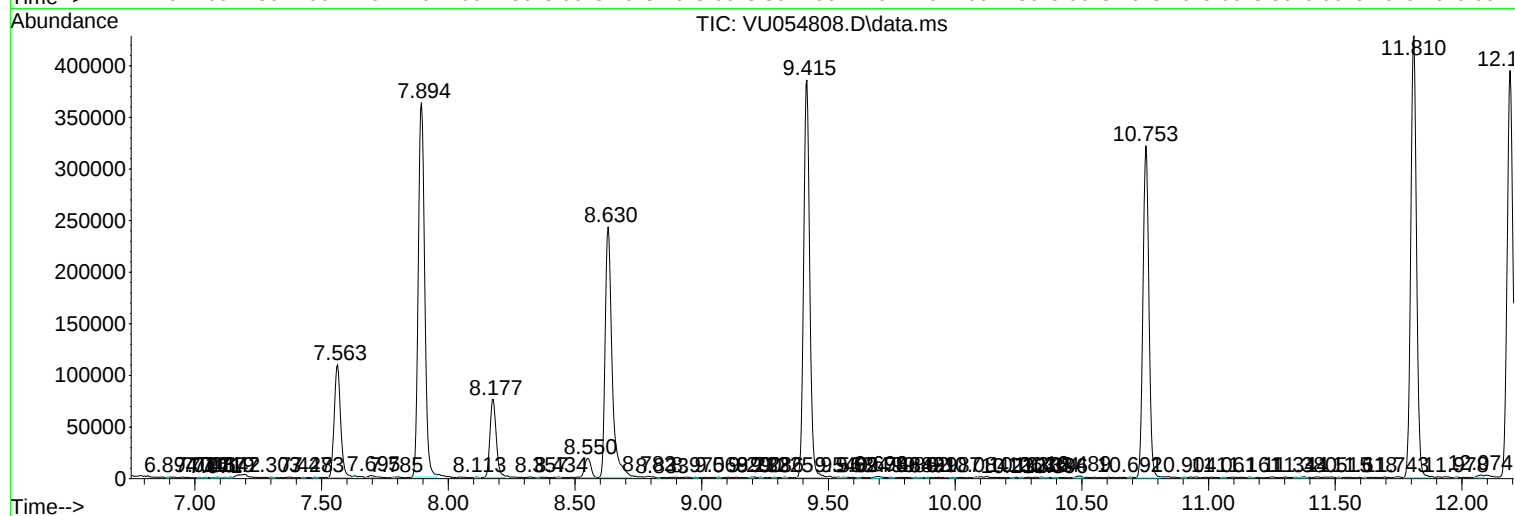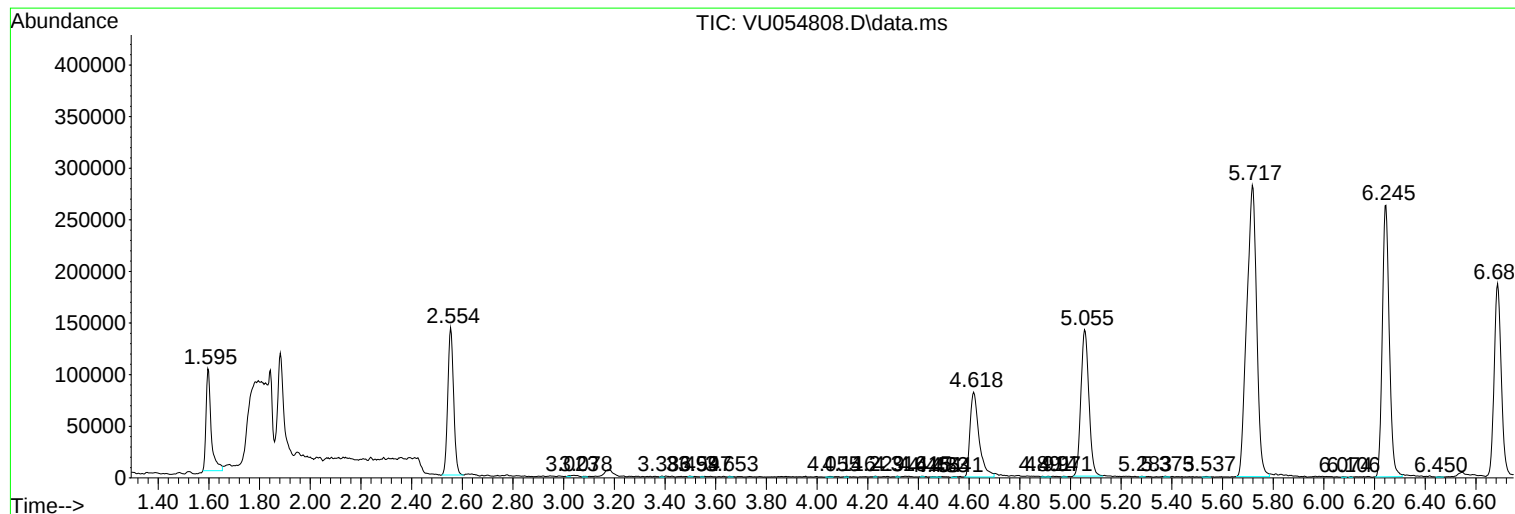

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
Data File : VU054808.D
Acq On : 18 Jul 2023 15:33
Operator : MD/SY
Sample : 03656-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH2W4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
Data File : VU054808.D
Acq On : 18 Jul 2023 15:33
Operator : MD/SY
Sample : 03656-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH2W4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------