

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
 Data File : VU054809.D
 Acq On : 18 Jul 2023 15:58
 Operator : MD/SY
 Sample : 03656-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH2X7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

Signal : TIC: VU054809.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	89	95	109	rBV	95551	126146	16.77%	1.964%
2	2.557	384	394	409	rVB	139906	227869	30.29%	3.548%
3	2.849	483	485	488	rVB2	844	342	0.05%	0.005%
4	3.181	574	588	605	rVB	9238	21529	2.86%	0.335%
5	3.759	765	768	770	rVB3	634	408	0.05%	0.006%
6	4.042	854	856	859	rBV2	385	249	0.03%	0.004%
7	4.084	866	869	870	rBV	279	149	0.02%	0.002%
8	4.107	874	876	879	rBV2	602	411	0.05%	0.006%
9	4.206	905	907	912	rVB3	689	458	0.06%	0.007%
10	4.254	919	922	925	rVB3	695	417	0.06%	0.006%
11	4.367	952	957	958	rBV2	542	461	0.06%	0.007%
12	4.492	993	996	998	rBV3	502	260	0.03%	0.004%
13	4.537	1008	1010	1011	rBV3	391	187	0.02%	0.003%
14	4.618	1024	1035	1057	rBV	81300	194820	25.90%	3.034%
15	5.000	1152	1154	1156	rBV3	691	337	0.04%	0.005%
16	5.058	1158	1172	1192	rVV	137579	306471	40.74%	4.772%
17	5.290	1241	1244	1247	rBV4	954	702	0.09%	0.011%
18	5.328	1251	1256	1261	rBV4	761	808	0.11%	0.013%
19	5.354	1261	1264	1266	rBV3	822	458	0.06%	0.007%
20	5.406	1272	1280	1283	rBV3	633	772	0.10%	0.012%
21	5.470	1297	1300	1302	rBV3	457	330	0.04%	0.005%
22	5.502	1307	1310	1312	rBV2	577	332	0.04%	0.005%
23	5.621	1342	1347	1348	rBV2	441	264	0.04%	0.004%
24	5.631	1348	1350	1354	rBV3	317	207	0.03%	0.003%
25	5.717	1358	1377	1397	rBV2	277094	752297	100.00%	11.714%
26	5.968	1453	1455	1458	rBV2	568	345	0.05%	0.005%
27	5.987	1458	1461	1466	rVB5	1044	947	0.13%	0.015%
28	6.110	1496	1499	1502	rBV3	718	440	0.06%	0.007%
29	6.158	1512	1514	1519	rVB3	607	420	0.06%	0.007%
30	6.187	1519	1523	1528	rBV4	752	841	0.11%	0.013%
31	6.245	1528	1541	1558	rBV	285599	540881	71.90%	8.422%
32	6.541	1623	1633	1643	rBV8	3371	8113	1.08%	0.126%
33	6.685	1665	1678	1698	rBV	183450	354430	47.11%	5.519%
34	6.923	1747	1752	1754	rVB4	720	512	0.07%	0.008%
35	6.942	1754	1758	1760	rBV2	605	470	0.06%	0.007%
36	6.975	1766	1768	1773	rVB4	816	458	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
 Data File : VU054809.D
 Acq On : 18 Jul 2023 15:58
 Operator : MD/SY
 Sample : 03656-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH2X7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

37	7.290	1863	1866	1874	rVB4	739	690	0.09%	0.011%
38	7.322	1874	1876	1877	rBV4	382	184	0.02%	0.003%
39	7.344	1881	1883	1885	rVB	558	173	0.02%	0.003%
40	7.422	1903	1907	1915	rBV5	754	676	0.09%	0.011%
41	7.454	1915	1917	1919	rBV3	383	144	0.02%	0.002%
42	7.470	1919	1922	1923	rBV2	587	303	0.04%	0.005%
43	7.489	1926	1928	1930	rVB2	672	242	0.03%	0.004%
44	7.508	1930	1934	1937	rBV3	544	492	0.07%	0.008%
45	7.563	1937	1951	1968	rBV	105326	189464	25.18%	2.950%
46	7.788	2018	2021	2023	rBV2	575	445	0.06%	0.007%
47	7.894	2038	2054	2074	rBV	352132	616980	82.01%	9.607%
48	8.177	2131	2142	2157	rBV2	71853	122706	16.31%	1.911%
49	8.357	2196	2198	2204	rVB3	827	538	0.07%	0.008%
50	8.454	2223	2228	2231	rBV4	655	561	0.07%	0.009%
51	8.508	2242	2245	2247	rBV3	496	248	0.03%	0.004%
52	8.550	2250	2258	2270	rBV6	10866	16934	2.25%	0.264%
53	8.630	2272	2283	2314	rBV2	223836	428055	56.90%	6.665%
54	8.894	2364	2365	2367	rBV2	474	215	0.03%	0.003%
55	8.942	2377	2380	2387	rBV4	642	697	0.09%	0.011%
56	8.975	2388	2390	2393	rVB3	571	299	0.04%	0.005%
57	9.016	2401	2403	2406	rBV	610	378	0.05%	0.006%
58	9.065	2417	2418	2420	rVB	584	208	0.03%	0.003%
59	9.081	2420	2423	2427	rBV4	670	549	0.07%	0.009%
60	9.200	2457	2460	2462	rBV3	467	197	0.03%	0.003%
61	9.264	2478	2480	2485	rVB3	785	497	0.07%	0.008%
62	9.296	2488	2490	2494	rBV	371	244	0.03%	0.004%
63	9.415	2513	2527	2551	rBV	406941	680955	90.52%	10.603%
64	9.566	2567	2574	2575	rBV2	795	717	0.10%	0.011%
65	9.618	2588	2590	2591	rBV	639	222	0.03%	0.003%
66	9.646	2595	2599	2603	rVV4	1114	815	0.11%	0.013%
67	9.775	2637	2639	2640	rBV	432	158	0.02%	0.002%
68	9.994	2705	2707	2709	rBV	271	141	0.02%	0.002%
69	10.065	2726	2729	2731	rBV3	323	186	0.02%	0.003%
70	10.077	2731	2733	2735	rBV3	395	226	0.03%	0.004%
71	10.103	2738	2741	2746	rBV5	1038	965	0.13%	0.015%
72	10.174	2760	2763	2765	rBV3	345	253	0.03%	0.004%
73	10.293	2798	2800	2804	rBV2	538	384	0.05%	0.006%
74	10.402	2831	2834	2838	rBV4	551	327	0.04%	0.005%
75	10.431	2840	2843	2845	rVV2	427	251	0.03%	0.004%
76	10.470	2853	2855	2857	rBV2	485	293	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
 Data File : VU054809.D
 Acq On : 18 Jul 2023 15:58
 Operator : MD/SY
 Sample : 03656-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH2X7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

77	10.569	2884	2886	2894	rVB3	573	532	0.07%	0.008%
78	10.601	2894	2896	2902	rBV2	602	397	0.05%	0.006%
79	10.666	2914	2916	2917	rBV	439	171	0.02%	0.003%
80	10.753	2929	2943	2961	rBV	301043	489930	65.12%	7.629%
81	10.868	2976	2979	2983	rVB3	846	570	0.08%	0.009%
82	11.052	3033	3036	3039	rVV3	400	248	0.03%	0.004%
83	11.142	3059	3064	3068	rBV3	918	1001	0.13%	0.016%
84	11.164	3068	3071	3077	rBV4	796	864	0.11%	0.013%
85	11.232	3088	3092	3093	rBV3	383	268	0.04%	0.004%
86	11.306	3109	3115	3118	rBV4	809	998	0.13%	0.016%
87	11.351	3127	3129	3131	rBV2	650	441	0.06%	0.007%
88	11.486	3169	3171	3176	rBV3	582	464	0.06%	0.007%
89	11.807	3259	3271	3286	rBV	453339	706740	93.94%	11.005%
90	11.923	3305	3307	3314	rBV4	797	703	0.09%	0.011%
91	12.064	3344	3351	3352	rBV5	1757	1900	0.25%	0.030%
92	12.190	3378	3390	3407	rBV	371790	601240	79.92%	9.362%
93	12.852	3593	3596	3598	rBV	524	329	0.04%	0.005%
94	13.007	3641	3644	3645	rBV2	440	246	0.03%	0.004%
95	13.042	3652	3655	3659	rVB3	877	617	0.08%	0.010%
96	13.254	3718	3721	3723	rBV2	396	264	0.04%	0.004%
97	13.518	3800	3803	3806	rBV3	537	438	0.06%	0.007%
98	13.916	3924	3927	3932	rBV2	1100	843	0.11%	0.013%
99	14.183	4008	4010	4011	rBV	413	139	0.02%	0.002%
100	14.408	4078	4080	4081	rBV	551	213	0.03%	0.003%




Sum of corrected areas: 6422109

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
Data File : VU054809.D
Acq On : 18 Jul 2023 15:58
Operator : MD/SY
Sample : 03656-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH2X7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

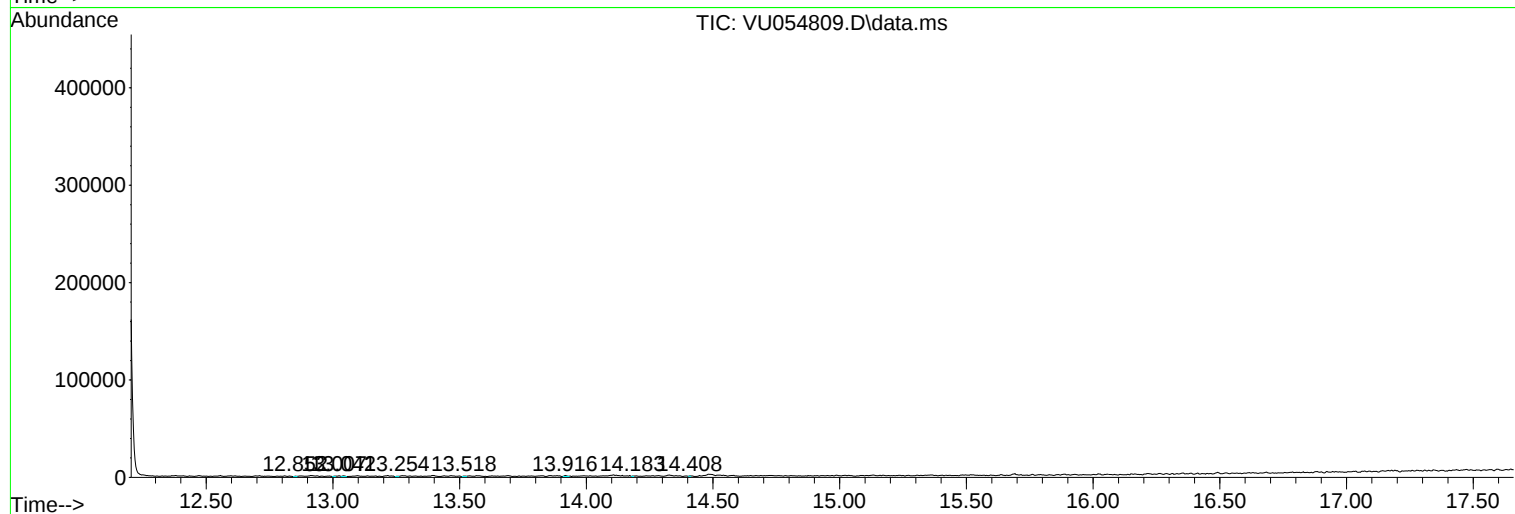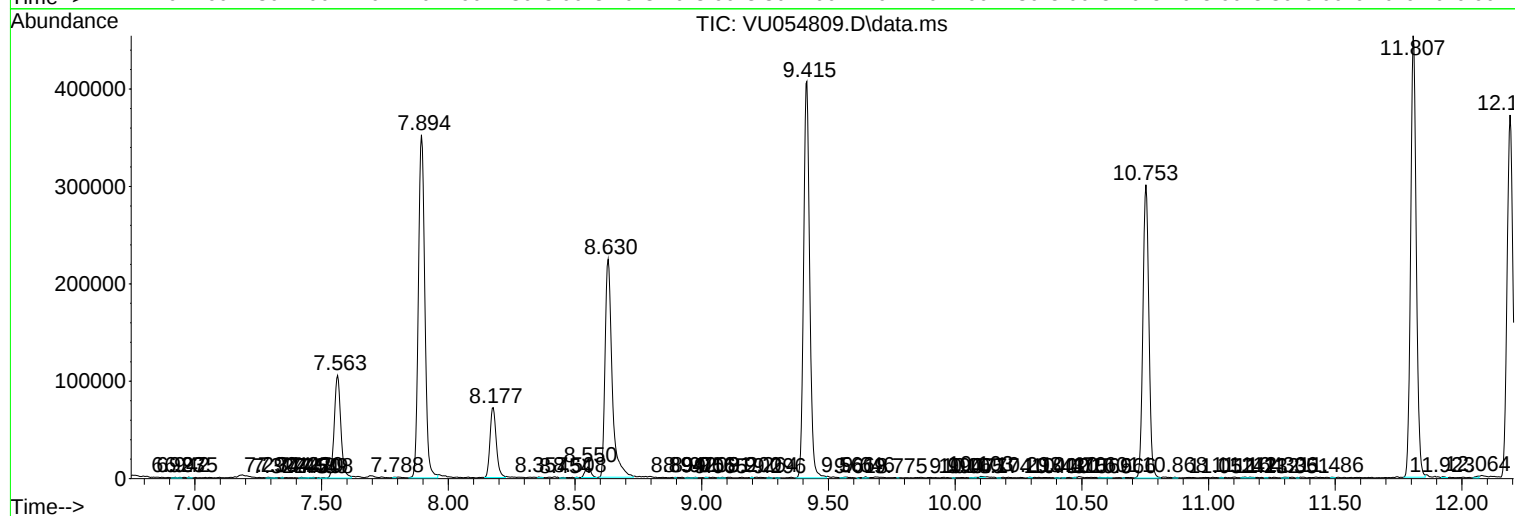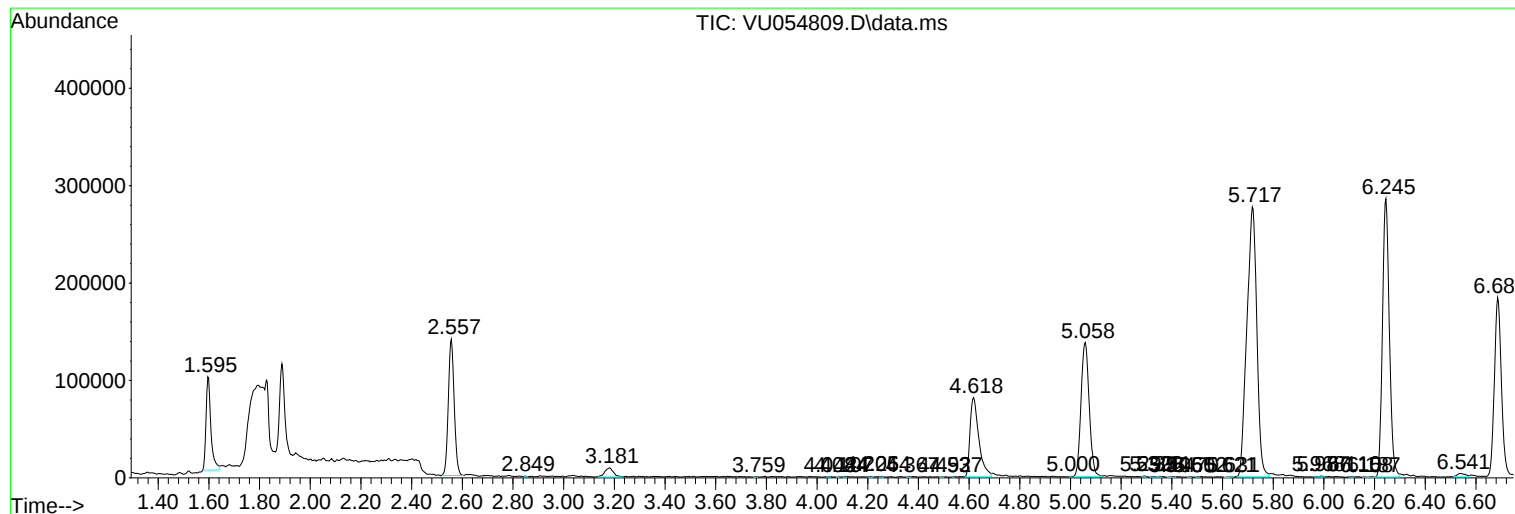

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
Data File : VU054809.D
Acq On : 18 Jul 2023 15:58
Operator : MD/SY
Sample : 03656-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH2X7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
Data File : VU054809.D
Acq On : 18 Jul 2023 15:58
Operator : MD/SY
Sample : 03656-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH2X7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------