

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
 Data File : VU054812.D
 Acq On : 18 Jul 2023 17:12
 Operator : MD/SY
 Sample : 03656-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

Signal : TIC: VU054812.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	89	95	110	rBV	87247	120967	16.45%	1.874%
2	2.550	382	392	408	rVB	136164	218676	29.74%	3.387%
3	2.898	498	500	503	rVB3	670	261	0.04%	0.004%
4	3.174	575	586	607	rVB	12790	30682	4.17%	0.475%
5	3.518	690	693	694	rBV2	709	454	0.06%	0.007%
6	3.647	729	733	736	rBV4	599	541	0.07%	0.008%
7	3.792	775	778	781	rVB	605	330	0.04%	0.005%
8	3.811	781	784	787	rVB3	525	345	0.05%	0.005%
9	3.843	787	794	795	rBV3	1030	933	0.13%	0.014%
10	3.923	815	819	822	rBV3	531	586	0.08%	0.009%
11	4.013	844	847	848	rBV	544	261	0.04%	0.004%
12	4.197	899	904	905	rBV2	412	360	0.05%	0.006%
13	4.431	973	977	979	rBV3	563	459	0.06%	0.007%
14	4.483	990	993	997	rVB3	624	388	0.05%	0.006%
15	4.618	1024	1035	1059	rBV2	78730	191094	25.99%	2.960%
16	5.055	1155	1171	1191	rBV	135190	301435	41.00%	4.669%
17	5.370	1266	1269	1270	rBV2	1367	798	0.11%	0.012%
18	5.428	1283	1287	1293	rVB5	639	661	0.09%	0.010%
19	5.470	1297	1300	1302	rBV2	450	330	0.04%	0.005%
20	5.515	1307	1314	1322	rBV6	1157	1551	0.21%	0.024%
21	5.718	1358	1377	1400	rBV2	267653	725182	98.63%	11.232%
22	5.962	1450	1453	1454	rBV	768	416	0.06%	0.006%
23	6.042	1476	1478	1480	rBV2	588	302	0.04%	0.005%
24	6.100	1494	1496	1499	rVB3	682	266	0.04%	0.004%
25	6.116	1499	1501	1503	rBV2	580	357	0.05%	0.006%
26	6.190	1521	1524	1526	rBV	429	260	0.04%	0.004%
27	6.242	1528	1540	1562	rVV	269713	515066	70.05%	7.978%
28	6.492	1614	1618	1620	rVB	462	312	0.04%	0.005%
29	6.521	1620	1627	1632	rBV6	2587	3894	0.53%	0.060%
30	6.631	1659	1661	1664	rBV2	510	347	0.05%	0.005%
31	6.685	1665	1678	1694	rBV	174461	343063	46.66%	5.314%
32	6.836	1722	1725	1727	rBV3	640	376	0.05%	0.006%
33	6.885	1736	1740	1743	rVB2	426	324	0.04%	0.005%
34	6.955	1757	1762	1764	rBV2	610	418	0.06%	0.006%
35	6.978	1767	1769	1772	rVB2	837	436	0.06%	0.007%
36	7.007	1772	1778	1780	rBV2	408	326	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
 Data File : VU054812.D
 Acq On : 18 Jul 2023 17:12
 Operator : MD/SY
 Sample : 03656-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

37	7.036	1784	1787	1789	rBV2	704	412	0.06%	0.006%
38	7.071	1796	1798	1803	rVB2	721	390	0.05%	0.006%
39	7.107	1805	1809	1812	rVV2	900	551	0.07%	0.009%
40	7.351	1880	1885	1888	rBV3	1221	1133	0.15%	0.018%
41	7.502	1929	1932	1935	rVB2	726	357	0.05%	0.006%
42	7.560	1938	1950	1974	rBV	100657	182848	24.87%	2.832%
43	7.698	1982	1993	2001	rBV8	2113	3453	0.47%	0.053%
44	7.762	2009	2013	2015	rBV3	747	501	0.07%	0.008%
45	7.894	2039	2054	2072	rBV	339972	591524	80.45%	9.162%
46	8.174	2131	2141	2163	rVV	71108	122907	16.72%	1.904%
47	8.338	2190	2192	2195	rBV2	602	372	0.05%	0.006%
48	8.396	2207	2210	2211	rBV2	846	433	0.06%	0.007%
49	8.422	2216	2218	2221	rBV2	607	342	0.05%	0.005%
50	8.518	2246	2248	2249	rBV	684	318	0.04%	0.005%
51	8.631	2272	2283	2316	rBV2	239165	452448	61.53%	7.008%
52	8.798	2332	2335	2342	rBV6	980	984	0.13%	0.015%
53	8.904	2363	2368	2369	rBV2	831	729	0.10%	0.011%
54	8.965	2385	2387	2390	rBV2	493	368	0.05%	0.006%
55	8.984	2390	2393	2395	rVV	408	276	0.04%	0.004%
56	9.023	2402	2405	2407	rBV2	422	281	0.04%	0.004%
57	9.116	2432	2434	2436	rBV	456	267	0.04%	0.004%
58	9.319	2491	2497	2498	rBV2	510	516	0.07%	0.008%
59	9.415	2514	2527	2545	rBV	390982	659055	89.63%	10.208%
60	9.544	2563	2567	2569	rBV2	790	641	0.09%	0.010%
61	9.569	2570	2575	2587	rVB6	2602	3668	0.50%	0.057%
62	9.695	2606	2614	2621	rBV7	2790	4379	0.60%	0.068%
63	9.775	2636	2639	2641	rBV2	409	321	0.04%	0.005%
64	9.907	2677	2680	2682	rVB3	830	440	0.06%	0.007%
65	9.981	2700	2703	2705	rBV2	410	284	0.04%	0.004%
66	10.081	2731	2734	2735	rBV2	620	277	0.04%	0.004%
67	10.113	2735	2744	2754	rVV7	3426	6526	0.89%	0.101%
68	10.312	2804	2806	2807	rBV2	762	383	0.05%	0.006%
69	10.360	2819	2821	2824	rBV2	329	237	0.03%	0.004%
70	10.454	2848	2850	2852	rBV2	467	251	0.03%	0.004%
71	10.489	2853	2861	2872	rVB7	6498	10710	1.46%	0.166%
72	10.676	2915	2919	2924	rBV3	686	589	0.08%	0.009%
73	10.704	2924	2928	2931	rBV2	432	376	0.05%	0.006%
74	10.753	2931	2943	2959	rBV	318122	513744	69.87%	7.957%
75	11.274	3103	3105	3107	rBV2	412	226	0.03%	0.004%
76	11.467	3157	3165	3166	rBV6	2041	2123	0.29%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
 Data File : VU054812.D
 Acq On : 18 Jul 2023 17:12
 Operator : MD/SY
 Sample : 03656-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

77	11.598	3203	3206	3207	rBV	811	452	0.06%	0.007%
78	11.640	3215	3219	3226	rBV2	629	676	0.09%	0.010%
79	11.714	3236	3242	3244	rBV2	820	728	0.10%	0.011%
80	11.743	3245	3251	3258	rVV8	2920	4291	0.58%	0.066%
81	11.807	3259	3271	3291	rVV	450913	735292	100.00%	11.389%
82	12.010	3328	3334	3339	rBV4	790	1018	0.14%	0.016%
83	12.190	3378	3390	3410	rBV	390511	632525	86.02%	9.797%
84	12.438	3458	3467	3469	rBV2	1291	1303	0.18%	0.020%
85	12.502	3483	3487	3488	rBV3	871	500	0.07%	0.008%
86	12.531	3489	3496	3507	rVV3	6387	10437	1.42%	0.162%
87	13.183	3696	3699	3700	rBV2	510	307	0.04%	0.005%
88	13.228	3707	3713	3717	rBV4	1587	1922	0.26%	0.030%
89	13.540	3804	3810	3813	rBV2	570	658	0.09%	0.010%
90	13.556	3813	3815	3821	rVV3	637	619	0.08%	0.010%
91	13.672	3848	3851	3854	rBV2	853	693	0.09%	0.011%
92	13.846	3899	3905	3907	rBV3	1638	1710	0.23%	0.026%
93	14.203	4014	4016	4017	rBV2	812	328	0.04%	0.005%
94	14.235	4024	4026	4028	rBV	846	556	0.08%	0.009%
95	14.296	4043	4045	4048	rBV	581	411	0.06%	0.006%
96	14.431	4081	4087	4088	rBV4	1284	1246	0.17%	0.019%
97	14.479	4096	4102	4116	rVB2	20334	31098	4.23%	0.482%
98	14.727	4175	4179	4181	rBV	831	592	0.08%	0.009%
99	14.778	4192	4195	4196	rBV2	616	343	0.05%	0.005%
100	15.190	4320	4323	4325	rBV	746	557	0.08%	0.009%




Sum of corrected areas: 6456359

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
Data File : VU054812.D
Acq On : 18 Jul 2023 17:12
Operator : MD/SY
Sample : 03656-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

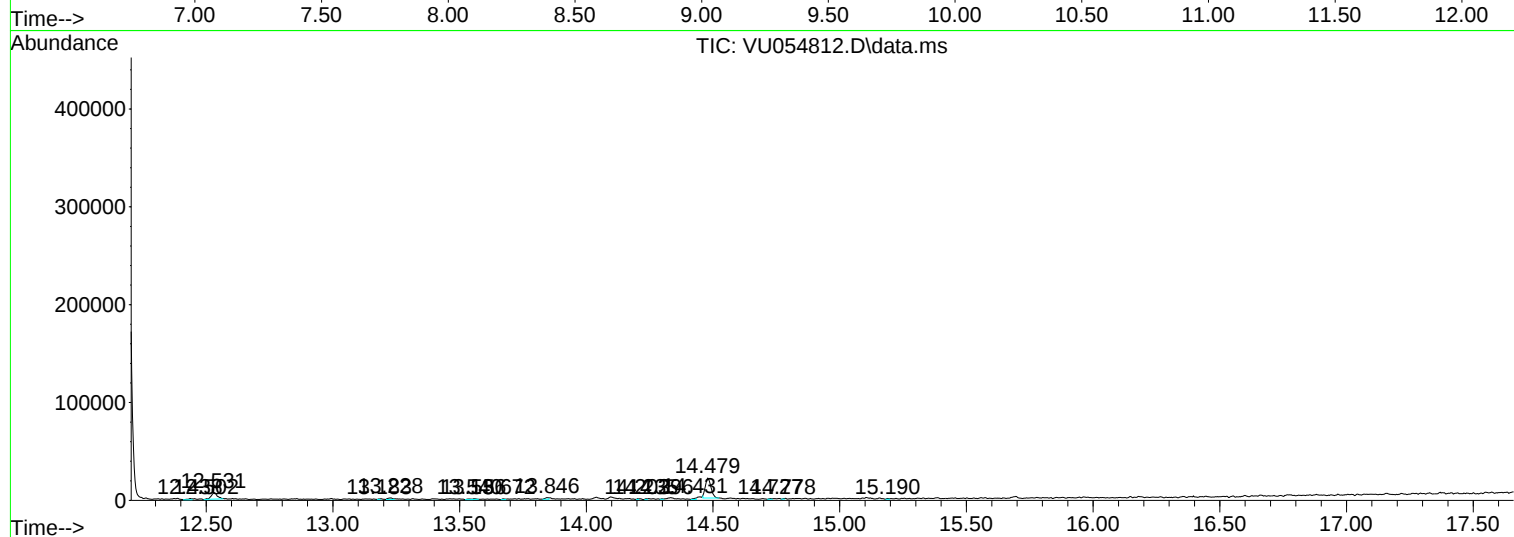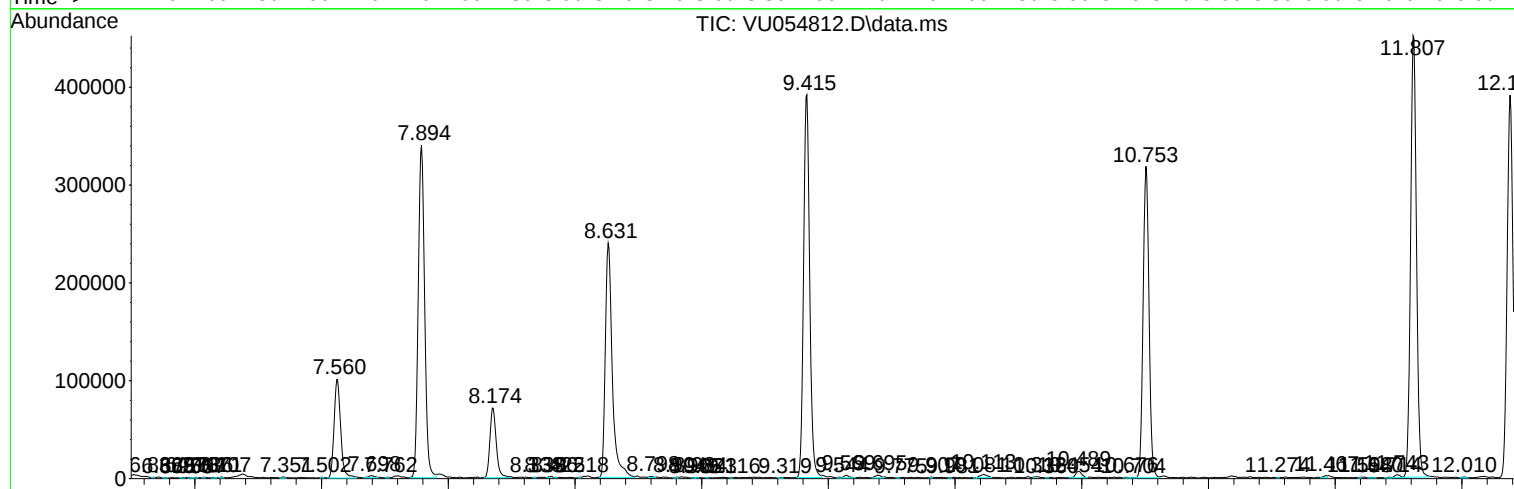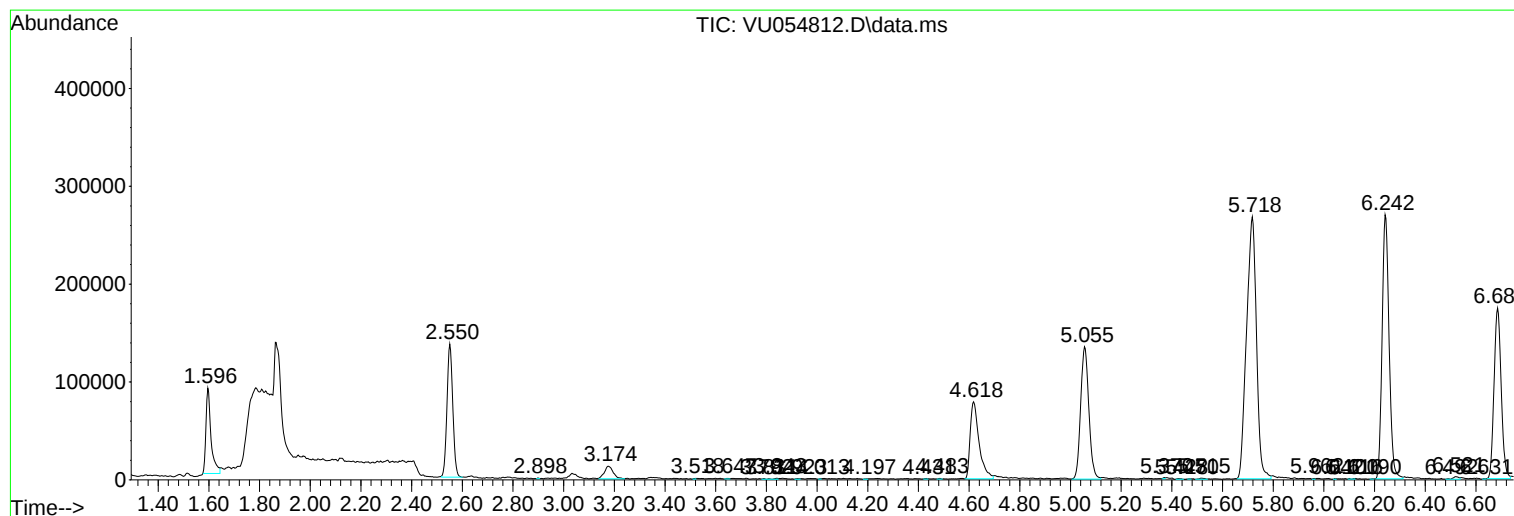

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
Data File : VU054812.D
Acq On : 18 Jul 2023 17:12
Operator : MD/SY
Sample : 03656-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
Data File : VU054812.D
Acq On : 18 Jul 2023 17:12
Operator : MD/SY
Sample : 03656-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------