


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071823\
Data File : VU054799.D
Acq On : 18 Jul 2023 08:29
Operator : MD/SY
Sample : BFB002
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB002

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Title : VOC Analysis
Last Update : Wed Jul 19 02:47:32 2023

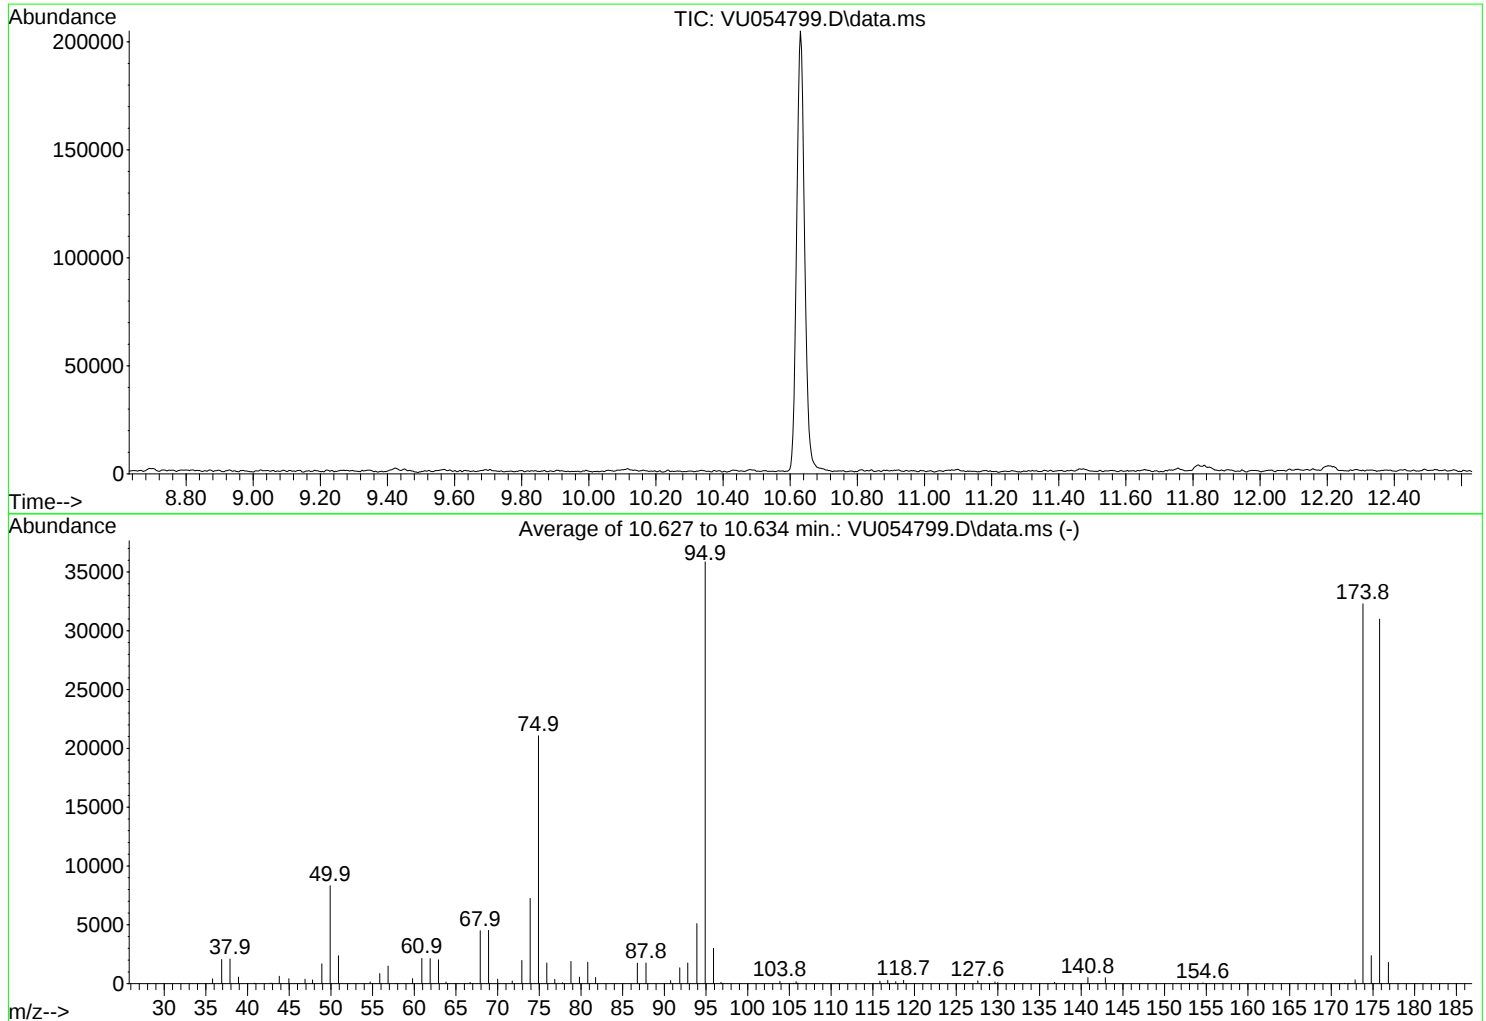

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2893

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.2	8329	PASS
75	95	30	80	58.8	21077	PASS
95	95	100	100	100.0	35861	PASS
96	95	5	9	8.4	3005	PASS
173	174	0.00	2	1.0	332	PASS
174	95	50	120	90.1	32301	PASS
175	174	5	9	7.4	2382	PASS
176	174	95	101	96.0	30995	PASS
177	176	5	9	5.9	1816	PASS

m/z	Abundance
38.80	178.0
39.70	192.0
40.80	215.0
41.80	189.0
42.80	100.0
43.80	345.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
35.80	357.0
36.90	1939.0
37.90	2145.0
38.90	697.0
39.70	184.0
40.80	256.0
42.90	150.0
43.90	919.0
44.90	411.0
46.80	423.0
47.80	258.0
48.90	1676.0
49.90	8241.0
50.90	2313.0
54.70	101.0
55.90	852.0
56.90	1534.0
59.80	392.0
60.90	2255.0
61.90	2086.0
62.90	2160.0
63.80	102.0
67.90	4634.0
68.90	4471.0
70.00	386.0
71.70	257.0
72.90	1908.0
73.90	7171.0
74.90	20720.0
75.90	1608.0
76.90	262.0
77.80	101.0
78.80	1892.0
79.80	566.0
80.80	1783.0
81.70	455.0
86.70	1737.0
87.80	1748.0
90.70	261.0
91.90	1330.0
92.80	1819.0
93.90	4937.0
94.90	35504.0
95.90	2891.0
103.80	202.0
105.80	201.0
115.80	158.0
116.80	250.0
117.70	199.0
118.70	298.0
127.60	220.0
129.70	175.0
136.80	123.0
140.80	500.0
142.90	497.0
153.00	125.0
172.80	352.0
173.80	31576.0
174.80	2275.0
175.80	29984.0
176.90	1845.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
35.80	411.0
36.90	2095.0
37.90	2151.0
39.00	767.0
39.80	145.0
40.80	257.0
42.80	151.0
43.90	975.0
45.00	424.0
46.90	375.0
47.80	345.0
48.90	1680.0
49.90	8613.0
50.90	2499.0
54.70	147.0
55.90	900.0
56.90	1525.0
59.80	459.0
60.90	2289.0
61.90	2219.0
62.90	2150.0
63.80	136.0
66.70	116.0
67.90	4640.0
68.90	4658.0
70.00	394.0
71.80	254.0
72.90	2009.0
73.90	7329.0
74.90	21744.0
75.90	1810.0
76.80	384.0
77.80	143.0
78.80	1932.0
79.80	589.0
80.80	1892.0
81.80	572.0
86.70	1789.0
87.80	1786.0
90.80	275.0
91.80	1376.0
92.80	1818.0
93.90	5196.0
94.90	37192.0
95.90	3119.0
96.80	132.0
103.80	201.0
105.60	141.0
105.90	180.0
115.80	219.0
116.80	300.0
117.80	183.0
118.70	284.0
127.60	267.0
129.60	155.0
130.00	142.0
136.80	129.0
140.80	535.0
142.90	504.0
154.60	115.0
172.80	336.0
173.80	33104.0
174.80	2464.0
175.80	32040.0
176.90	1811.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
35.80	460.0
36.90	2123.0
37.90	2001.0
39.00	760.0
39.80	129.0
40.80	241.0
42.80	182.0
43.80	1025.0
45.00	420.0
47.00	351.0
47.80	355.0
48.90	1724.0
49.90	8132.0
50.90	2292.0
54.70	205.0
55.80	817.0
56.80	1436.0
57.80	105.0
59.80	411.0
60.90	1921.0
61.90	2050.0
62.90	1763.0
63.80	154.0
66.70	201.0
67.90	4220.0
68.90	4449.0
70.00	367.0
71.80	194.0
72.90	1999.0
73.90	7253.0
74.90	20768.0
75.90	1860.0
76.80	455.0
78.80	1855.0
79.80	523.0
80.80	1792.0
81.80	539.0
86.80	1691.0
87.80	1746.0
90.80	228.0
91.80	1339.0
92.80	1612.0
93.90	5178.0
94.90	34888.0
95.90	3005.0
96.80	188.0
103.90	208.0
105.50	133.0
106.00	165.0
115.90	263.0
116.80	294.0
117.80	140.0
118.70	266.0
127.60	234.0
129.60	107.0
130.00	154.0
136.80	110.0
140.80	500.0
142.90	504.0
154.60	105.0
156.90	138.0
171.60	106.0
172.10	100.0
172.90	309.0
173.80	32224.0
174.80	2406.0
175.80	30960.0
176.80	1791.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002