




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060035.D
Acq On : 18 Jul 2024 22:22
Operator : MD/SY
Sample : P3237-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GA2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:39:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 01:30:22 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

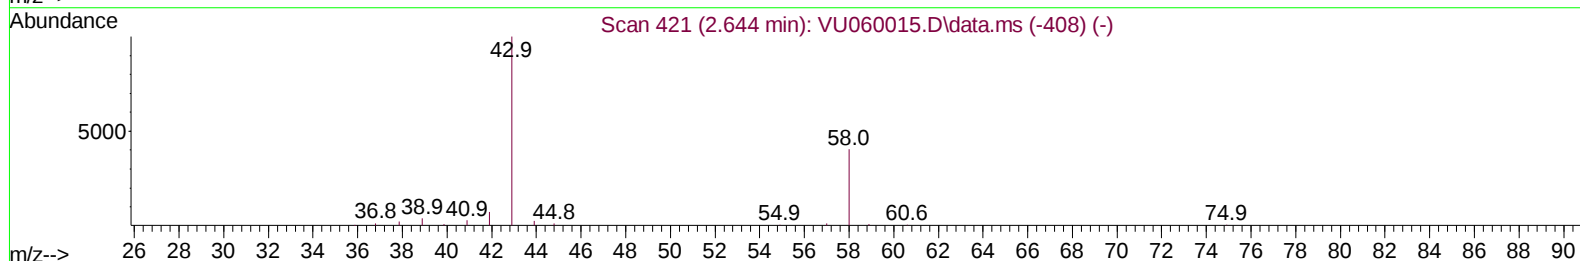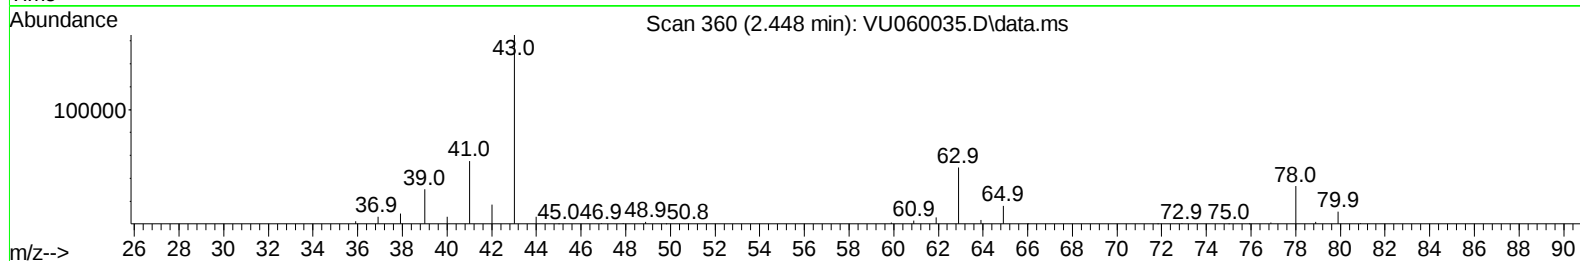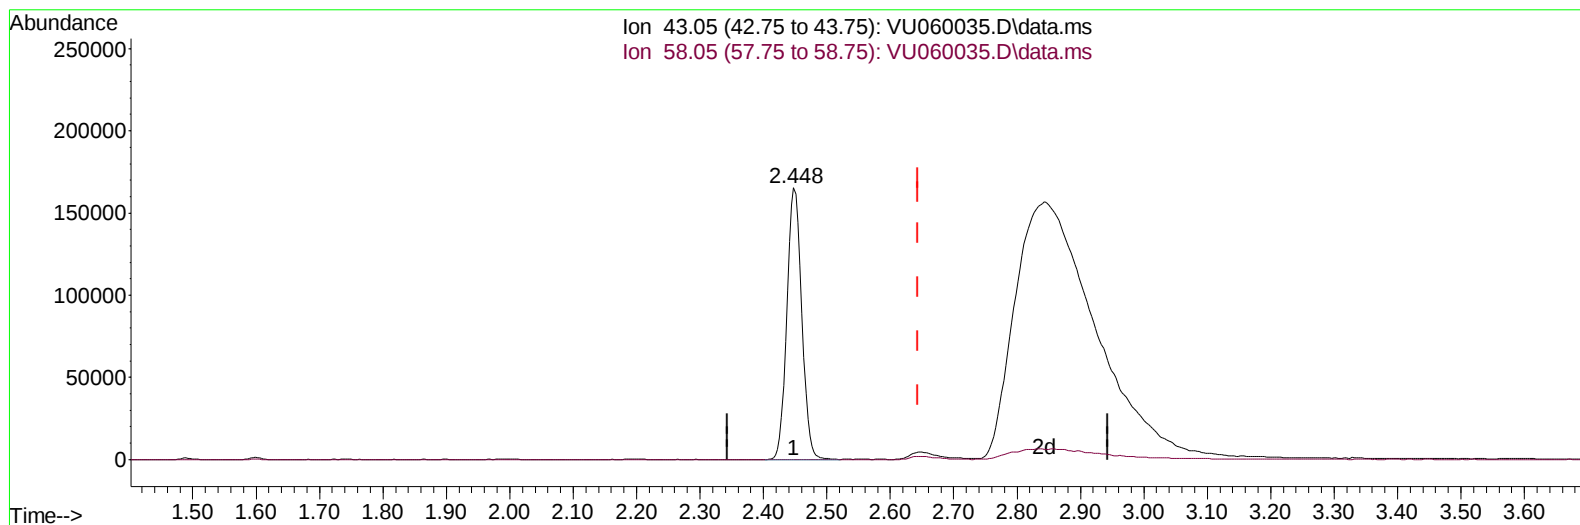

TIC: VU060035.D\data.ms

(13) Acetone (T)

2.448min (-0.196) 167.39 ug/L

response 269376

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	1.92
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060035.D
Acq On : 18 Jul 2024 22:22
Operator : MD/SY
Sample : P3237-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GA2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:39:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 01:30:22 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

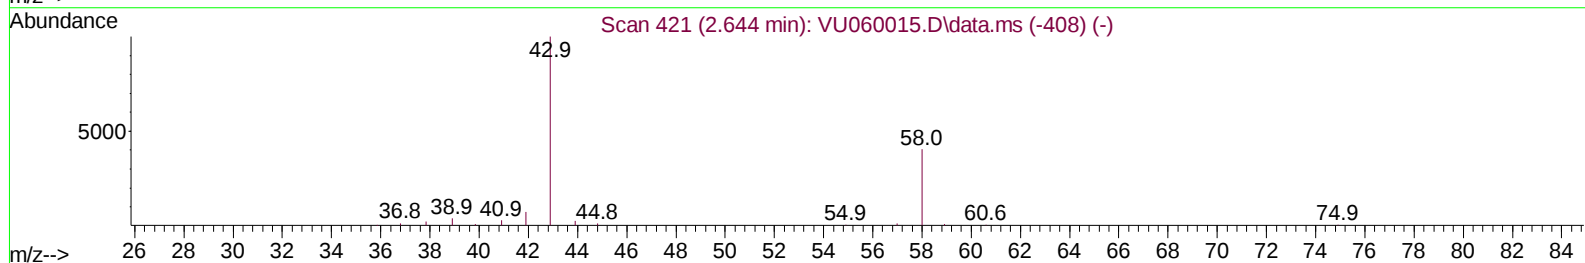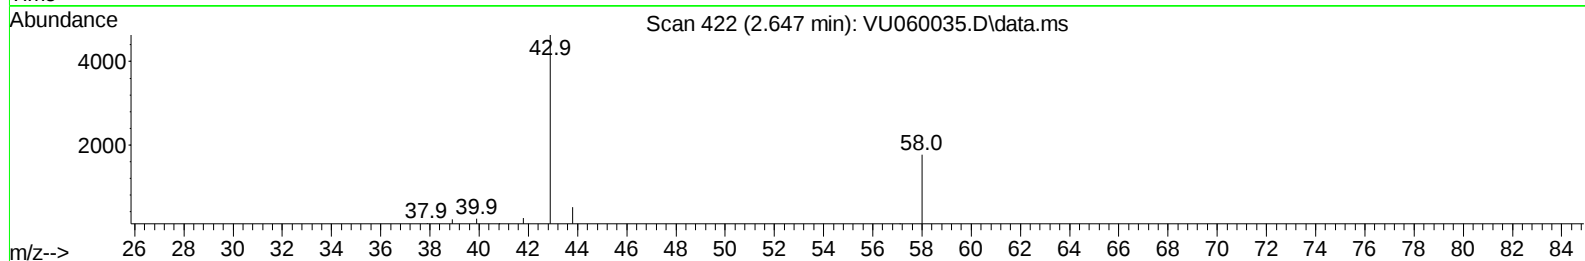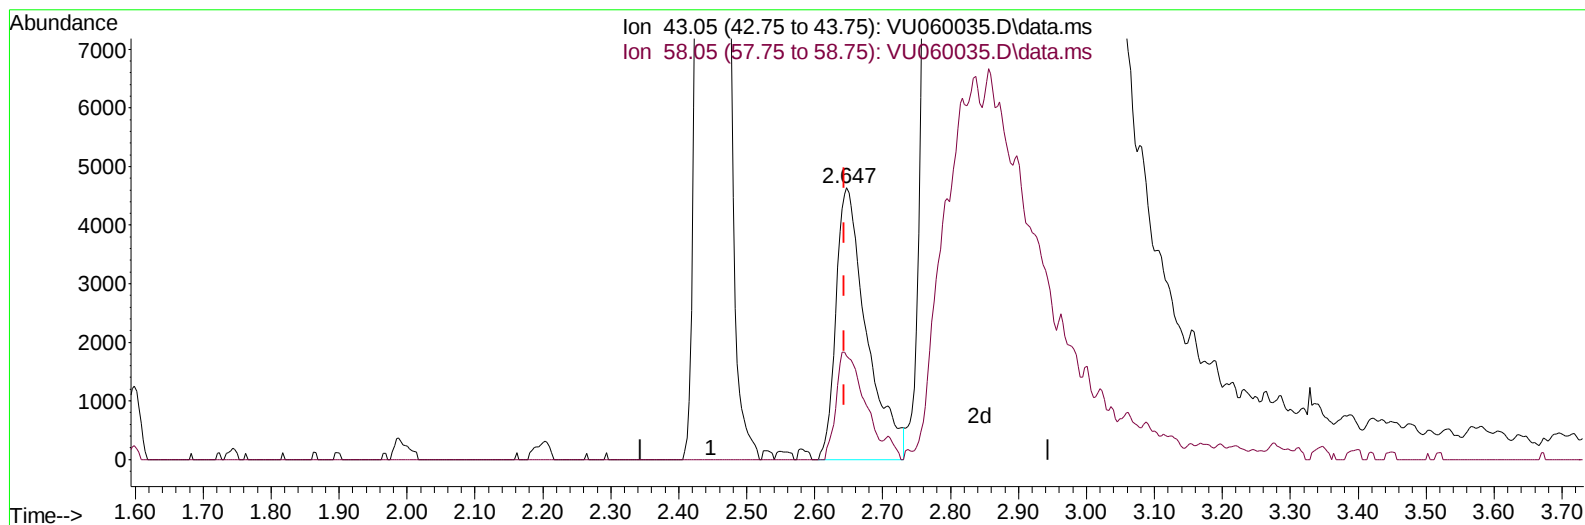

TIC: VU060035.D\data.ms

(13) Acetone (T)

2.647min (+ 0.003) 8.98 ug/L m

response 14454

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	35.78
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
 Data File : VU060035.D
 Acq On : 18 Jul 2024 22:22
 Operator : MD/SY
 Sample : P3237-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GA2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:39:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 19 01:30:22 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
 Supervised By :Semsettin Yesilyurt 07/24/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		149554	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		151847	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		71576	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		42952	4.128	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	82.600%	
7) Chloroethane-d5	1.911	69		42562	4.403	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	88.000%	
11) 1,1-Dichloroethene-d2	2.563	65		18329	4.512	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	90.200%	
20) 2-Butanone-d5	4.628	46		138674	57.003	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	114.000%	
24) Chloroform-d	5.055	84		94806	4.335	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	86.800%	
26) 1,2-Dichloroethane-d4	5.695	65		49433	4.855	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	97.000%	
32) Benzene-d6	5.721	84		193679	4.761	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	95.200%	
36) 1,2-Dichloropropane-d6	6.682	67		63945	4.933	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	98.600%	
41) Toluene-d8	7.891	98		163244	4.441	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	88.800%	
43) trans-1,3-Dichloroprop...	8.177	79		20676	4.685	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	93.800%	
46) 2-Hexanone-d5	8.627	63		109313	55.822	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	111.640%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		57051	4.945	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	98.800%	
66) 1,2-Dichlorobenzene-d4	12.187	152		66930	5.180	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	103.600%	
Target Compounds							
13) Acetone	2.647	43		14454m	8.982	ug/L	
16) Methylene chloride	3.039	84		2293	0.164	ug/L	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060035.D
Acq On : 18 Jul 2024 22:22
Operator : MD/SY
Sample : P3237-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GA2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:39:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 01:30:22 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

