




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060036.D
Acq On : 18 Jul 2024 22:46
Operator : MD/SY
Sample : P3237-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GA1

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:39:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 01:30:22 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

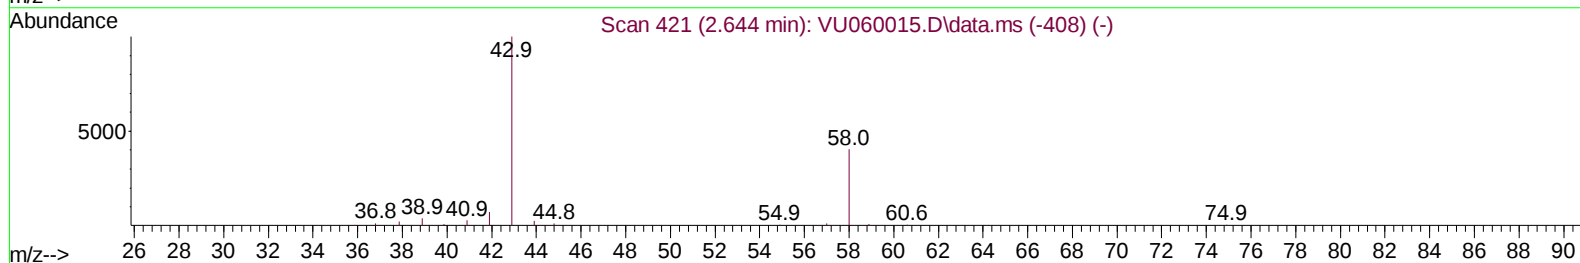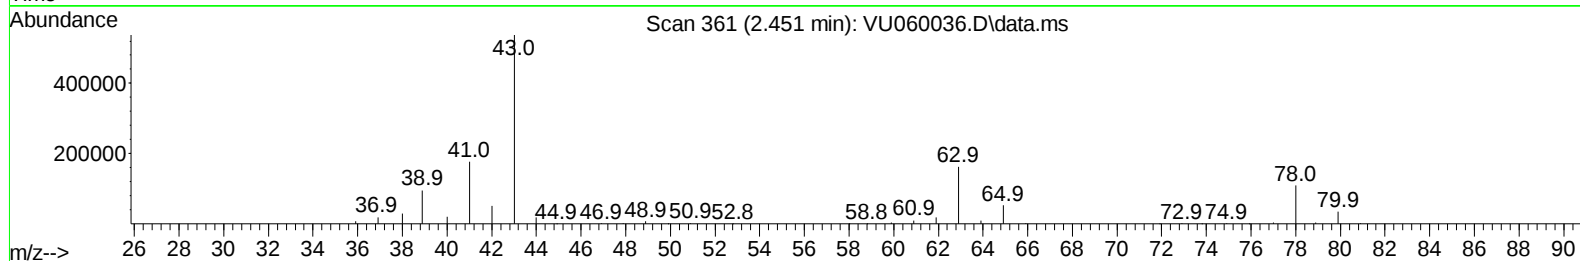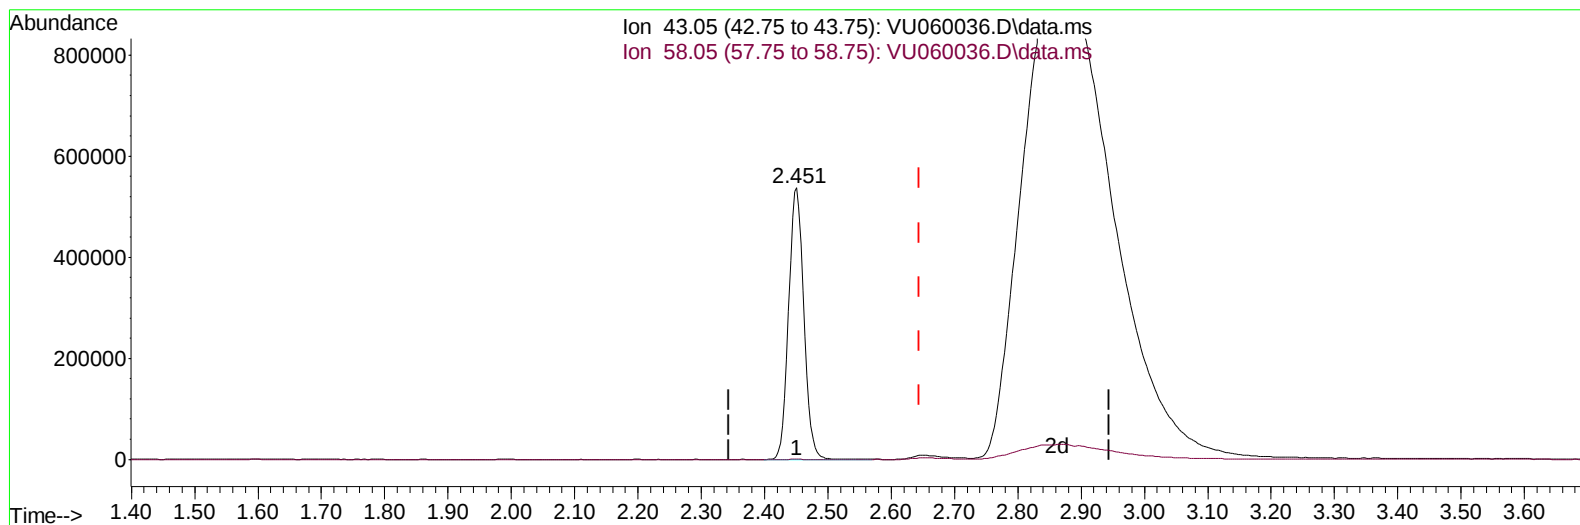

TIC: VU060036.D\data.ms

(13) Acetone (T)

2.451min (-0.193) 559.07 ug/L

response 893183

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	1.38
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060036.D
Acq On : 18 Jul 2024 22:46
Operator : MD/SY
Sample : P3237-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GA1

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:39:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 01:30:22 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

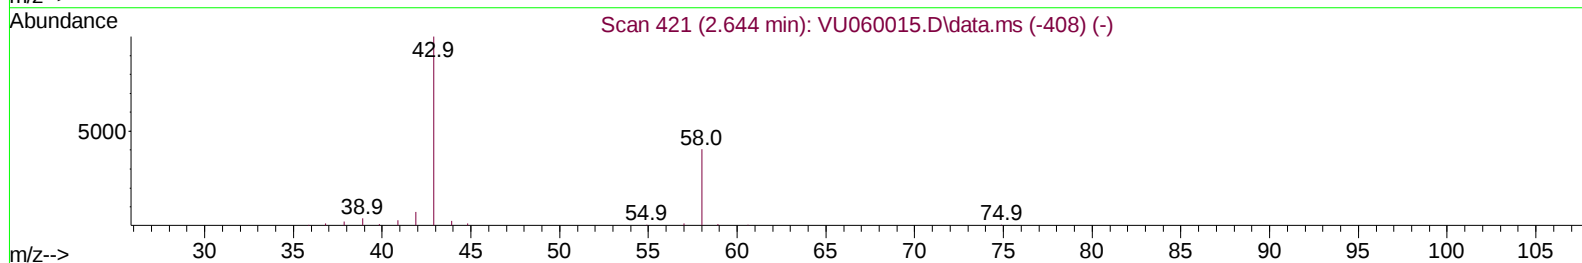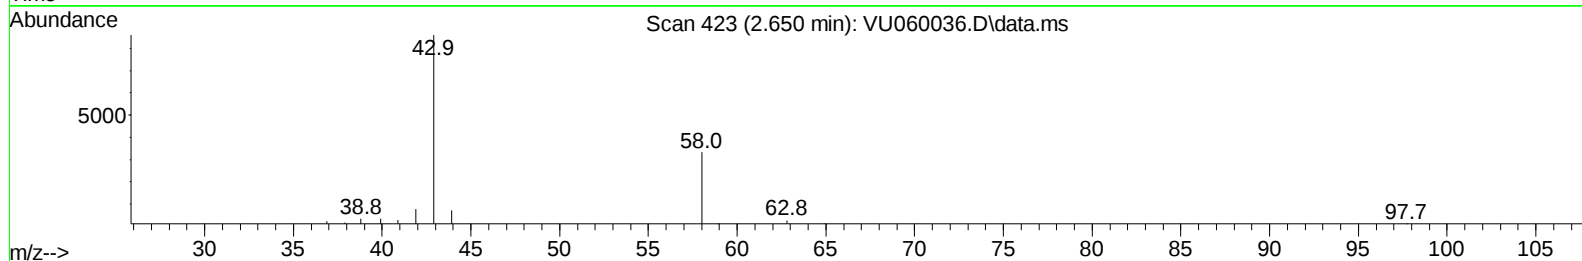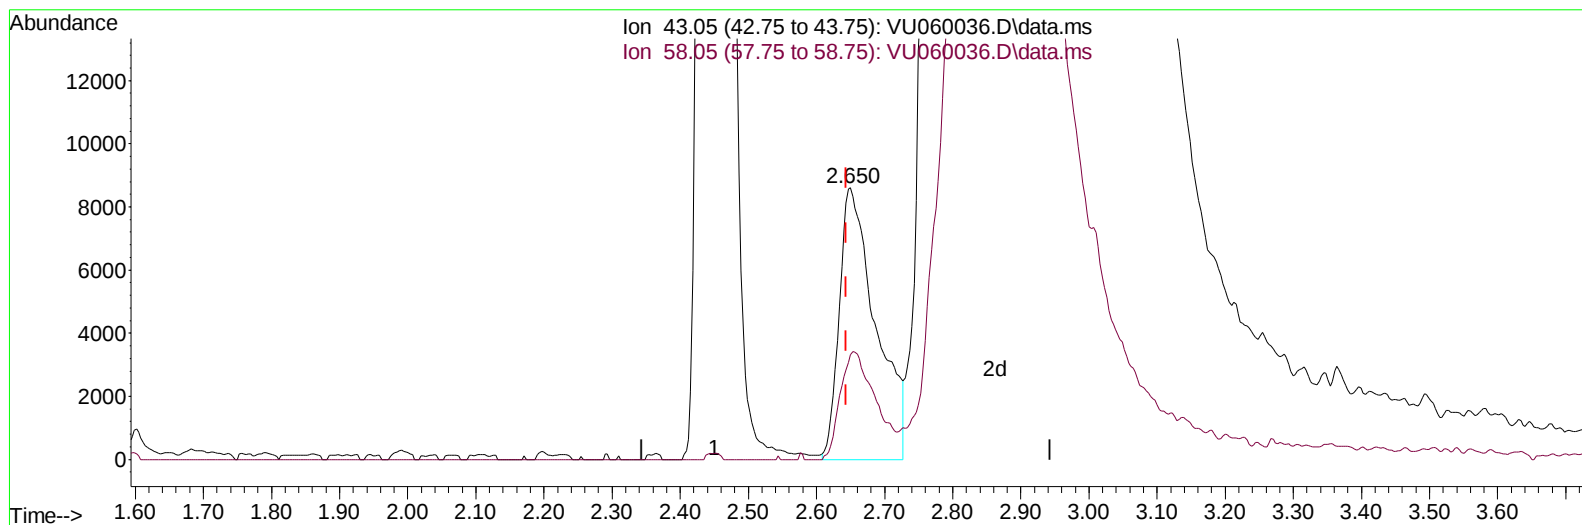

TIC: VU060036.D\data.ms

(13) Acetone (T)

2.650min (+ 0.006) 20.09 ug/L m

response 32104

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	38.30
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
 Data File : VU060036.D
 Acq On : 18 Jul 2024 22:46
 Operator : MD/SY
 Sample : P3237-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GA1

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:39:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 19 01:30:22 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
 Supervised By :Semsettin Yesilyurt 07/24/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		148475	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		150406	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		70589	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		43473	4.208	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	84.200%		
7) Chloroethane-d5	1.911	69		42423	4.420	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	88.400%		
11) 1,1-Dichloroethene-d2	2.563	65		17529	4.346	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	87.000%		
20) 2-Butanone-d5	4.631	46		139513	57.765	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	115.540%		
24) Chloroform-d	5.055	84		95239	4.387	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	87.800%		
26) 1,2-Dichloroethane-d4	5.695	65		49509	4.897	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	98.000%		
32) Benzene-d6	5.721	84		196486	4.876	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	97.600%		
36) 1,2-Dichloropropane-d6	6.682	67		62387	4.858	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	97.200%		
41) Toluene-d8	7.894	98		161362	4.432	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	88.600%		
43) trans-1,3-Dichloroprop...	8.177	79		21440	4.905	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	98.000%		
46) 2-Hexanone-d5	8.627	63		111007	57.230	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	114.460%		
56) 1,1,2,2-Tetrachloroeth...	10.749	84		56981	4.986	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	99.800%		
66) 1,2-Dichlorobenzene-d4	12.190	152		68507	5.377	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	107.600%		
Target Compounds							
13) Acetone	2.650	43		32104m	20.095	ug/L	
16) Methylene chloride	3.039	84		2078	0.150	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060036.D
Acq On : 18 Jul 2024 22:46
Operator : MD/SY
Sample : P3237-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GA1

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

Quant Time: Jul 19 01:39:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 01:30:22 2024
Response via : Initial Calibration

