




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
 Data File : VU060037.D
 Acq On : 18 Jul 2024 23:10
 Operator : MD/SY
 Sample : P3237-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GD0

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:40:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 19 01:30:22 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
 Supervised By :Semsettin Yesilyurt 07/24/2024

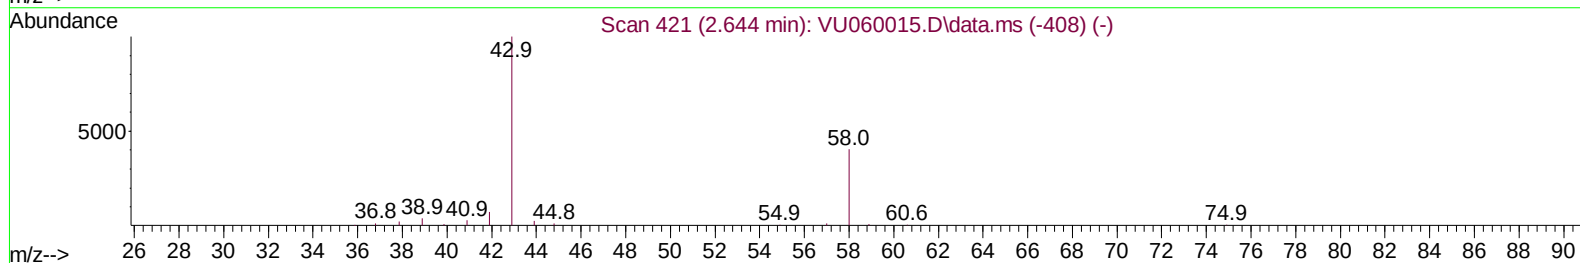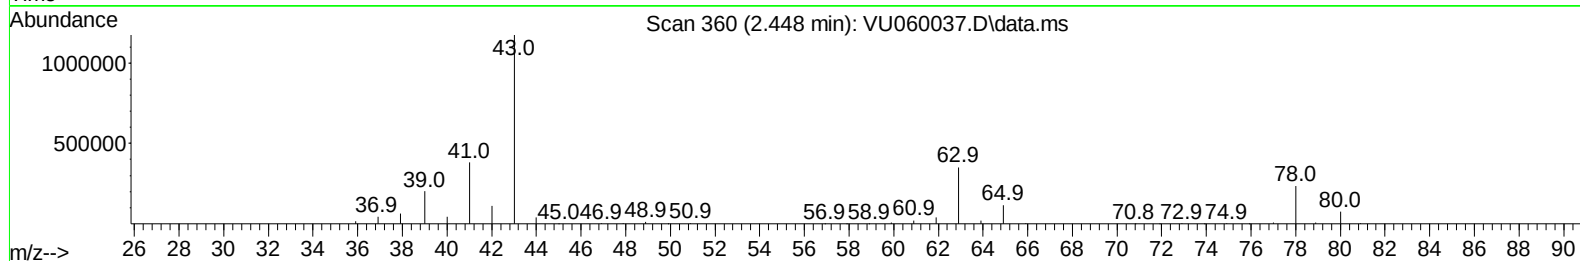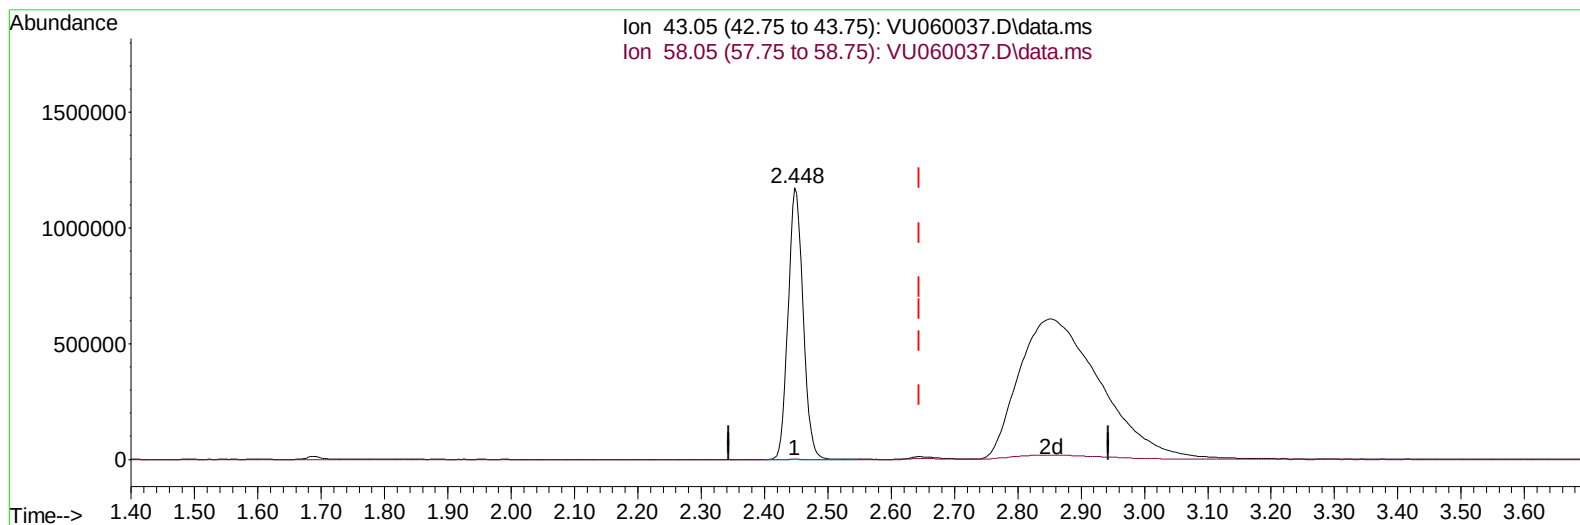

TIC: VU060037.D\data.ms

(13) Acetone (T)

2.448min (-0.196) 1165.84 ug/L

response 1932833

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	0.82
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
 Data File : VU060037.D
 Acq On : 18 Jul 2024 23:10
 Operator : MD/SY
 Sample : P3237-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GD0

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:40:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 19 01:30:22 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
 Supervised By :Semsettin Yesilyurt 07/24/2024

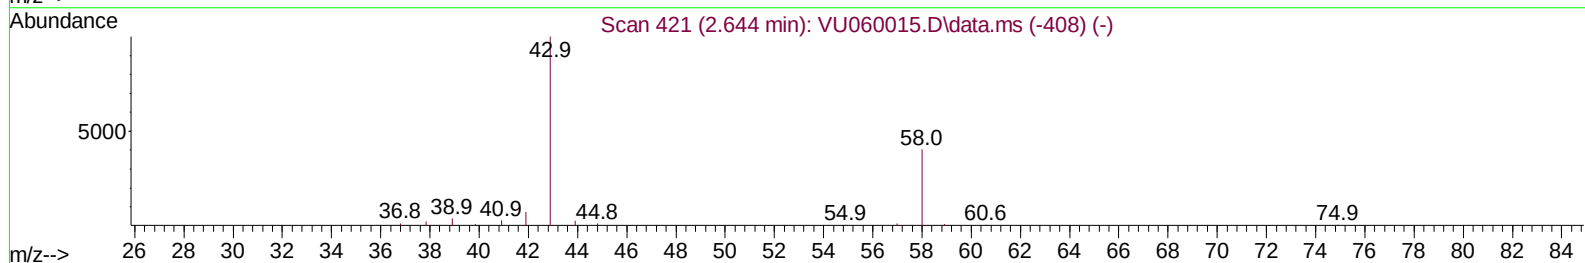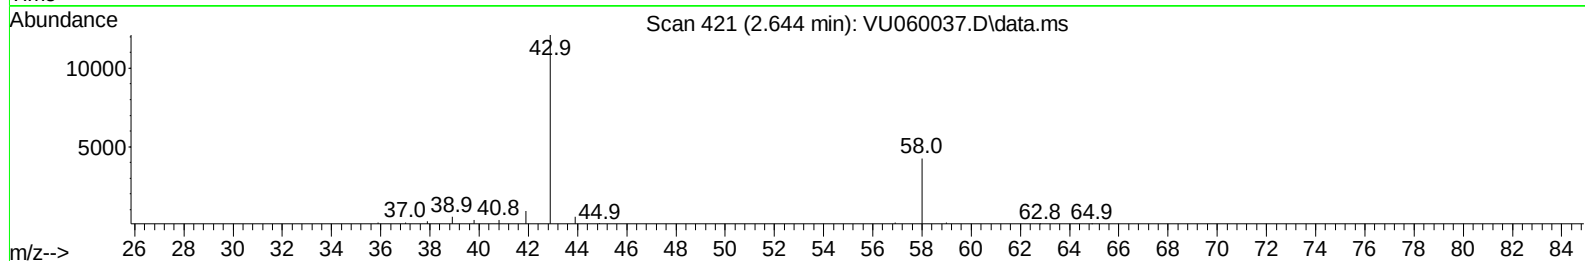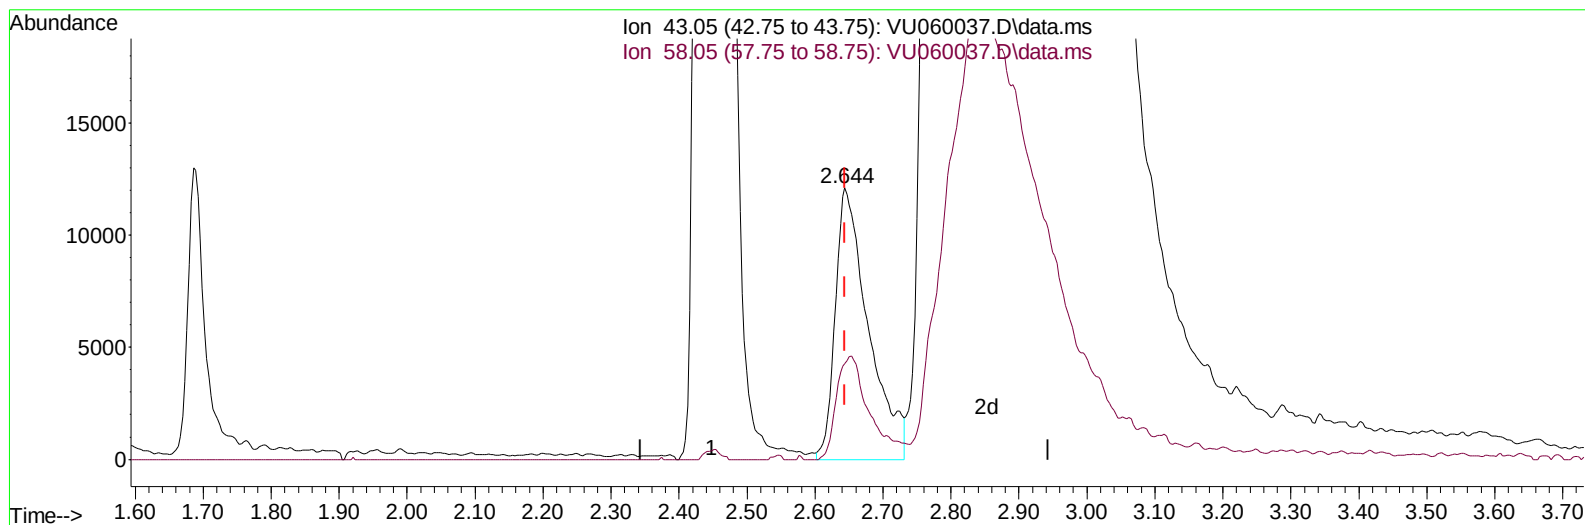

TIC: VU060037.D\data.ms

(13) Acetone (T)

2.644min (+ 0.000) 24.70 ug/L m

response 40954

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	38.69
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
 Data File : VU060037.D
 Acq On : 18 Jul 2024 23:10
 Operator : MD/SY
 Sample : P3237-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GD0

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:40:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 19 01:30:22 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
 Supervised By :Semsettin Yesilyurt 07/24/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		154074	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		158383	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.808	152		75568	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		45372	4.232	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	84.600%	
7) Chloroethane-d5	1.911	69		44449	4.463	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	89.200%	
11) 1,1-Dichloroethene-d2	2.560	65		19143	4.574	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	91.400%	
20) 2-Butanone-d5	4.628	46		144060	57.480	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	114.960%	
24) Chloroform-d	5.055	84		100300	4.452	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	89.000%	
26) 1,2-Dichloroethane-d4	5.695	65		51089	4.870	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	97.400%	
32) Benzene-d6	5.721	84		202632	4.775	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	95.600%	
36) 1,2-Dichloropropane-d6	6.682	67		66477	4.916	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	98.400%	
41) Toluene-d8	7.891	98		173611	4.528	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	90.600%	
43) trans-1,3-Dichloroprop...	8.177	79		20937	4.549	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	91.000%	
46) 2-Hexanone-d5	8.628	63		111122	54.404	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	108.800%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		58788	4.885	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	97.600%	
66) 1,2-Dichlorobenzene-d4	12.187	152		72571	5.320	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	106.400%	
Target Compounds							
13) Acetone	2.644	43		40954m	24.703	ug/L	
16) Methylene chloride	3.036	84		2981	0.207	ug/L	91
63) 1,2,4-Trimethylbenzene	11.464	105		6330	0.173	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060037.D
Acq On : 18 Jul 2024 23:10
Operator : MD/SY
Sample : P3237-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GD0

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:40:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 01:30:22 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

