




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060039.D
Acq On : 18 Jul 2024 23:58
Operator : MD/SY
Sample : P3237-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE5

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:40:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 01:30:22 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

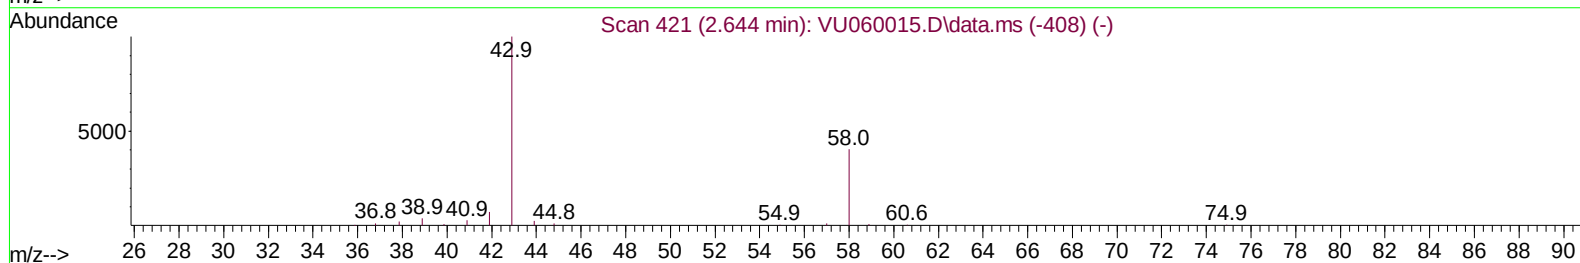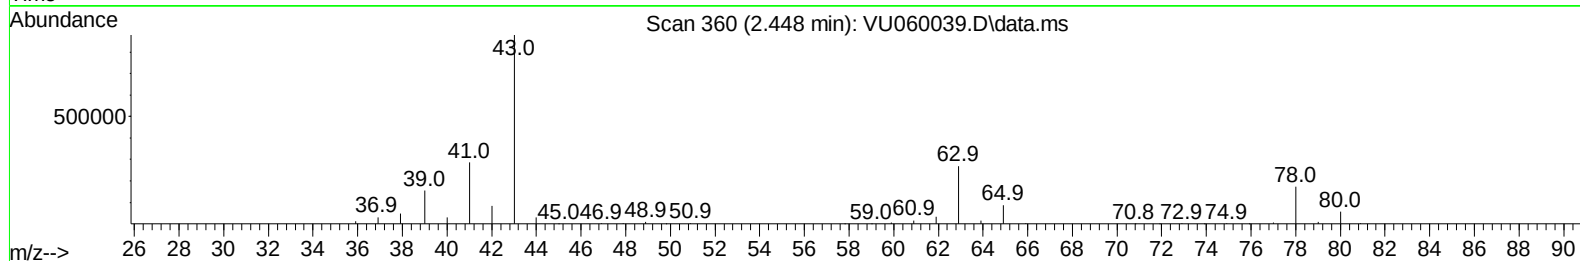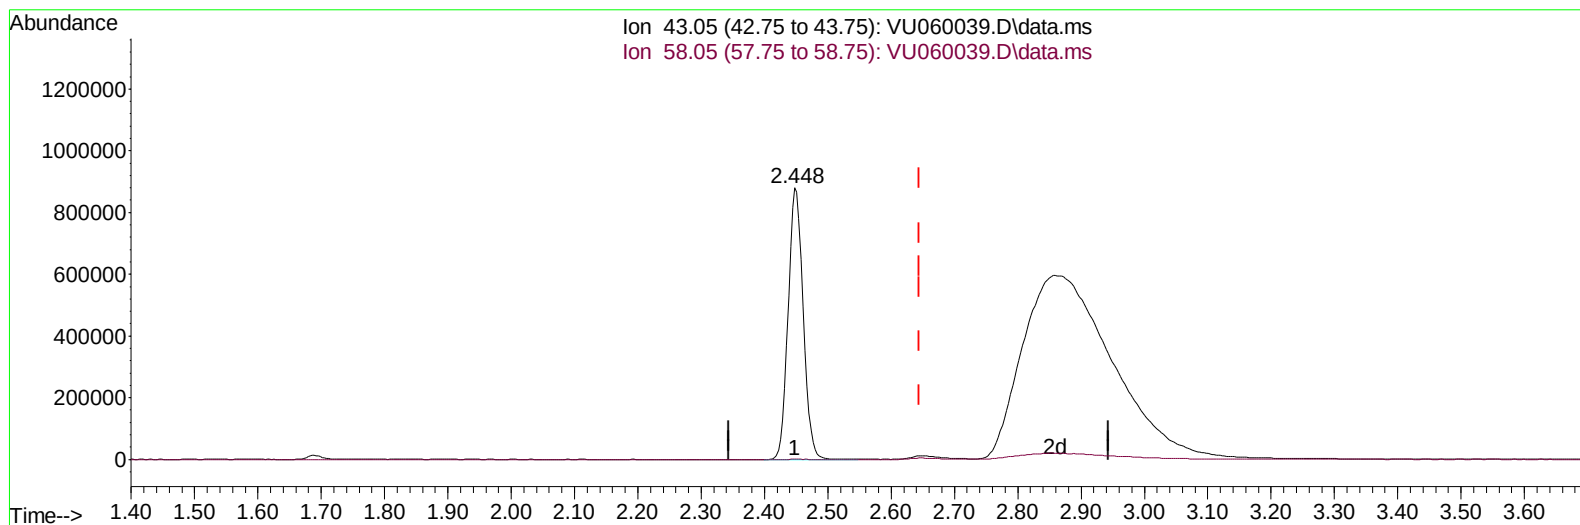

TIC: VU060039.D\data.ms

(13) Acetone (T)

2.448min (-0.196) 737.40 ug/L

response 1451401

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	1.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060039.D
Acq On : 18 Jul 2024 23:58
Operator : MD/SY
Sample : P3237-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE5

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:40:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 01:30:22 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

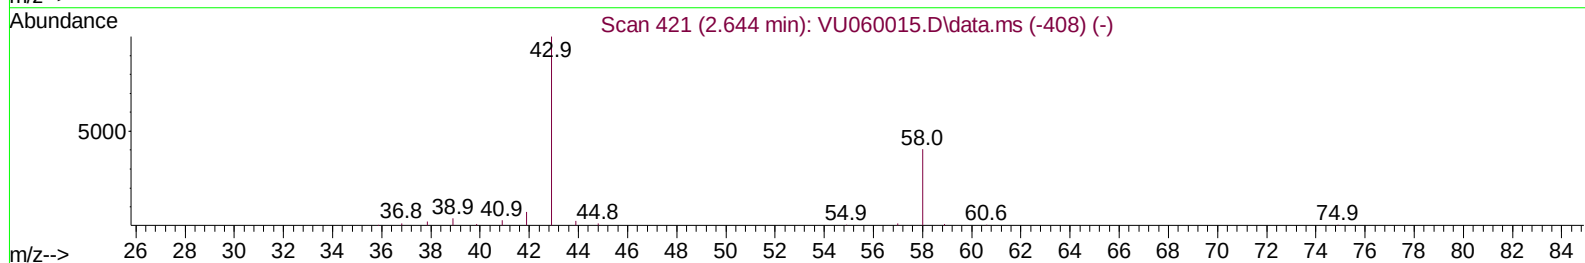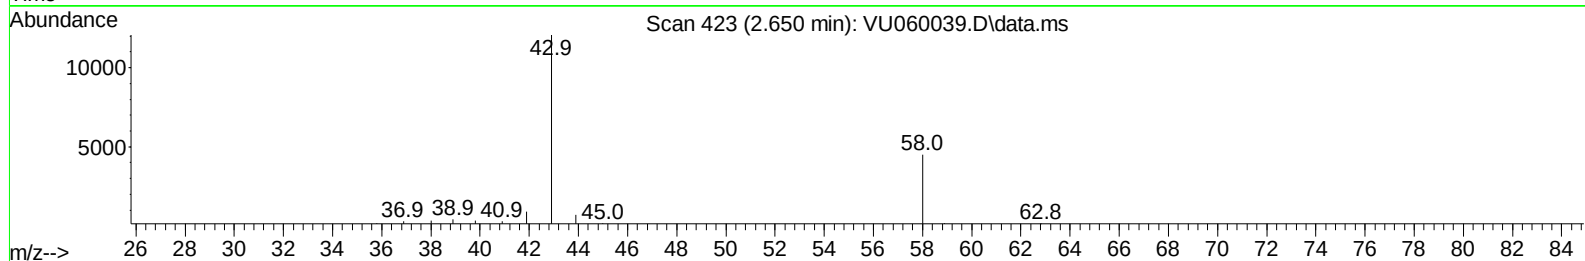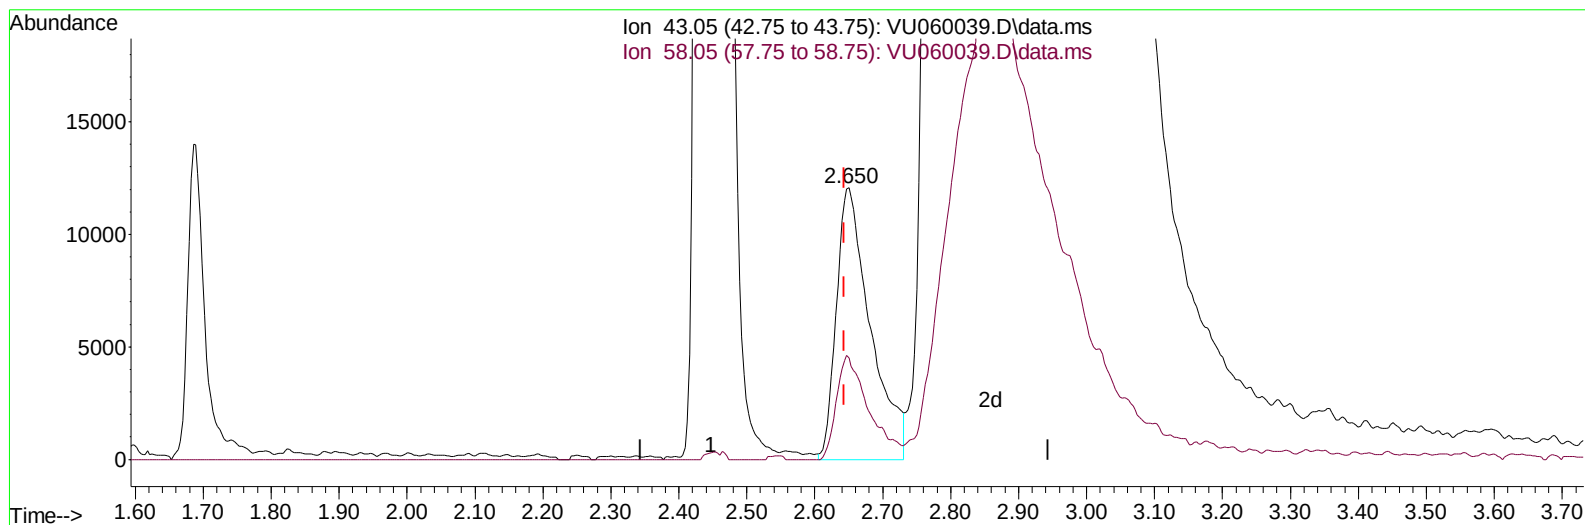

TIC: VU060039.D\data.ms

(13) Acetone (T)

2.650min (+ 0.006) 21.28 ug/L m

response 41877

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	36.27
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
 Data File : VU060039.D
 Acq On : 18 Jul 2024 23:58
 Operator : MD/SY
 Sample : P3237-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GE5

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:40:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 19 01:30:22 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
 Supervised By :Semsettin Yesilyurt 07/24/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		182919	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		186103	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		85871	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		42981	3.377	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.600%	
7) Chloroethane-d5	1.911	69		41847	3.539	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	70.800%	
11) 1,1-Dichloroethene-d2	2.563	65		17634	3.549	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.000%	
20) 2-Butanone-d5	4.631	46		135135	45.416	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.840%	
24) Chloroform-d	5.055	84		94506	3.533	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	70.600%	
26) 1,2-Dichloroethane-d4	5.695	65		46996	3.773	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.400%	
32) Benzene-d6	5.721	84		189962	3.810	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.200%	
36) 1,2-Dichloropropane-d6	6.682	67		63005	3.965	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.400%	
41) Toluene-d8	7.894	98		162099	3.598	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.000%	
43) trans-1,3-Dichloroprop...	8.177	79		20024	3.702	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.000%	
46) 2-Hexanone-d5	8.628	63		105564	43.985	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.960%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		56458	3.993	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.800%	
66) 1,2-Dichlorobenzene-d4	12.187	152		66933	4.318	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.400%	
Target Compounds							
13) Acetone	2.650	43		41877m	21.276	ug/L	
16) Methylene chloride	3.039	84		3019	0.176	ug/L	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060039.D
Acq On : 18 Jul 2024 23:58
Operator : MD/SY
Sample : P3237-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE5

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:40:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 01:30:22 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

