




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060046.D
Acq On : 19 Jul 2024 09:07
Operator : MD/SY
Sample : P3237-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GD1

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:55:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 02:49:52 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

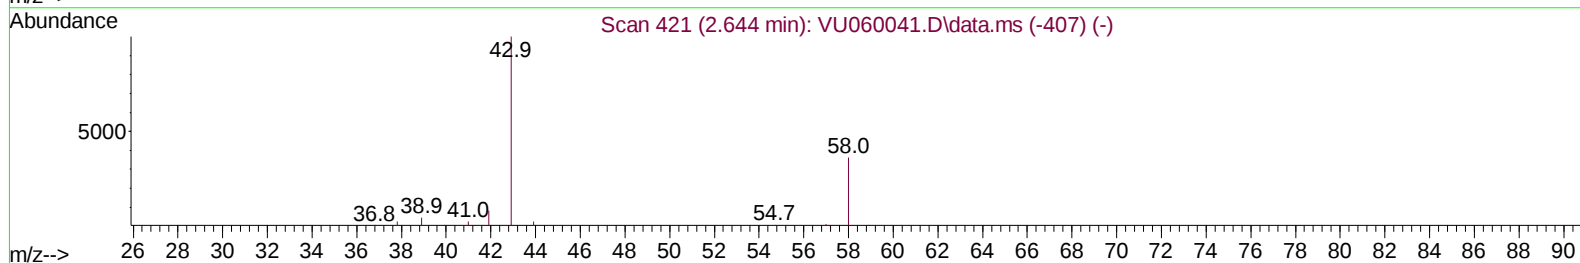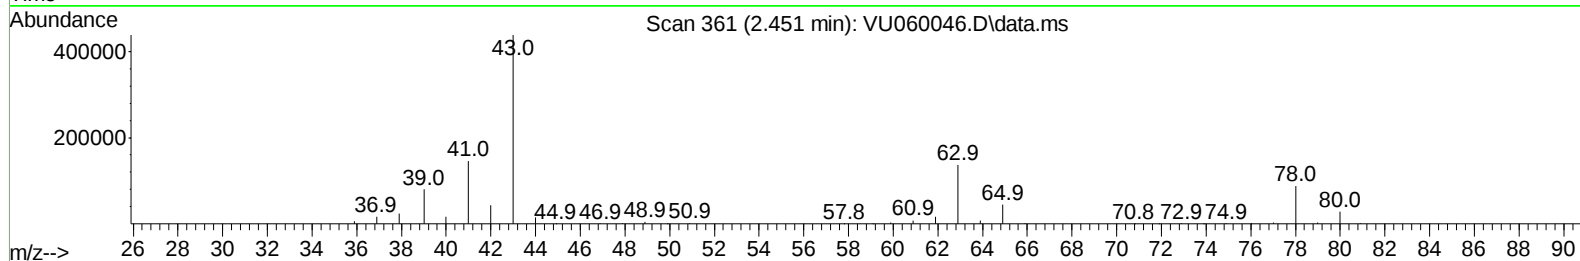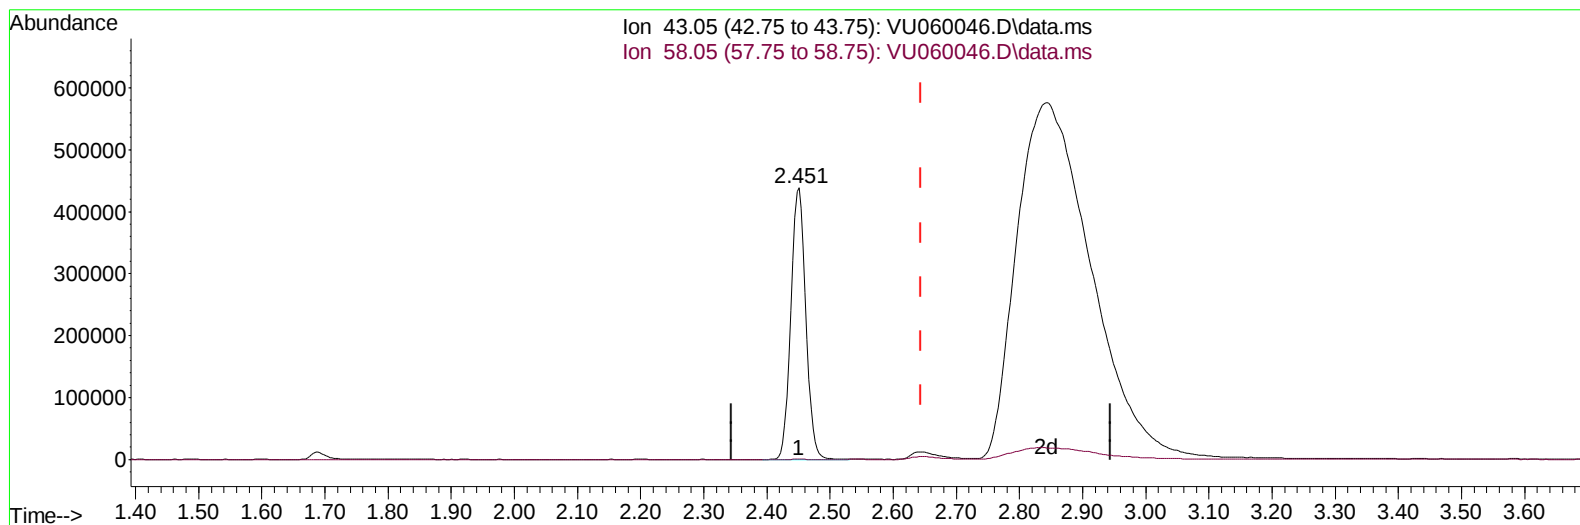

TIC: VU060046.D\data.ms

(13) Acetone (T)

2.451min (-0.193) 435.51 ug/L

response 720886

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	2.14
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060046.D
Acq On : 19 Jul 2024 09:07
Operator : MD/SY
Sample : P3237-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GD1

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

Quant Time: Jul 20 00:55:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 02:49:52 2024
Response via : Initial Calibration

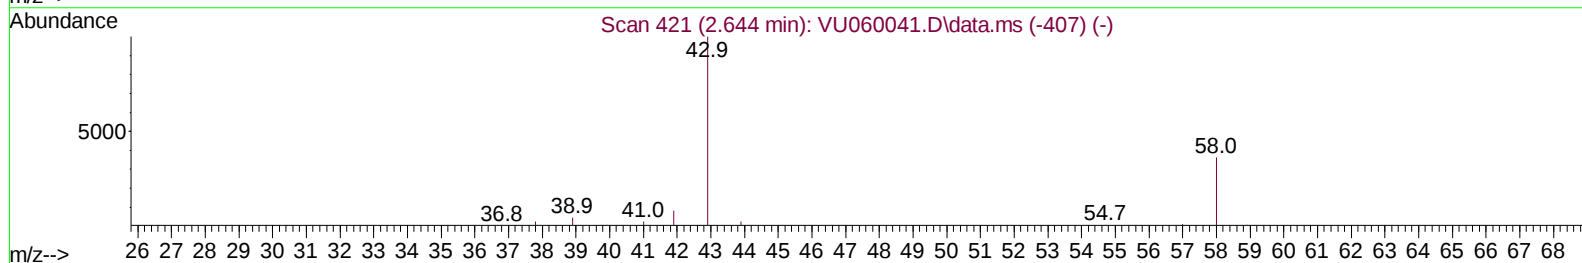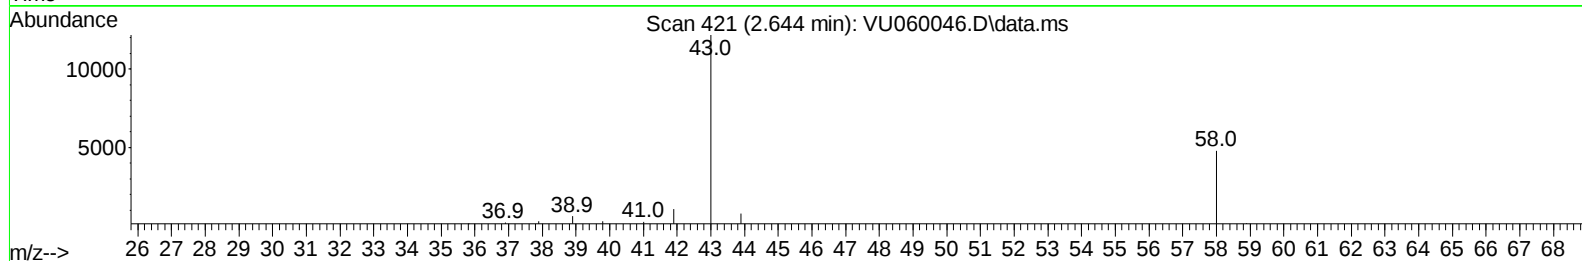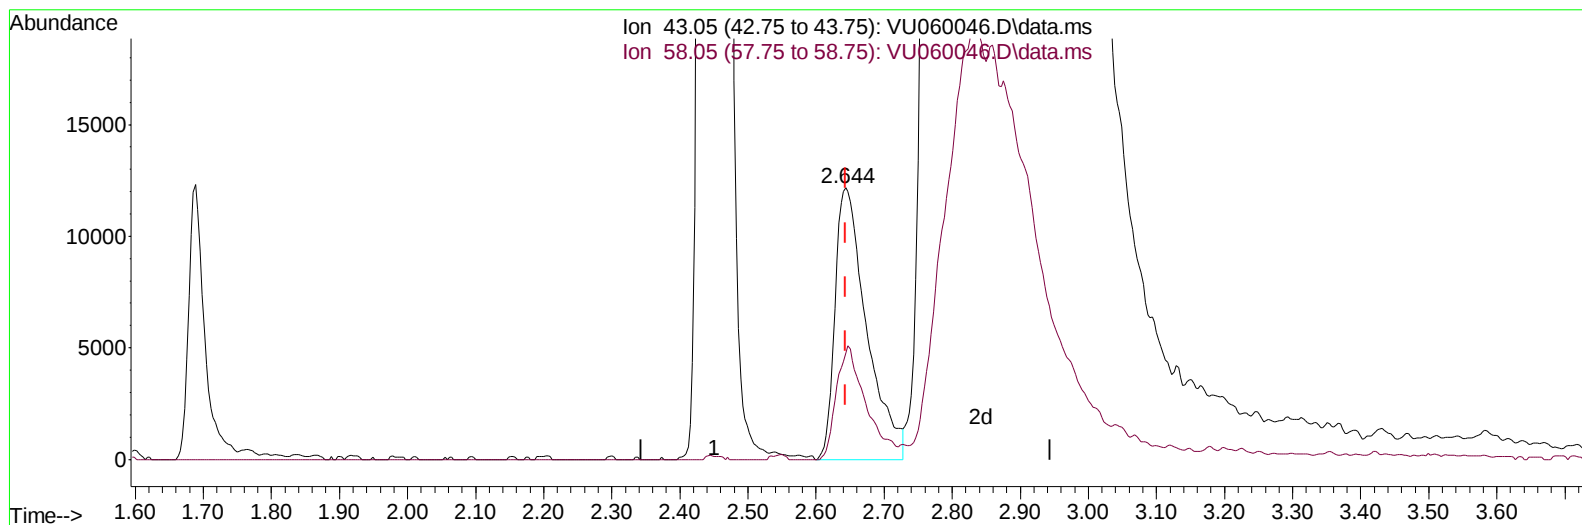

TIC: VU060046.D\data.ms

(13) Acetone (T)

2.644min (-0.000) 23.68 ug/L m

response 39201

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	39.34
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
 Data File : VU060046.D
 Acq On : 19 Jul 2024 09:07
 Operator : MD/SY
 Sample : P3237-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GD1

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:55:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 19 02:49:52 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
 Supervised By :Semsettin Yesilyurt 07/24/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.241	114		153831	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		154195	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		73171	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		39630	3.703	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.000%	
7) Chloroethane-d5	1.910	69		39080	3.930	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.600%	
11) 1,1-Dichloroethene-d2	2.560	65		16520	3.953	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.000%	
20) 2-Butanone-d5	4.627	46		112560	44.983	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.960%	
24) Chloroform-d	5.055	84		89897	3.996	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.000%	
26) 1,2-Dichloroethane-d4	5.698	65		45080	4.304	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.000%	
32) Benzene-d6	5.721	84		182787	4.424	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.400%	
36) 1,2-Dichloropropane-d6	6.685	67		57484	4.367	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.400%	
41) Toluene-d8	7.894	98		153746	4.119	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.400%	
43) trans-1,3-Dichloroprop...	8.177	79		17806	3.974	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.400%	
46) 2-Hexanone-d5	8.627	63		87485	43.995	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.980%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		50620	4.320	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.400%	
66) 1,2-Dichlorobenzene-d4	12.187	152		63485	4.807	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.200%	
Target Compounds							
13) Acetone	2.644	43		39201m	23.683	ug/L	
16) Methylene chloride	3.036	84		2520	0.175	ug/L	95
63) 1,2,4-Trimethylbenzene	11.466	105		5839	0.165	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060046.D
Acq On : 19 Jul 2024 09:07
Operator : MD/SY
Sample : P3237-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GD1

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

Quant Time: Jul 20 00:55:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 02:49:52 2024
Response via : Initial Calibration

