




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060049.D
Acq On : 19 Jul 2024 10:17
Operator : MD/SY
Sample : P3237-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB7

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:56:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 02:49:52 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

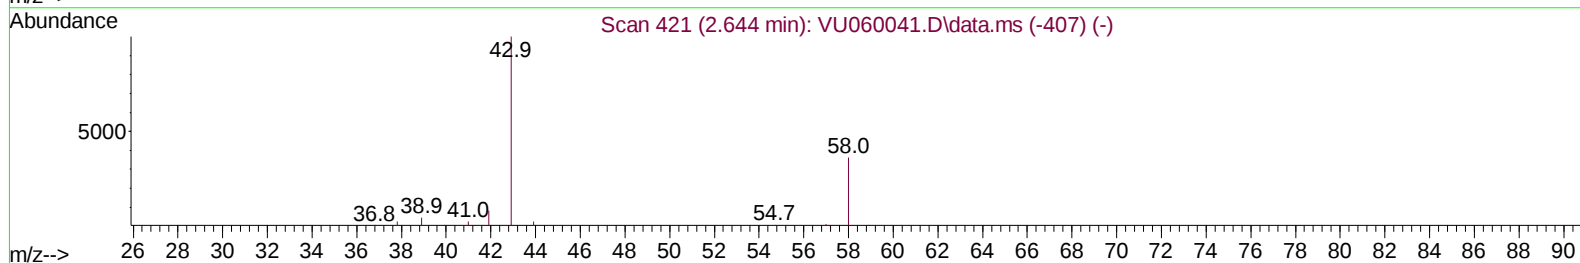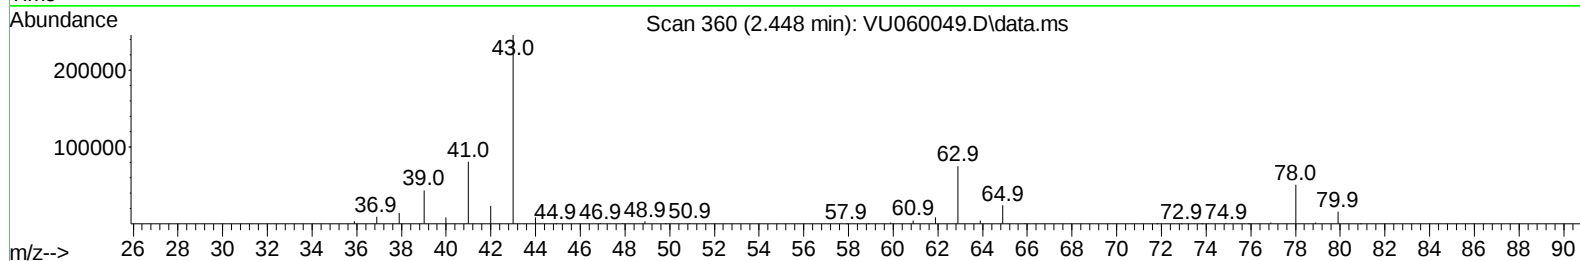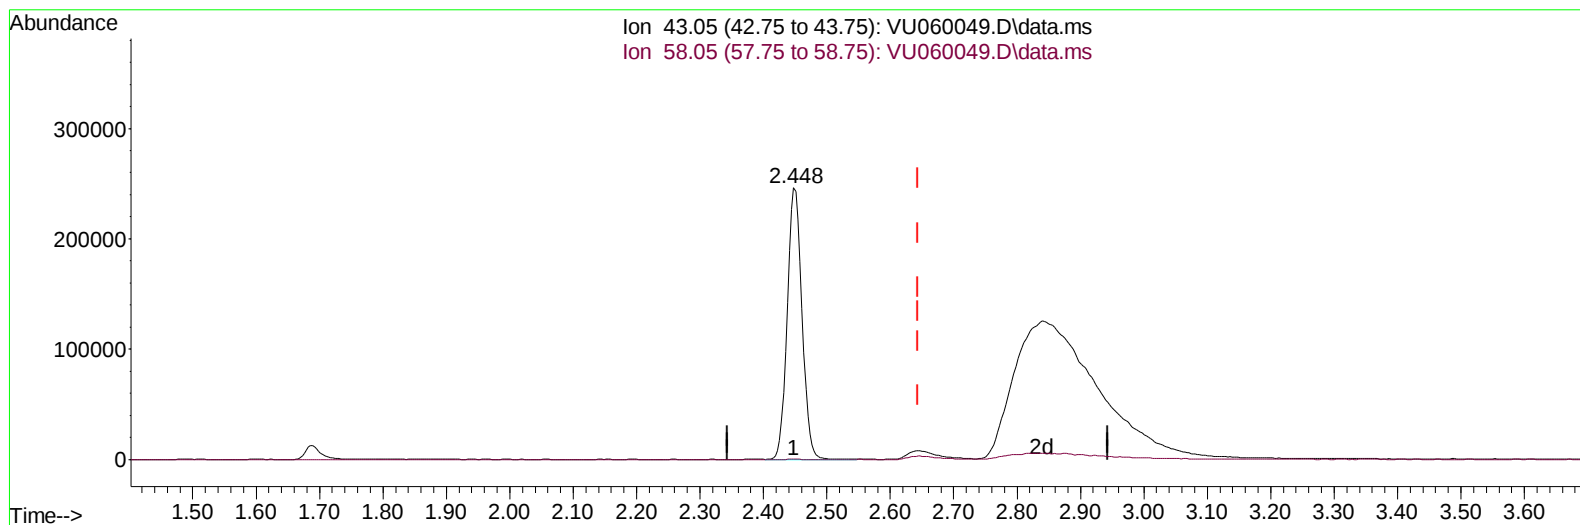

TIC: VU060049.D\data.ms

(13) Acetone (T)

2.448min (-0.196) 259.46 ug/L

response 398367

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	2.47
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060049.D
Acq On : 19 Jul 2024 10:17
Operator : MD/SY
Sample : P3237-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB7

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

Quant Time: Jul 20 00:56:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 02:49:52 2024
Response via : Initial Calibration

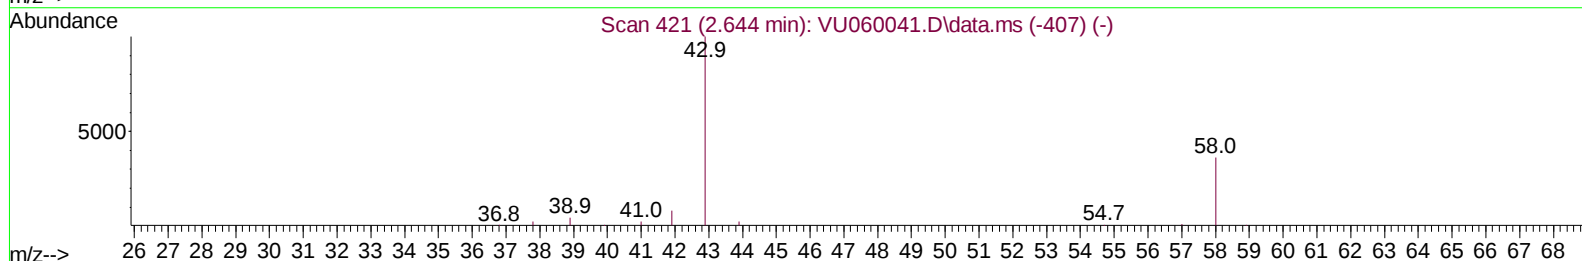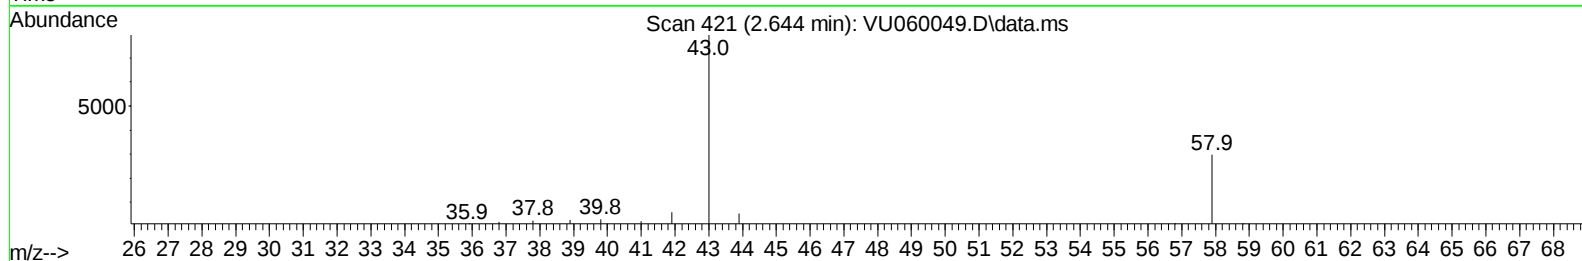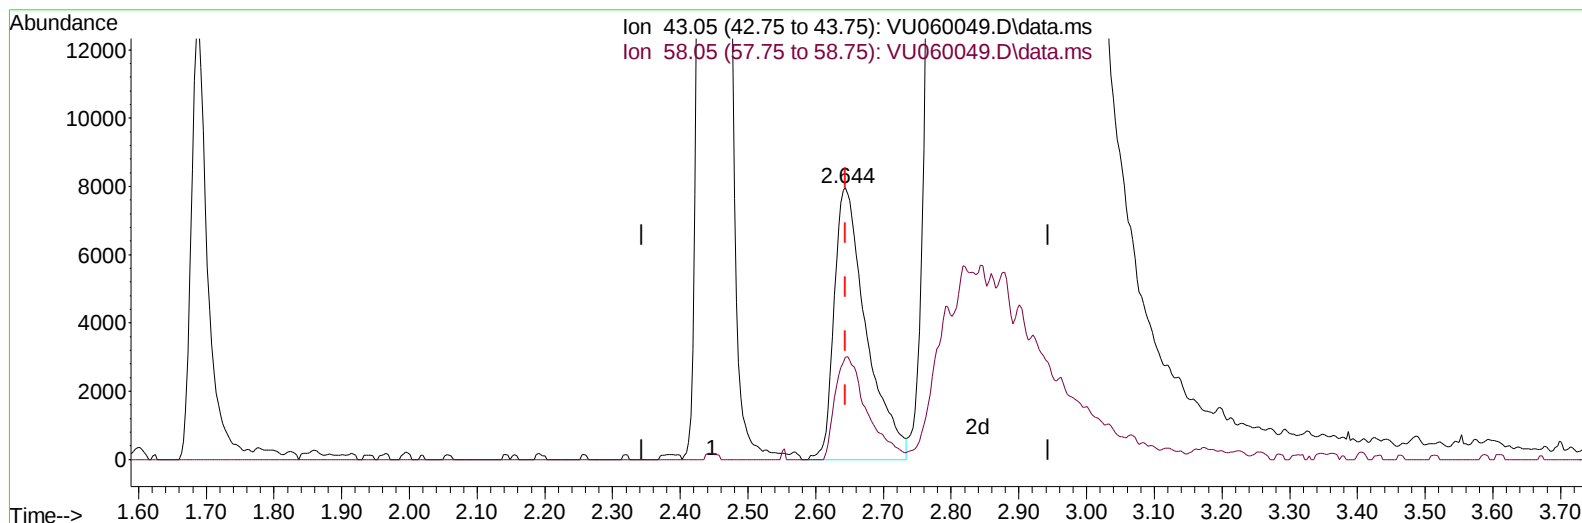

TIC: VU060049.D\data.ms

(13) Acetone (T)

2.644min (-0.000) 17.11 ug/L m

response 26267

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	37.52
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
 Data File : VU060049.D
 Acq On : 19 Jul 2024 10:17
 Operator : MD/SY
 Sample : P3237-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GB7

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:56:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 19 02:49:52 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
 Supervised By :Semsettin Yesilyurt 07/24/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		142691	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		143758	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		65183	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		36237	3.650	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	73.000%	
7) Chloroethane-d5	1.911	69		37145	4.027	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	80.600%	
11) 1,1-Dichloroethene-d2	2.563	65		14637	3.776	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	75.600%	
20) 2-Butanone-d5	4.624	46		100460	43.281	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	86.560%	
24) Chloroform-d	5.055	84		83367	3.995	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	80.000%	
26) 1,2-Dichloroethane-d4	5.695	65		41883	4.311	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	86.200%	
32) Benzene-d6	5.721	84		170091	4.416	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	88.400%	
36) 1,2-Dichloropropane-d6	6.682	67		54653	4.453	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	89.000%	
41) Toluene-d8	7.894	98		142278	4.088	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	81.800%	
43) trans-1,3-Dichloroprop...	8.177	79		15899	3.806	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	76.200%	
46) 2-Hexanone-d5	8.627	63		77284	41.687	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	83.380%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		46332	4.242	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	84.800%	
66) 1,2-Dichlorobenzene-d4	12.187	152		56873	4.834	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	96.600%	
Target Compounds							
13) Acetone	2.644	43		26267m	17.108	ug/L	
16) Methylene chloride	3.036	84		2441	0.183	ug/L	91
63) 1,2,4-Trimethylbenzene	11.467	105		5911	0.188	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060049.D
Acq On : 19 Jul 2024 10:17
Operator : MD/SY
Sample : P3237-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB7

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:56:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 19 02:49:52 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

