

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060039.D
Acq On : 18 Jul 2024 23:58
Operator : MD/SY
Sample : P3237-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU060039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.448	346	360	385	rBV	2257919	3723284	7.77%	6.934%
2	2.859	448	488	628	rBV	4881532	47921878	100.00%	89.244%
3	5.718	1356	1377	1403	rBV2	191693	502889	1.05%	0.937%
4	8.628	2269	2282	2311	rBV	286171	549783	1.15%	1.024%
5	9.412	2514	2526	2553	rBV	310007	520500	1.09%	0.969%
6	11.807	3259	3271	3291	rBV	293608	479543	1.00%	0.893%




Sum of corrected areas: 53697877

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060039.D
Acq On : 18 Jul 2024 23:58
Operator : MD/SY
Sample : P3237-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

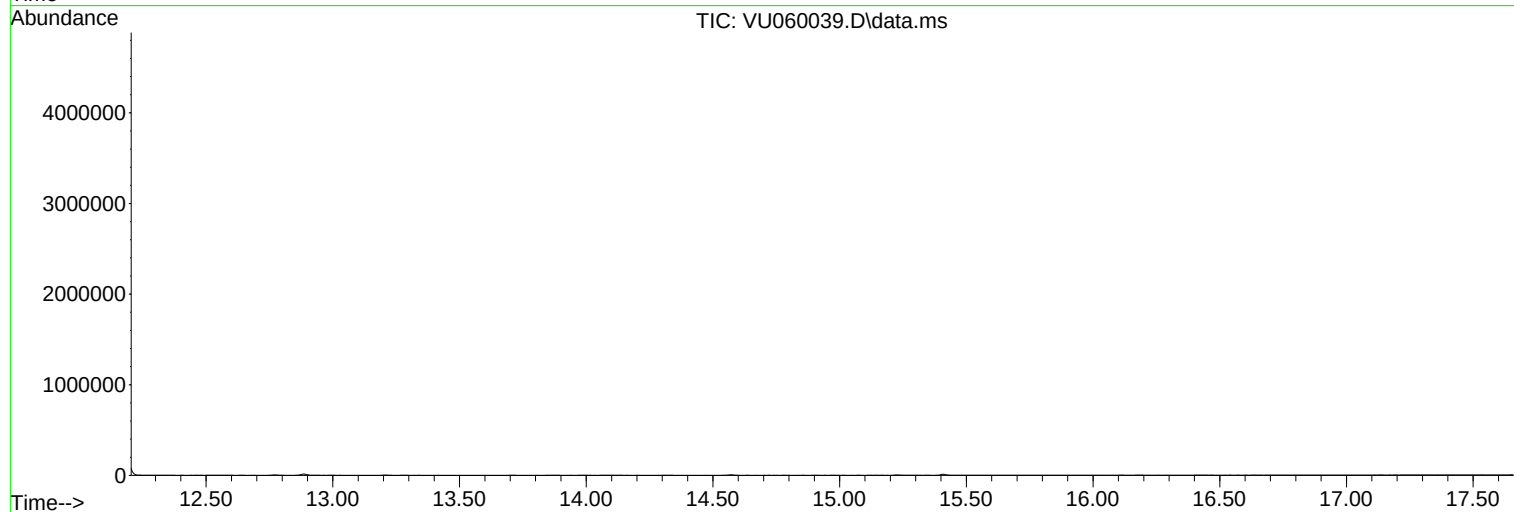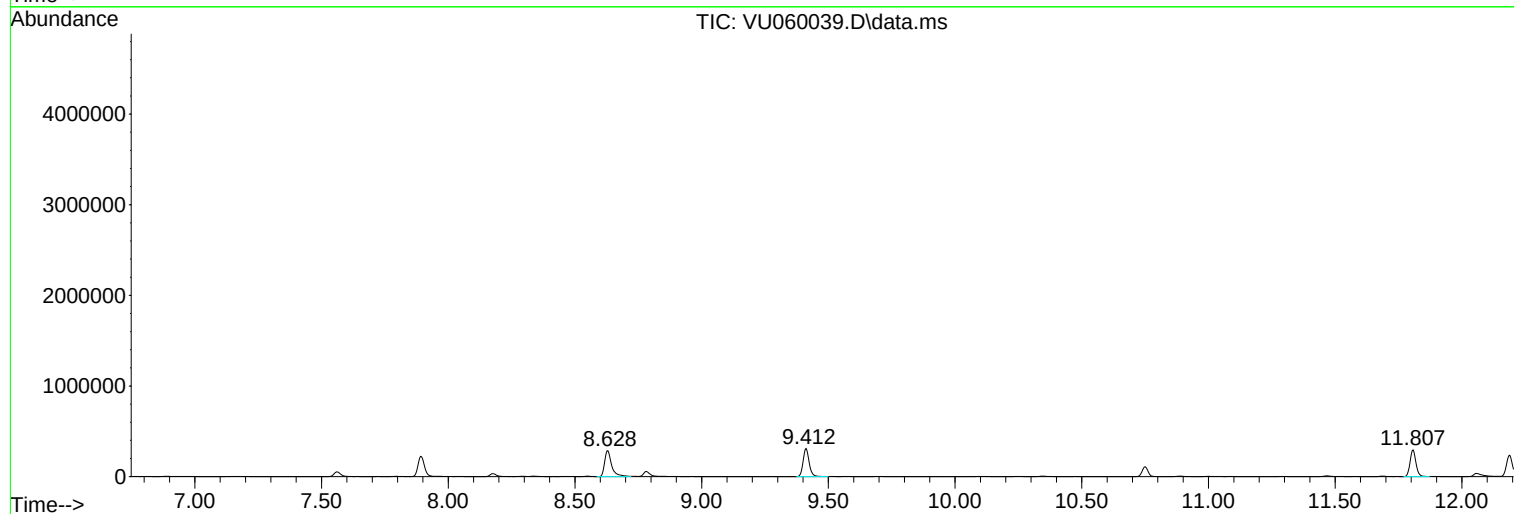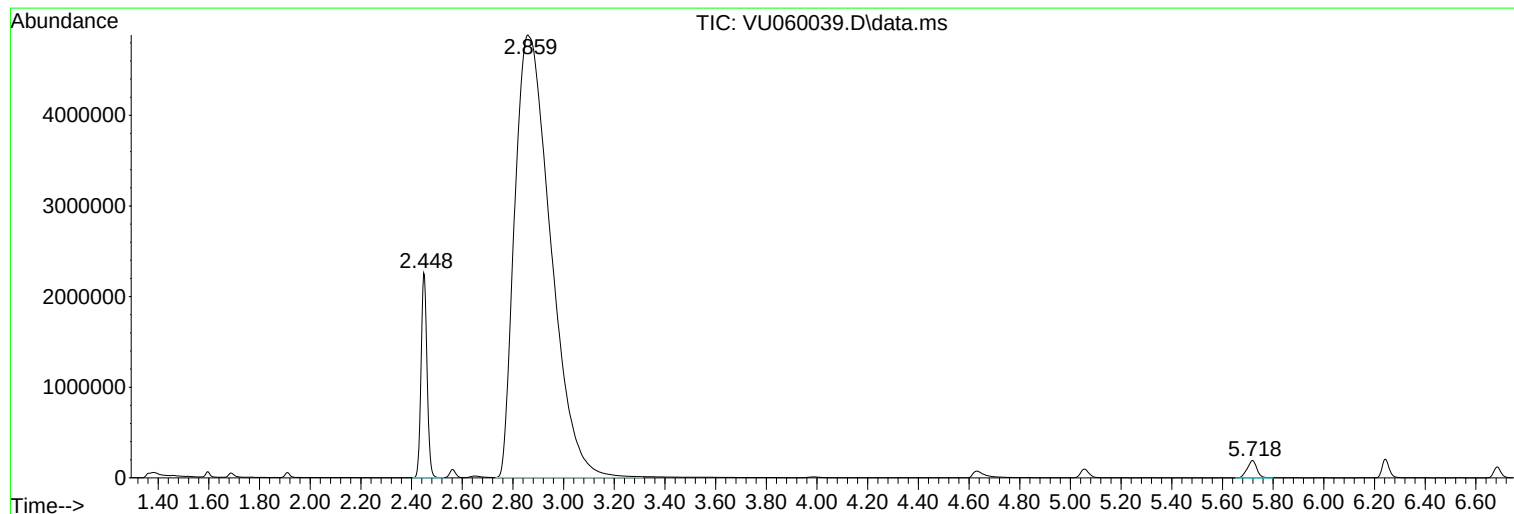

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060039.D
Acq On : 18 Jul 2024 23:58
Operator : MD/SY
Sample : P3237-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.448	37.02 ug/L	3723280	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	91
2			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	64
3			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	42
4			Acetyl chloride	78	C2H3ClO	000075-36-5	9
5			2-Chloroethanol	80	C2H5ClO	000107-07-3	4

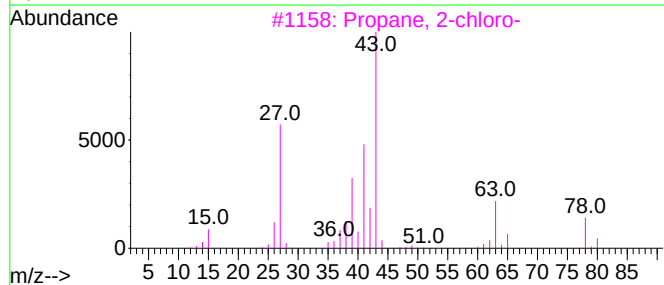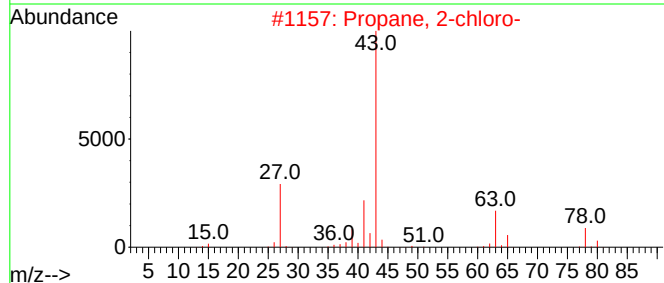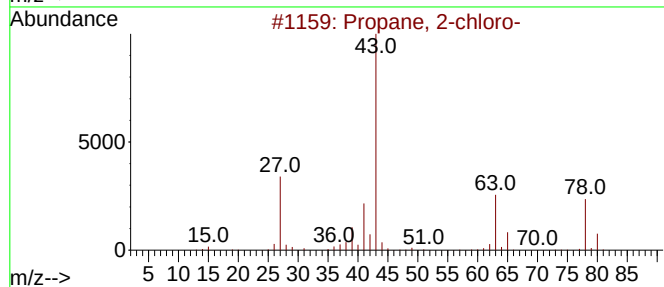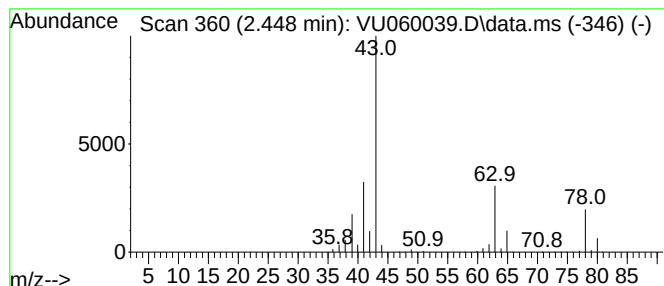

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060039.D
Acq On : 18 Jul 2024 23:58
Operator : MD/SY
Sample : P3237-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.859	476.47 ug/L	47921900	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
5			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

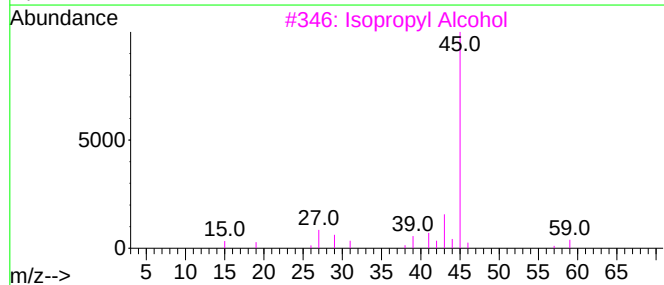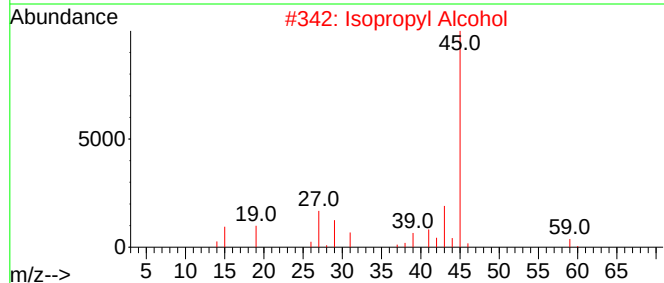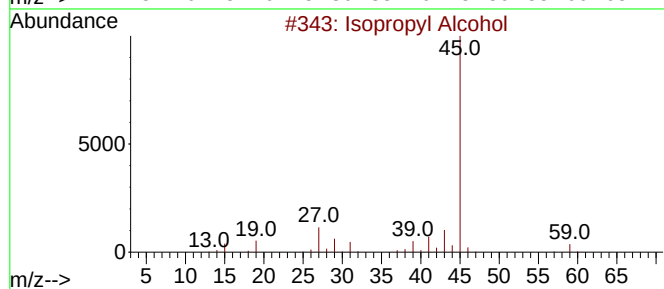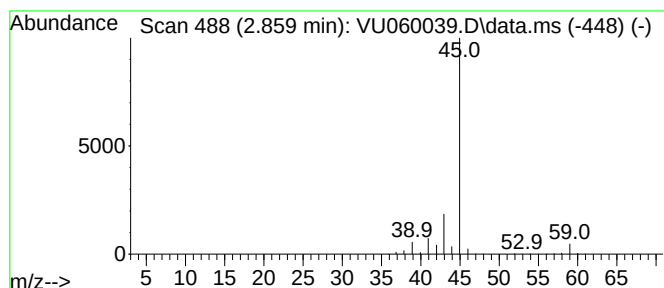

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060039.D
Acq On : 18 Jul 2024 23:58
Operator : MD/SY
Sample : P3237-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.448	37.0	ug/L	3723280	1	6.242	502889	5.0
Isopropyl Alcohol	2.859	476.5	ug/L	47921900	1	6.242	502889	5.0