

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060047.D
Acq On : 19 Jul 2024 09:29
Operator : MD/SY
Sample : P3237-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU060047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.451	343	361	385	rVB	1156787	1905366	5.28%	4.754%
2	2.827	445	478	567	rBV	5141704	36069244	100.00%	90.002%
3	5.718	1358	1377	1398	rBV2	180851	472469	1.31%	1.179%
4	7.891	2038	2053	2069	rBV	212553	375037	1.04%	0.936%
5	8.628	2269	2282	2311	rBV	235822	453427	1.26%	1.131%
6	9.412	2511	2526	2547	rBV	243014	410767	1.14%	1.025%
7	11.807	3258	3271	3292	rBV	236606	389569	1.08%	0.972%




Sum of corrected areas: 40075879

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060047.D
Acq On : 19 Jul 2024 09:29
Operator : MD/SY
Sample : P3237-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

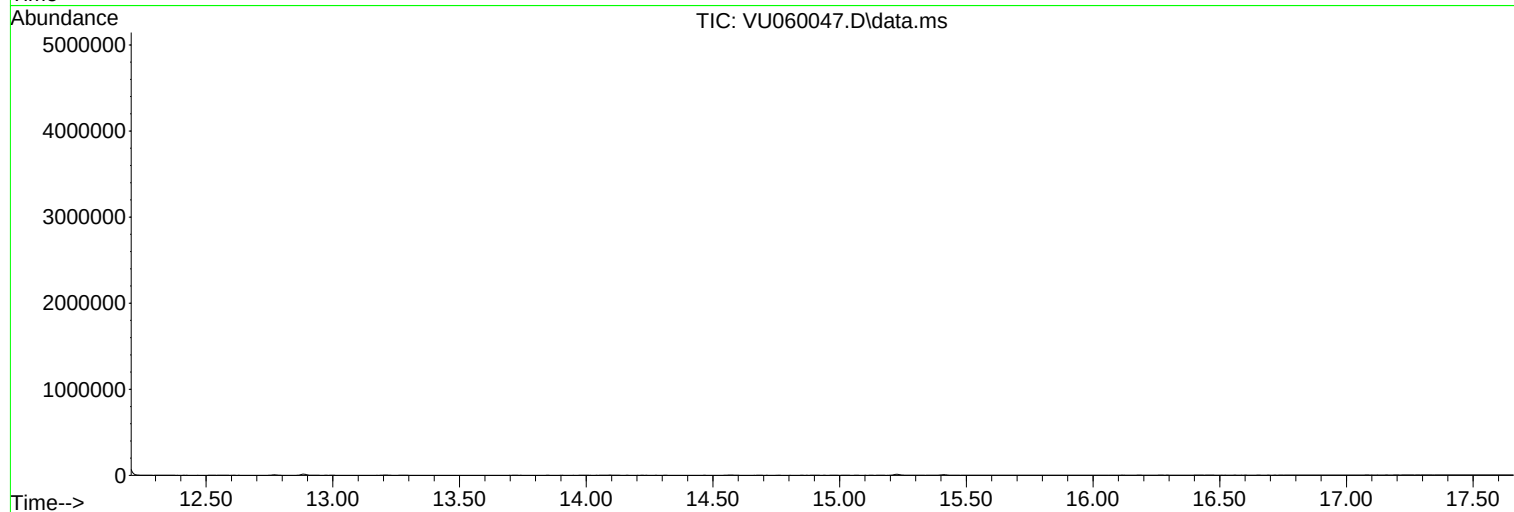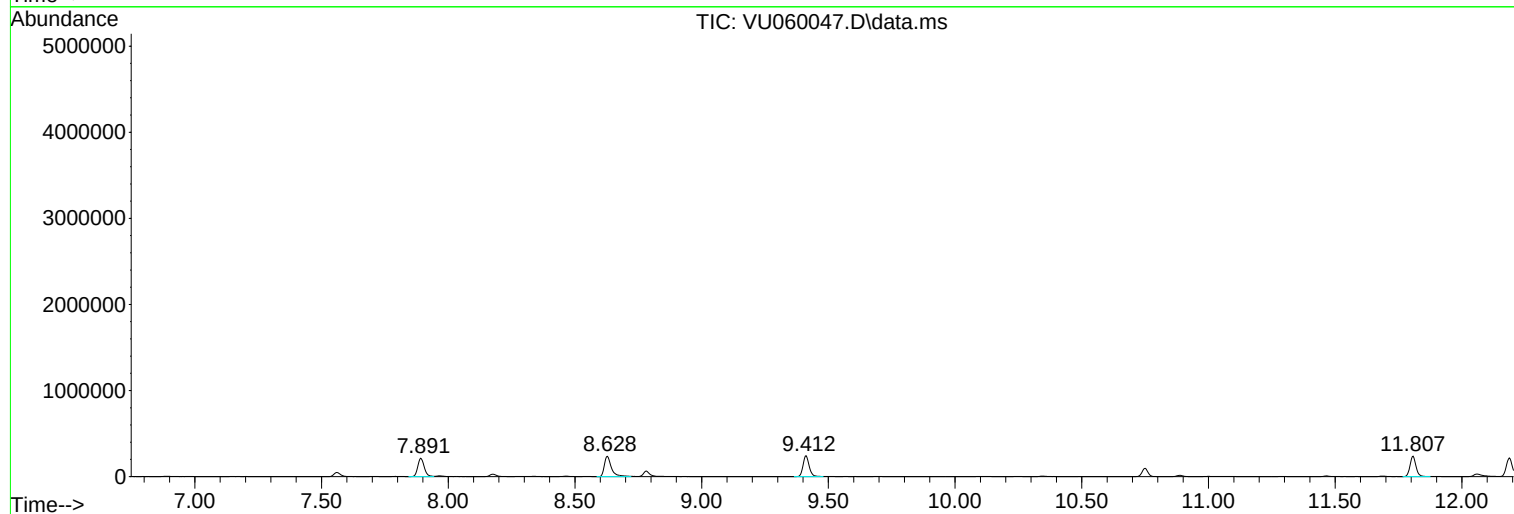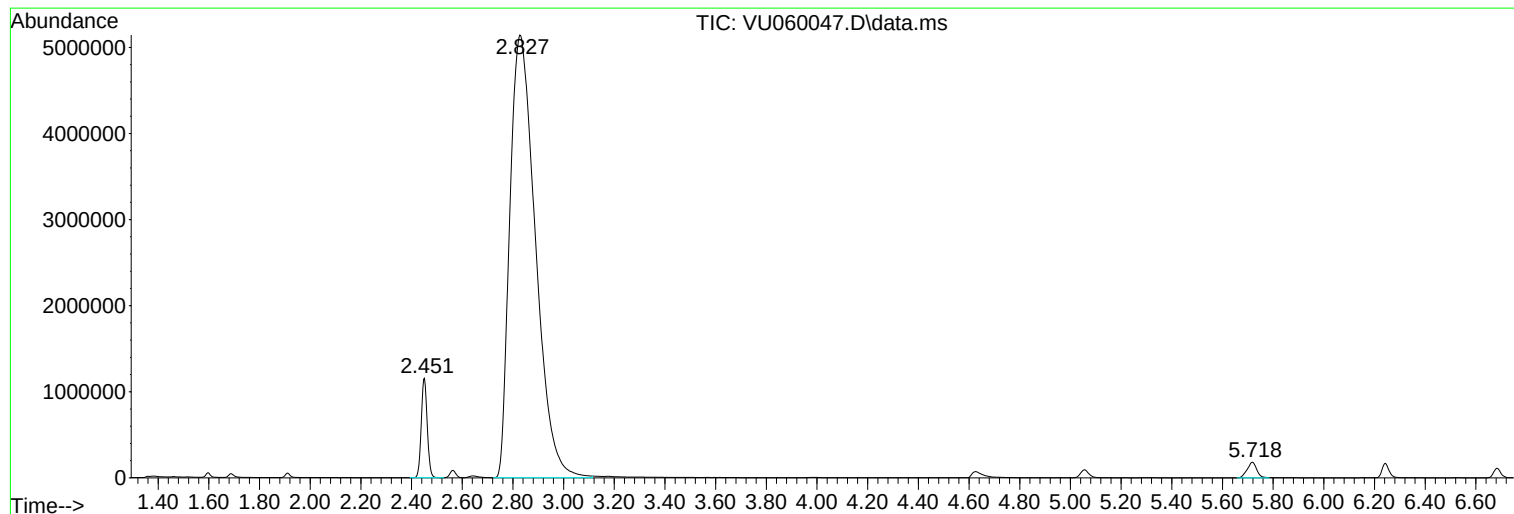

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060047.D
Acq On : 19 Jul 2024 09:29
Operator : MD/SY
Sample : P3237-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.451	20.16 ug/L	1905370	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	91
2			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	78
3			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	64
4			Acetyl chloride	78	C2H3ClO	000075-36-5	9
5			2-Chloroethanol	80	C2H5ClO	000107-07-3	4

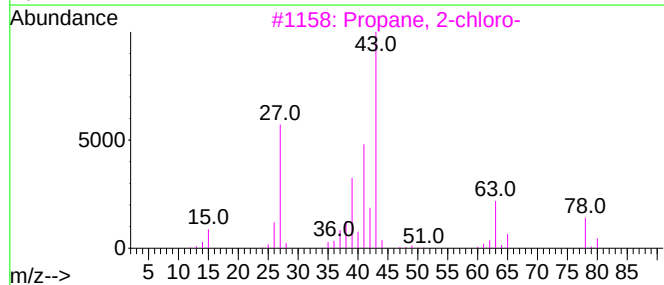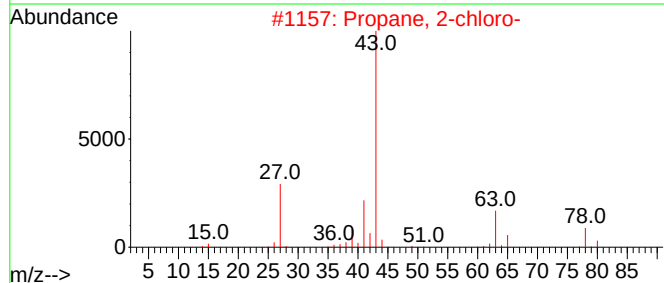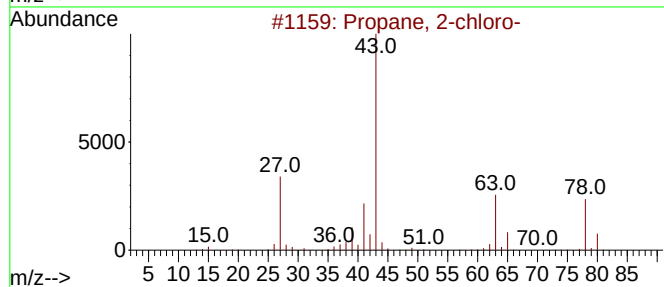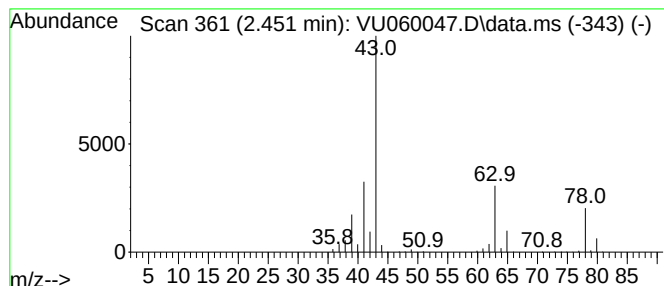

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060047.D
Acq On : 19 Jul 2024 09:29
Operator : MD/SY
Sample : P3237-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.827	381.71 ug/L	36069200	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
5			Propanoic acid, 2-hydroxy-, meth...	104	C4H8O3	000547-64-8	9

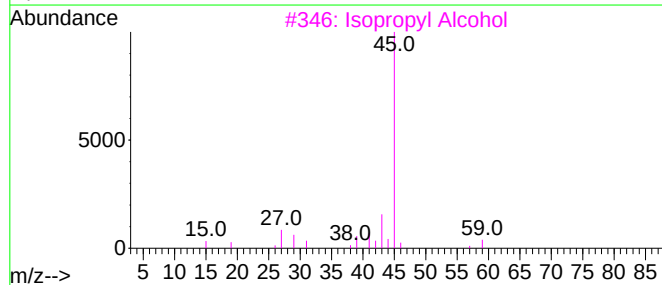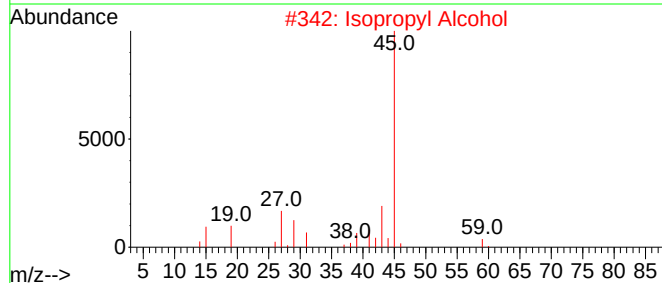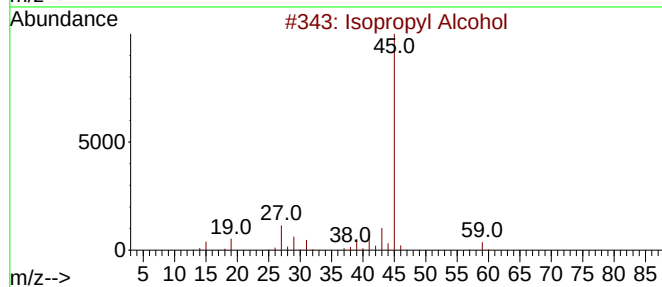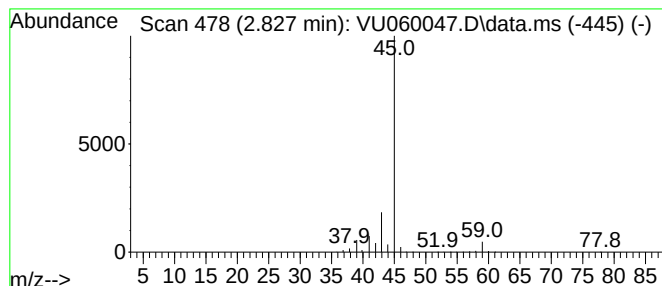

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060047.D
Acq On : 19 Jul 2024 09:29
Operator : MD/SY
Sample : P3237-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.451	20.2	ug/L	1905370	1	6.242	472469	5.0
Isopropyl Alcohol	2.827	381.7	ug/L	36069200	1	6.242	472469	5.0