

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
 Data File : VU060077.D
 Acq On : 19 Jul 2024 21:53
 Operator : MD/SY
 Sample : P3244-09 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YDZG0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU060077.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	111	rVB	40869	48086	11.54%	1.487%
2	1.911	182	193	208	rBV	39294	53723	12.90%	1.661%
3	2.560	379	395	412	rVB	63875	105768	25.39%	3.270%
4	3.039	532	544	562	rVB2	10917	21087	5.06%	0.652%
5	3.181	573	588	602	rBV	8499	18870	4.53%	0.583%
6	4.631	1025	1039	1077	rBV	60753	196102	47.08%	6.063%
7	5.055	1156	1171	1204	rBV	73522	167150	40.13%	5.168%
8	5.718	1354	1377	1400	rBV2	140416	369441	88.69%	11.423%
9	6.245	1529	1541	1570	rBV	126805	250539	60.14%	7.747%
10	6.682	1665	1677	1700	rBV	88897	178382	42.82%	5.515%
11	7.560	1940	1950	1968	rBV	35866	67342	16.17%	2.082%
12	7.894	2042	2054	2070	rBV	155416	268859	64.54%	8.313%
13	8.177	2133	2142	2162	rBV2	22523	40118	9.63%	1.240%
14	8.631	2271	2283	2323	rBV	204487	416573	100.00%	12.880%
15	9.412	2515	2526	2558	rBV	191369	326170	78.30%	10.085%
16	10.750	2931	2942	2959	rBV	83488	137328	32.97%	4.246%
17	10.888	2976	2985	2996	rBB3	3670	5379	1.29%	0.166%
18	11.807	3259	3271	3291	rBV	172651	284095	68.20%	8.784%
19	12.190	3378	3390	3408	rBV	152497	261809	62.85%	8.095%
20	12.769	3557	3570	3582	rVB2	4034	5811	1.39%	0.180%
21	14.573	4119	4131	4145	rVB2	6655	11573	2.78%	0.358%




Sum of corrected areas: 3234205

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060077.D
Acq On : 19 Jul 2024 21:53
Operator : MD/SY
Sample : P3244-09 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

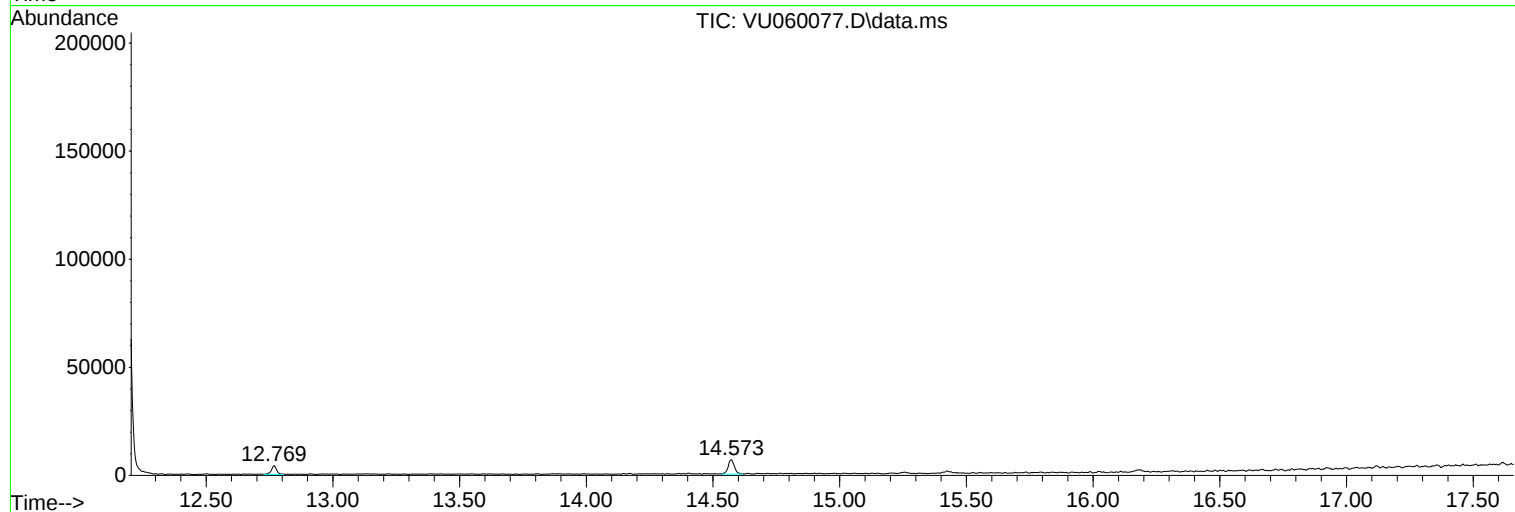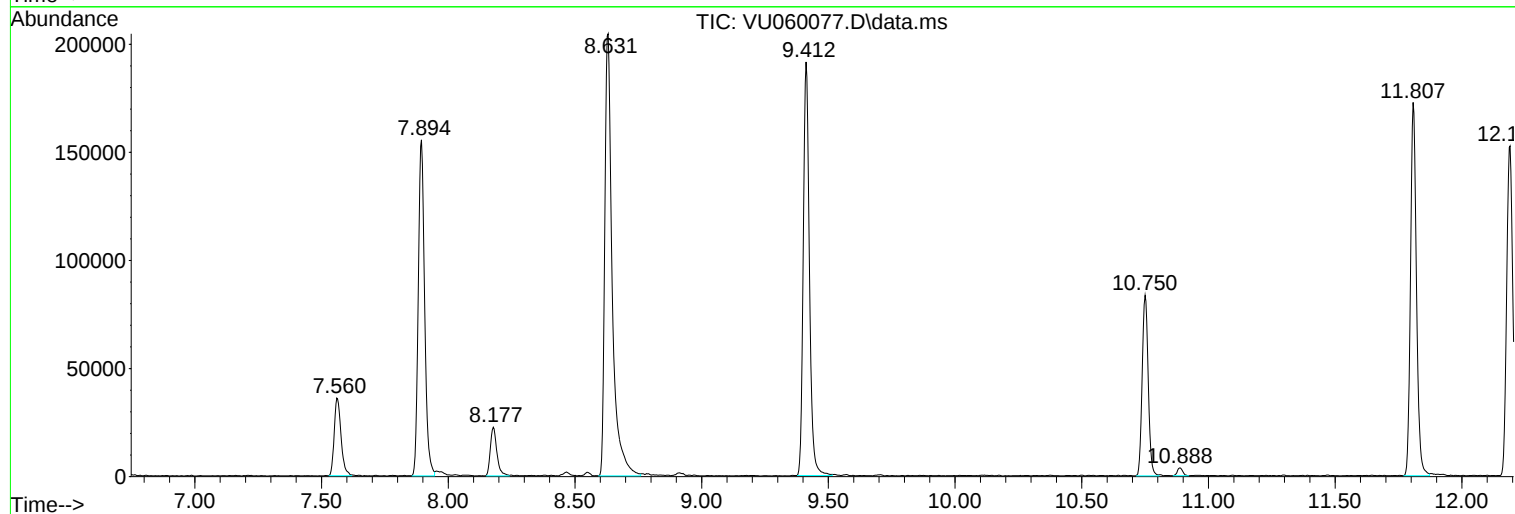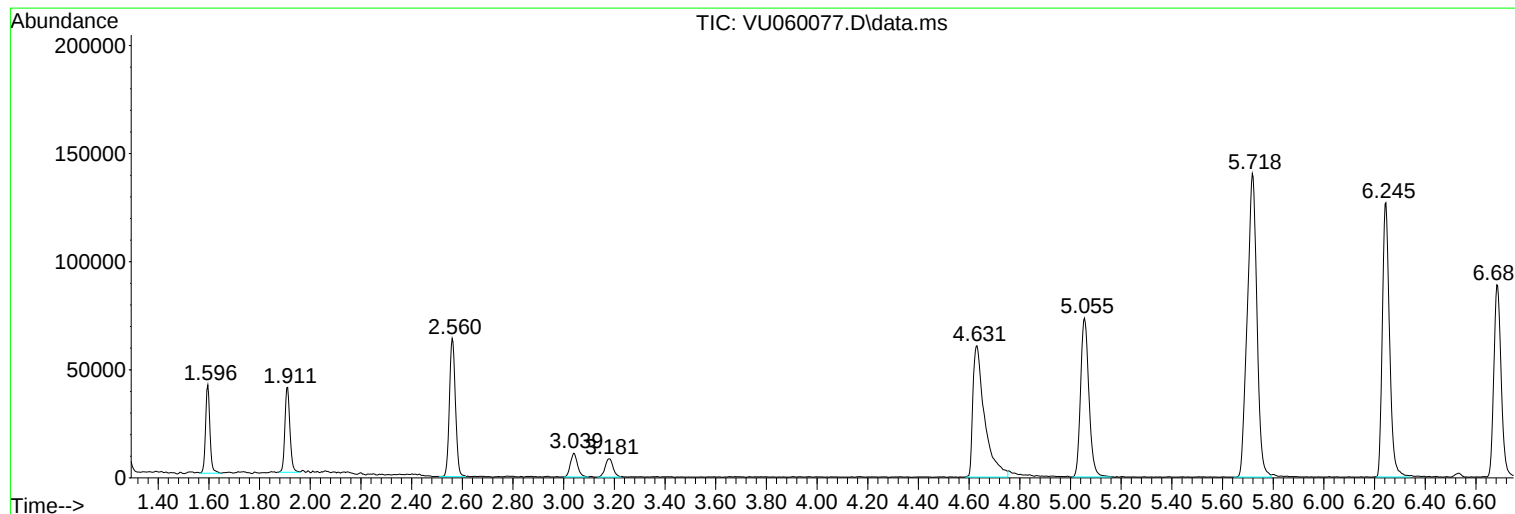

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060077.D
Acq On : 19 Jul 2024 21:53
Operator : MD/SY
Sample : P3244-09 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060077.D
Acq On : 19 Jul 2024 21:53
Operator : MD/SY
Sample : P3244-09 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc