


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071824\
Data File : VU060008.D
Acq On : 18 Jul 2024 09:01
Operator : MD/SY
Sample : BFB175
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB175

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Jul 20 01:37:26 2024

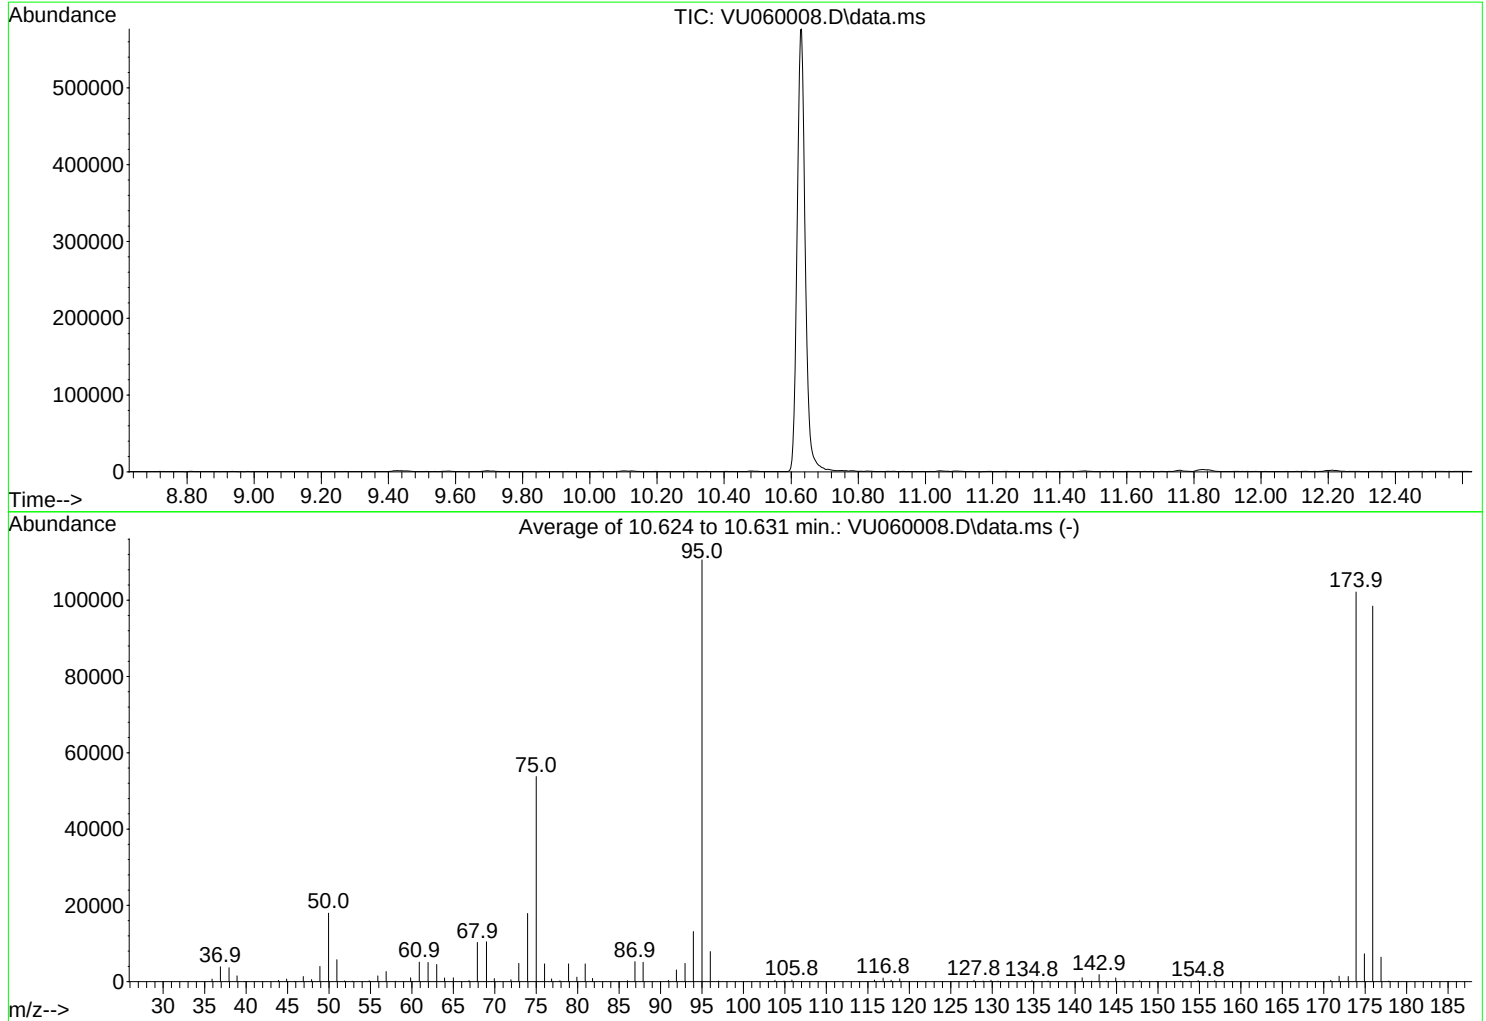

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.3	17976	PASS
75	95	30	80	48.6	53771	PASS
95	95	100	100	100.0	110587	PASS
96	95	5	9	7.1	7892	PASS
173	174	0.00	2	1.3	1341	PASS
174	95	50	120	92.4	102152	PASS
175	174	5	9	7.1	7295	PASS
176	174	95	101	96.4	98461	PASS
177	176	5	9	6.5	6426	PASS

Scan 2890 (10.583 min): VU060008.D\data.ms
BFB175

m/z	Abundance
39.80	244.0
43.90	245.0

Instrument :
MSVOA_U
ClientSampleId :
BFB175

m/z	Abundance
35.90	647.0
36.90	3809.0
37.90	3524.0
38.90	1494.0
39.80	270.0
43.90	577.0
44.90	622.0
45.90	111.0
46.90	1244.0
47.90	547.0
48.90	3903.0
50.00	17032.0
51.00	5470.0
51.90	188.0
52.90	167.0
54.80	255.0
55.90	1498.0
56.90	2753.0
58.00	127.0
59.80	871.0
60.90	4849.0
62.00	4756.0
63.00	4265.0
64.00	995.0
65.00	935.0
66.90	295.0
67.90	9817.0
69.00	10171.0
70.00	819.0
72.00	472.0
72.90	4509.0
74.00	16976.0
75.00	50296.0
76.00	4447.0
76.90	691.0
77.80	325.0
78.90	4460.0
79.90	1075.0
80.90	4639.0
81.80	753.0
86.00	219.0
86.90	4838.0
87.90	4596.0
90.90	336.0
91.90	2836.0
92.90	4603.0
94.00	12382.0
95.00	103856.0
96.00	7671.0
97.00	176.0
103.80	398.0
104.90	180.0
105.80	414.0
115.80	400.0
116.90	799.0
117.80	356.0
118.90	680.0
127.80	380.0
128.90	181.0
129.90	369.0
130.70	151.0
134.80	272.0
136.70	200.0
140.80	924.0
142.90	1757.0
143.80	175.0
144.90	986.0
146.00	121.0
147.80	223.0
149.90	101.0
152.80	170.0
153.80	101.0
154.90	269.0
155.70	100.0
156.80	181.0
160.60	117.0
170.80	329.0
171.90	1258.0
172.90	1293.0
173.90	93776.0
174.90	6781.0
175.90	90240.0
176.90	5931.0
177.90	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB175

m/z	Abundance
35.90	702.0
36.90	4064.0
38.00	3798.0
38.90	1562.0
39.80	312.0
43.90	591.0
44.90	684.0
46.90	1405.0
47.90	543.0
48.90	4062.0
50.00	18600.0
51.00	5945.0
51.90	211.0
52.80	153.0
54.90	236.0
55.90	1551.0
56.90	2789.0
58.00	144.0
59.90	1061.0
60.90	5325.0
61.90	5208.0
63.00	4624.0
64.00	977.0
65.00	1058.0
66.90	287.0
67.90	10624.0
69.00	10836.0
69.90	814.0
72.00	533.0
72.90	4965.0
73.90	18384.0
75.00	55528.0
76.00	4732.0
76.80	734.0
78.90	4870.0
79.90	1205.0
80.90	4825.0
81.80	846.0
86.00	294.0
86.90	5458.0
87.90	5257.0
90.90	349.0
91.90	3257.0
92.90	4975.0
93.90	13519.0
95.00	114200.0
96.00	8099.0
97.00	172.0
103.80	397.0
104.90	189.0
105.90	439.0
115.80	443.0
116.80	928.0
117.80	401.0
118.90	768.0
127.80	418.0
128.90	189.0
129.90	374.0
130.70	186.0
134.80	301.0
136.80	194.0
139.90	128.0
140.90	1061.0
142.00	158.0
142.90	1884.0
143.80	161.0
144.90	1023.0
145.90	163.0
147.80	241.0
149.00	101.0
152.80	184.0
153.80	128.0
154.80	299.0
156.90	249.0
170.90	366.0
171.80	1419.0
172.90	1361.0
173.90	105552.0
174.90	7491.0
175.90	101480.0
176.90	6638.0
177.90	173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB175

m/z	Abundance
35.90	691.0
36.90	3813.0
38.00	3659.0
38.90	1505.0
39.80	311.0
43.90	602.0
44.90	670.0
45.80	120.0
46.90	1346.0
47.90	575.0
48.90	3967.0
49.90	18296.0
50.90	5843.0
51.90	221.0
52.70	119.0
54.90	221.0
55.90	1541.0
56.90	2421.0
58.00	129.0
59.90	1108.0
60.90	5217.0
61.90	5184.0
63.00	4529.0
63.90	887.0
65.00	1073.0
65.90	145.0
66.90	267.0
67.90	10363.0
69.00	10329.0
69.90	722.0
71.90	538.0
72.90	4894.0
73.90	18224.0
75.00	55488.0
76.00	4811.0
76.80	741.0
77.90	382.0
78.90	4689.0
79.90	1242.0
80.90	4516.0
81.80	867.0
86.00	233.0
86.90	5415.0
87.90	5417.0
91.00	363.0
91.90	3160.0
93.00	4752.0
94.00	13538.0
95.00	113704.0
96.00	7905.0
97.00	181.0
103.80	390.0
104.90	188.0
105.90	422.0
115.80	417.0
116.80	998.0
117.80	409.0
118.80	839.0
127.80	384.0
128.90	197.0
129.80	348.0
130.70	162.0
134.80	271.0
136.80	173.0
139.90	125.0
140.90	1040.0
142.00	189.0
142.90	1871.0
143.80	117.0
144.90	952.0
145.80	201.0
147.80	256.0
149.80	102.0
152.70	164.0
153.80	108.0
154.80	310.0
156.90	278.0
158.90	108.0
170.90	360.0
171.90	1600.0
173.00	1370.0
173.90	107128.0
174.90	7614.0
175.90	103664.0
176.90	6710.0
177.80	173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB175