

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063533.D
 Acq On : 18 Jul 2025 10:49
 Operator : MD/SY
 Sample : VU0718WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0718WBL01

Quant Time: Jul 18 23:47:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.100	96	25256	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.630	95	7573	0.792	ug/l	0.00
Spiked Amount 1.000			Recovery	=	79.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	6388	0.722	ug/l	0.00
Spiked Amount 1.000			Recovery	=	72.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
Data File : VU063533.D
Acq On : 18 Jul 2025 10:49
Operator : MD/SY
Sample : VU0718WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0718WBL01


Quant Time: Jul 18 23:47:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 17 03:49:40 2025
Response via : Initial Calibration

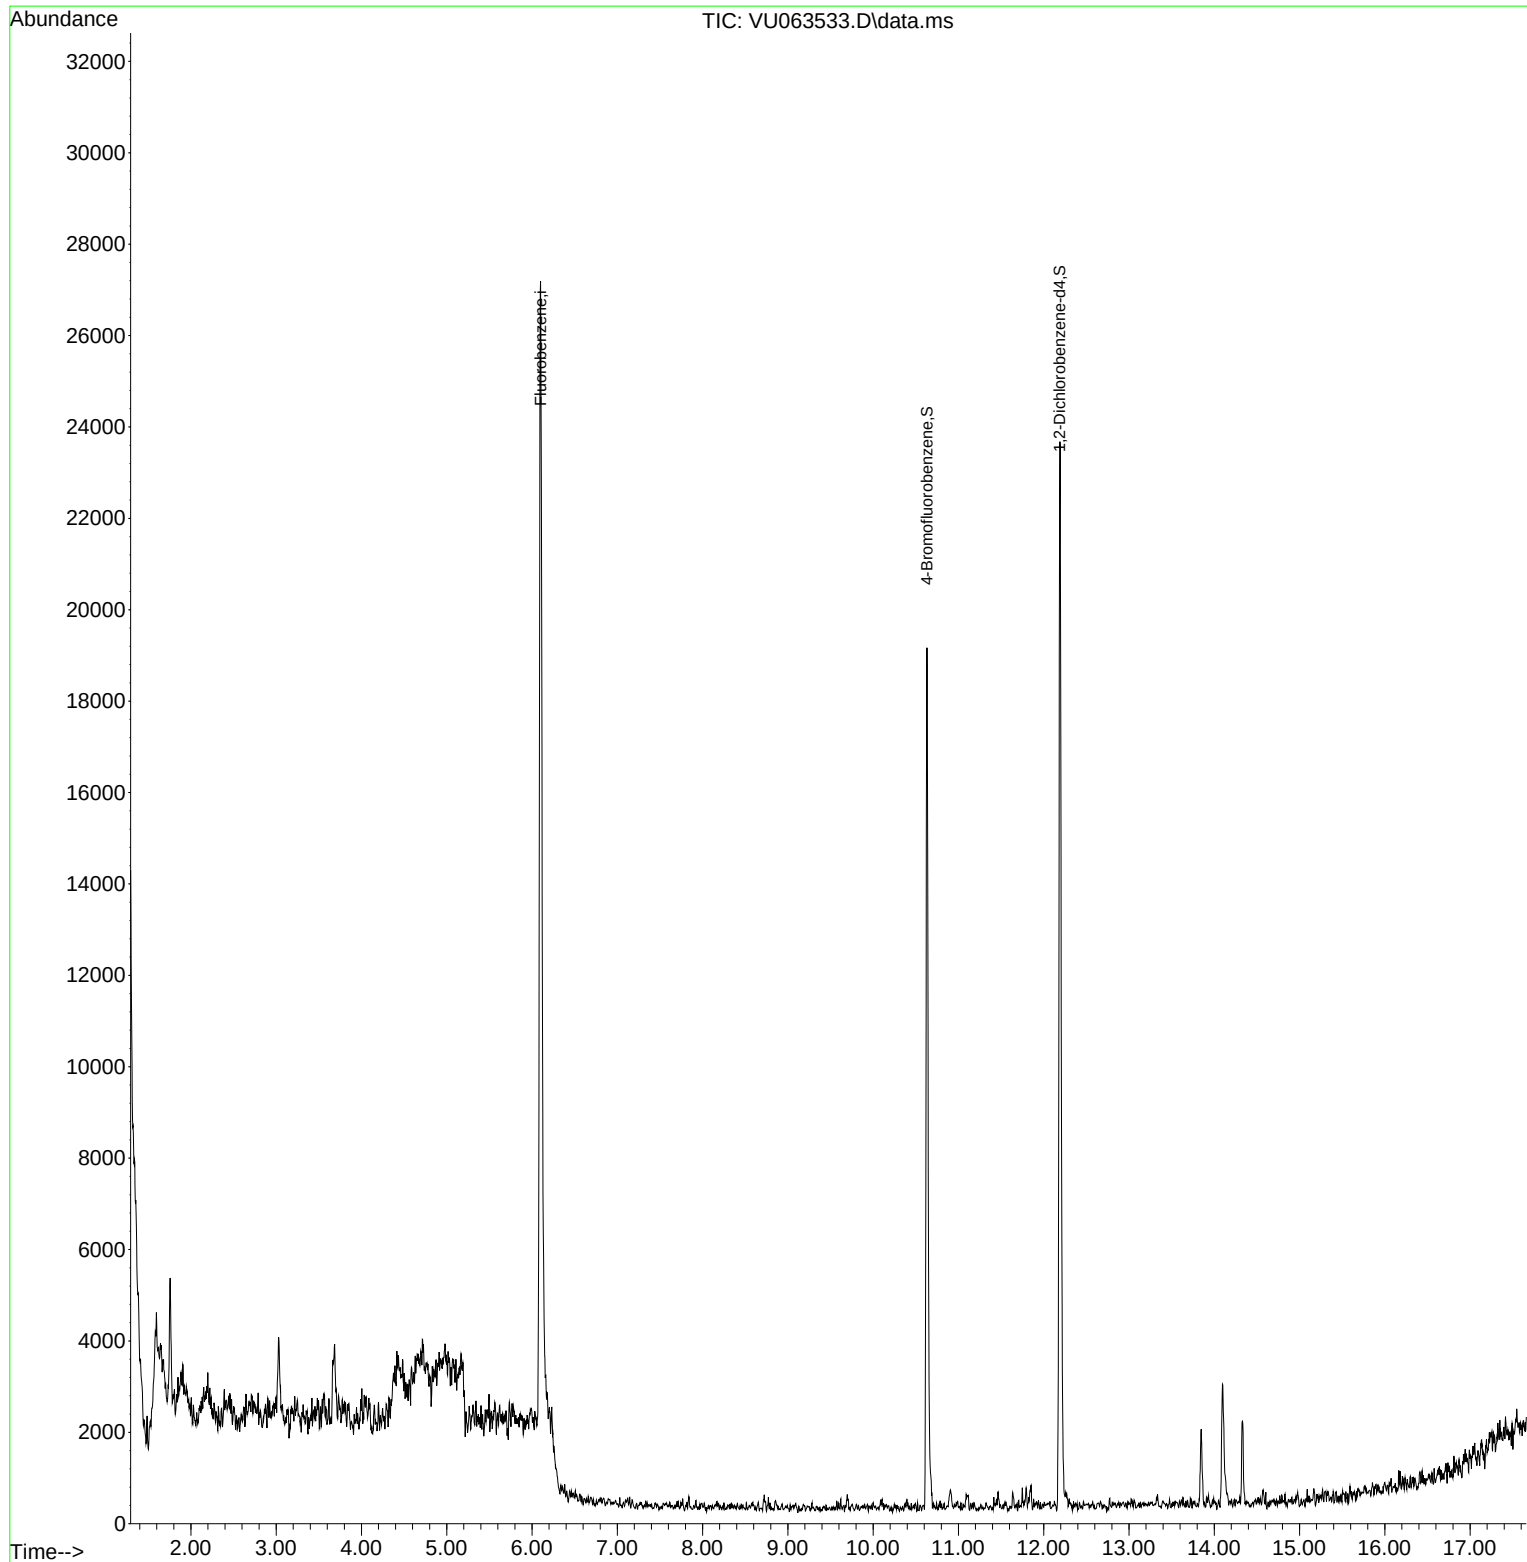



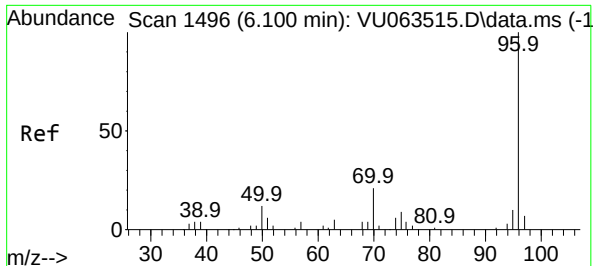


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.100 min Scan# 1496
Delta R.T. 0.000 min
Lab File: VU063533.D
Acq: 18 Jul 2025 10:49

Instrument :
MSVOA_U
ClientSampleId :
VU0718WBL01



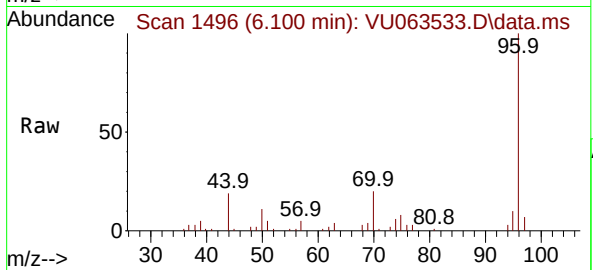



Tgt Ion:	96	Resp:	25256
Ion	Ratio	Lower	Upper
96	100		
70	17.9	15.0	22.4
95	8.9	7.4	11.0
97	5.1	0.0	0.0

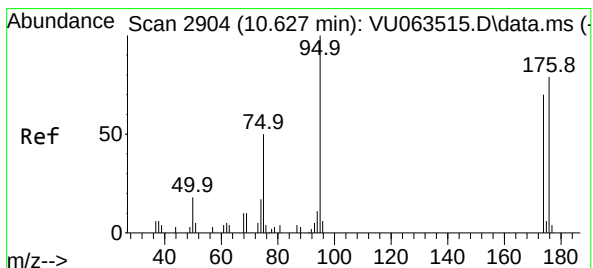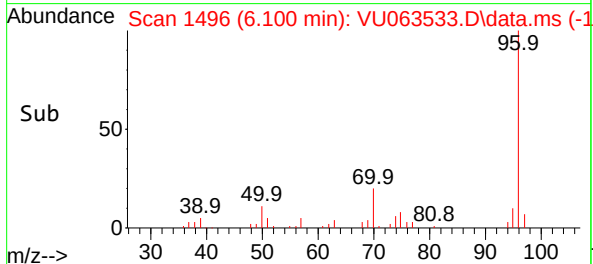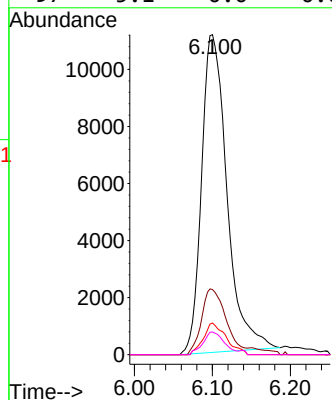

#57
4-Bromofluorobenzene
Concen: 0.792 ug/l
RT: 10.630 min Scan# 2905
Delta R.T. 0.003 min
Lab File: VU063533.D
Acq: 18 Jul 2025 10:49


Tgt Ion:	95	Resp:	7573
Ion	Ratio	Lower	Upper
95	100		
174	68.0	59.8	89.8
176	66.6	61.8	92.8

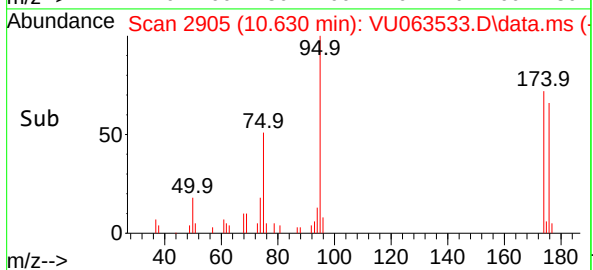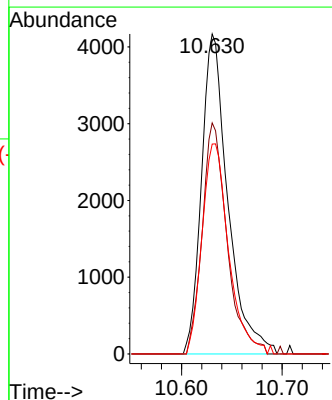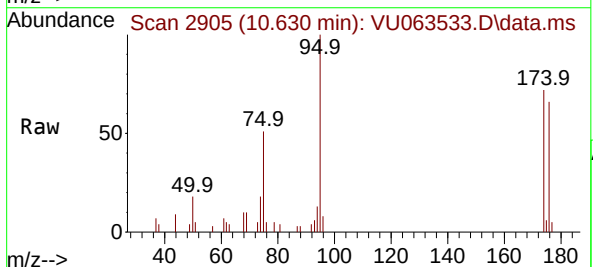

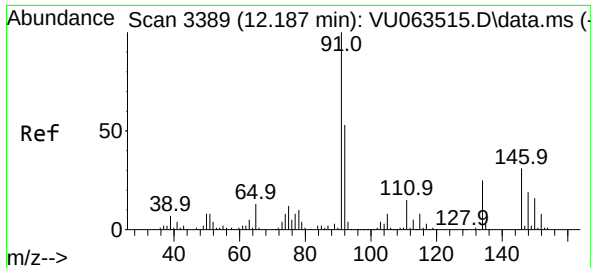

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.722 ug/l
 RT: 12.187 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VU063533.D
 Acq: 18 Jul 2025 10:49

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0718WBL01

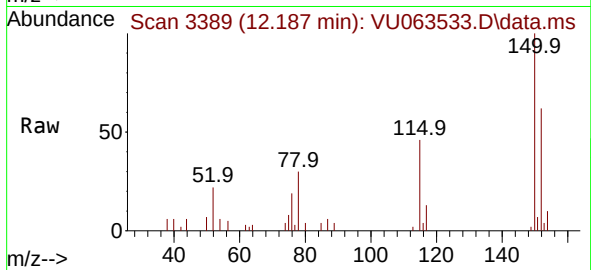

Tgt Ion:	152	Resp:	6388
Ion Ratio	Lower	Upper	
152	100		
115	71.0	0.0	262.2
150	165.4	0.0	651.2

