

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063533.D
 Acq On : 18 Jul 2025 10:49
 Operator : MD/SY
 Sample : VU0718WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0718WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.647	418	422	426	rBV2	721	645	1.20%	0.433%
2	2.901	498	501	505	rBV2	658	595	1.11%	0.399%
3	3.029	534	541	547	rBV5	1651	2558	4.76%	1.715%
4	3.666	734	739	740	rBV2	1396	1194	2.22%	0.801%
5	4.322	940	943	948	rBV4	645	608	1.13%	0.408%
6	4.586	1022	1025	1029	rBV4	837	909	1.69%	0.610%
7	5.734	1378	1382	1388	rBV2	824	1037	1.93%	0.695%
8	6.100	1485	1496	1513	rBV	24884	53721	100.00%	36.027%
9	6.232	1533	1537	1543	rVB4	997	1093	2.03%	0.733%
10	10.630	2896	2905	2922	rBV	18861	31537	58.71%	21.150%
11	10.907	2983	2991	2998	rBV	367	634	1.18%	0.425%
12	12.190	3378	3390	3409	rBV2	23397	42193	78.54%	28.296%
13	13.846	3895	3905	3915	rBV5	1695	2599	4.84%	1.743%
14	14.097	3974	3983	3998	rBV2	2700	5690	10.59%	3.816%
15	14.331	4048	4056	4065	rVB2	1821	2657	4.95%	1.782%
16	17.135	4921	4928	4931	rBV4	564	756	1.41%	0.507%
17	17.193	4940	4946	4948	rBV4	642	686	1.28%	0.460%




Sum of corrected areas: 149112

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
Data File : VU063533.D
Acq On : 18 Jul 2025 10:49
Operator : MD/SY
Sample : VU0718WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0718WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

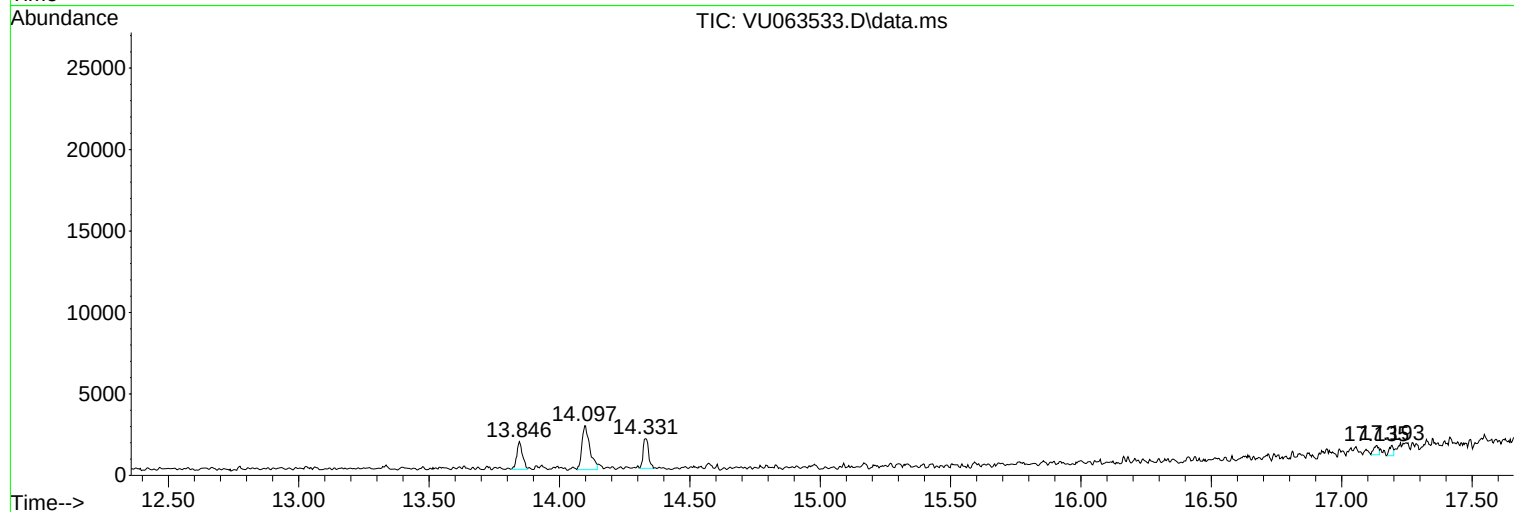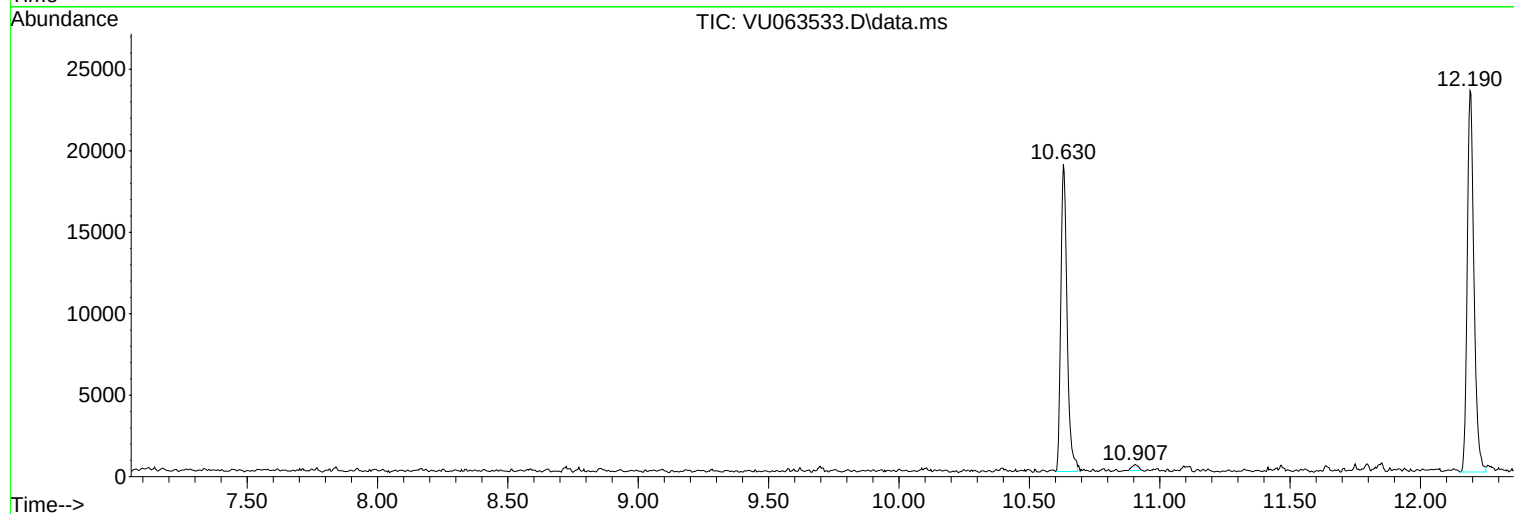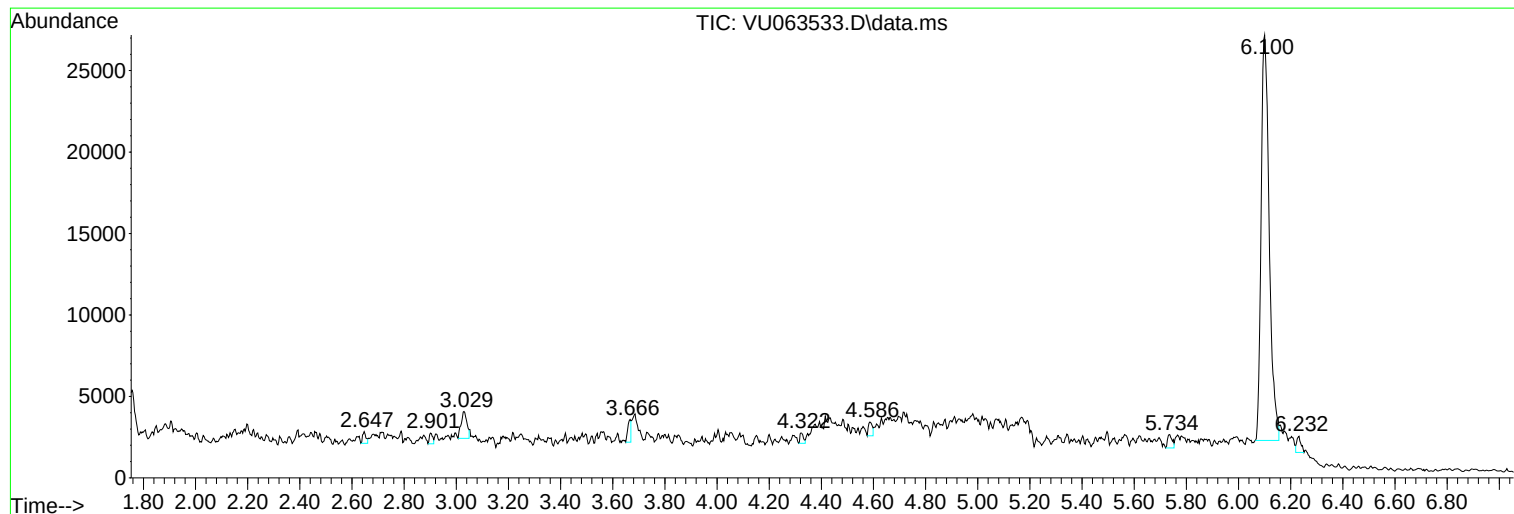

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
Data File : VU063533.D
Acq On : 18 Jul 2025 10:49
Operator : MD/SY
Sample : VU0718WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0718WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
Data File : VU063533.D
Acq On : 18 Jul 2025 10:49
Operator : MD/SY
Sample : VU0718WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0718WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------