

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063538.D
 Acq On : 18 Jul 2025 15:54
 Operator : MD/SY
 Sample : Q2552-08
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-UNRVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.846	165	173	186	rBV	62736	80597	5.64%	0.544%
2	2.129	248	261	279	rBV	770708	1136954	79.58%	7.674%
3	2.708	431	441	454	rBV	10997	19161	1.34%	0.129%
4	3.358	626	643	670	rBV	561758	1303347	91.23%	8.797%
5	3.850	781	796	815	rBV	73876	172315	12.06%	1.163%
6	4.644	1026	1043	1066	rBV2	169517	420801	29.45%	2.840%
7	4.956	1125	1140	1168	rBV	160896	352807	24.70%	2.381%
8	5.502	1294	1310	1352	rBV	296882	660081	46.20%	4.455%
9	6.097	1485	1495	1514	rVB2	24921	50865	3.56%	0.343%
10	6.907	1734	1747	1779	rBV	105917	204329	14.30%	1.379%
11	7.599	1950	1962	1988	rBV	190373	342383	23.97%	2.311%
12	8.203	2138	2150	2173	rBV	115024	199687	13.98%	1.348%
13	8.570	2249	2264	2283	rBV	39232	76110	5.33%	0.514%
14	9.525	2548	2561	2596	rVB	314261	521893	36.53%	3.523%
15	10.476	2844	2857	2879	rBV	293417	461991	32.34%	3.118%
16	10.627	2893	2904	2920	rVB2	19896	33220	2.33%	0.224%
17	10.775	2937	2950	2957	rBV2	233577	392311	27.46%	2.648%
18	10.814	2957	2962	2975	rVV	94986	149171	10.44%	1.007%
19	10.898	2976	2988	3003	rVV	758086	1181222	82.68%	7.973%
20	10.978	3004	3013	3033	rVV	100927	176163	12.33%	1.189%
21	11.084	3033	3046	3071	rVB3	353828	630704	44.15%	4.257%
22	11.409	3134	3147	3155	rBV	204096	324793	22.73%	2.192%
23	11.460	3155	3163	3179	rVB	165500	253526	17.75%	1.711%
24	11.634	3202	3217	3236	rBV	568557	864181	60.49%	5.833%
25	11.737	3237	3249	3255	rVV	189924	298467	20.89%	2.015%
26	11.785	3255	3264	3304	rVB	791673	1223040	85.61%	8.255%
27	12.200	3378	3393	3411	rBV	490485	757877	53.05%	5.115%
28	14.010	3944	3956	3968	rBV	929546	1428655	100.00%	9.643%
29	14.081	3968	3978	3996	rVB	144480	245057	17.15%	1.654%
30	14.319	4040	4052	4077	rBV	511298	854030	59.78%	5.764%




Sum of corrected areas: 14815738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
Data File : VU063538.D
Acq On : 18 Jul 2025 15:54
Operator : MD/SY
Sample : Q2552-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

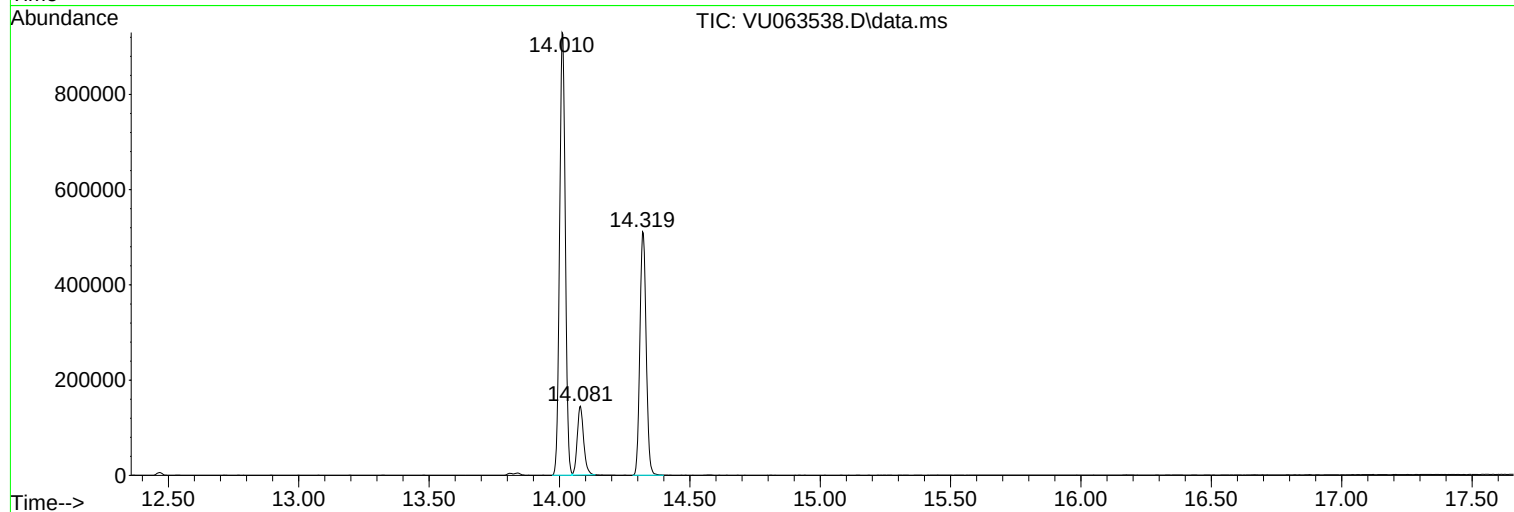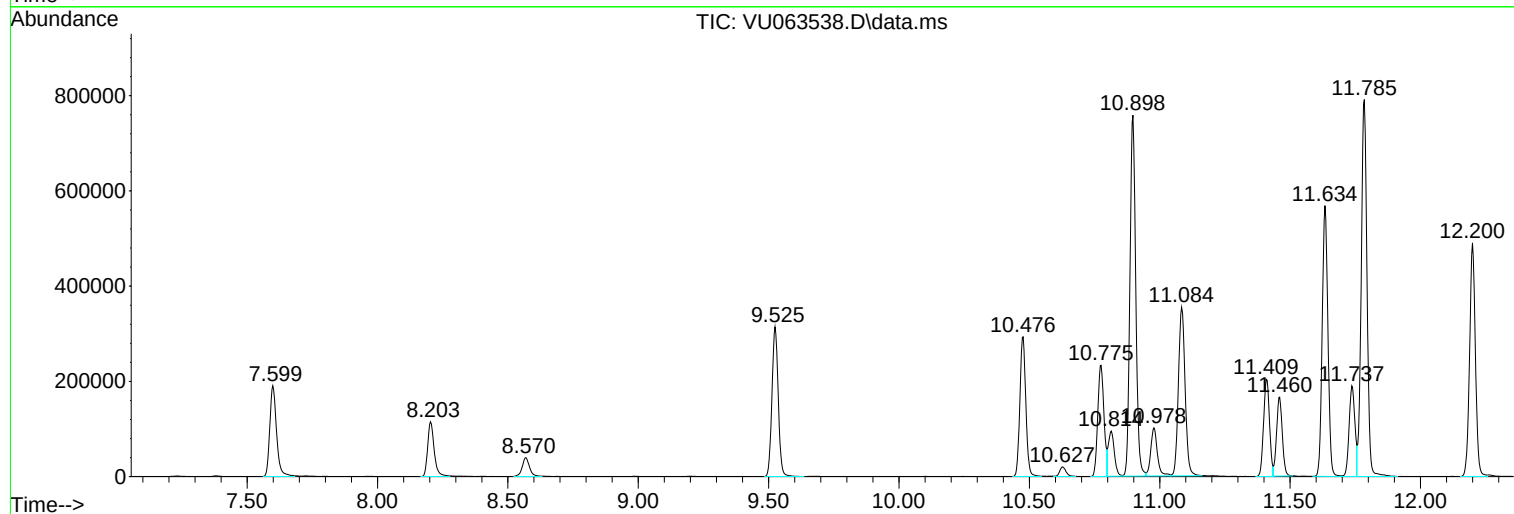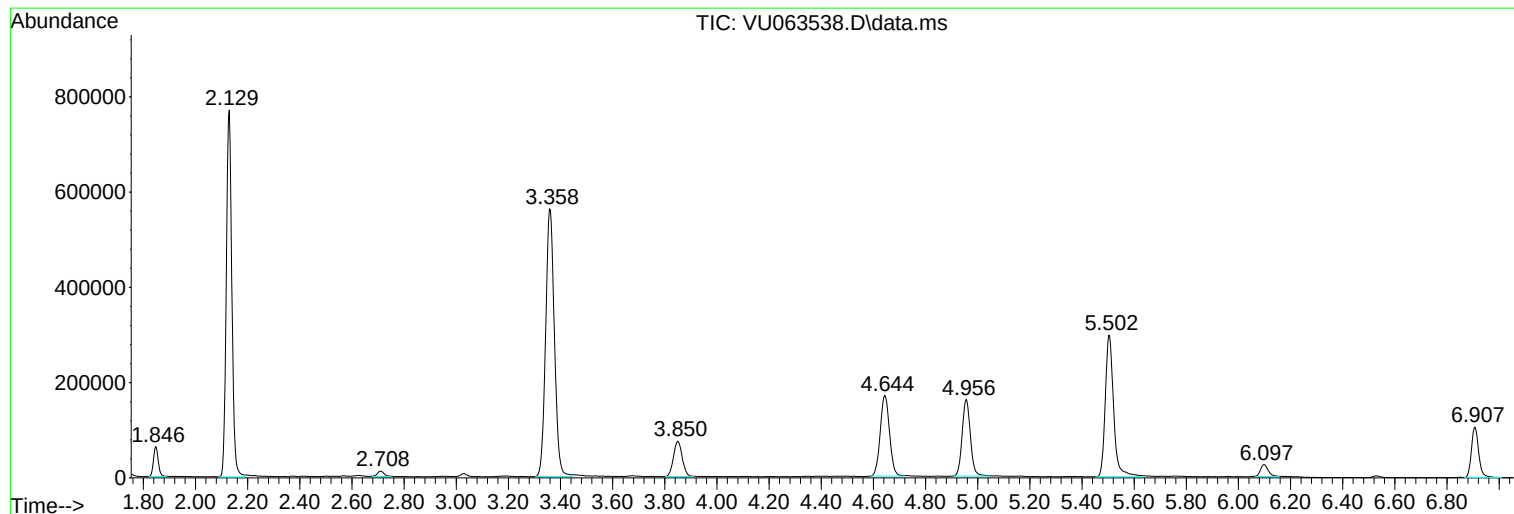

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
Data File : VU063538.D
Acq On : 18 Jul 2025 15:54
Operator : MD/SY
Sample : Q2552-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
Data File : VU063538.D
Acq On : 18 Jul 2025 15:54
Operator : MD/SY
Sample : Q2552-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------