

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063540.D
 Acq On : 18 Jul 2025 16:55
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.104	248	253	256	rBV4	786	888	1.02%	0.339%
2	3.030	529	541	561	rVB	47249	86908	100.00%	33.211%
3	3.673	734	741	753	rVB8	1795	3715	4.27%	1.420%
4	6.100	1482	1496	1508	rBV	18625	36409	41.89%	13.913%
5	10.631	2896	2905	2924	rVB	16383	26421	30.40%	10.096%
6	10.907	2980	2991	3002	rBV2	2842	4204	4.84%	1.607%
7	11.100	3042	3051	3059	rBV4	910	1579	1.82%	0.603%
8	11.637	3212	3218	3228	rVB2	1689	2359	2.71%	0.901%
9	11.750	3246	3253	3258	rBV4	897	1087	1.25%	0.415%
10	11.791	3258	3266	3272	rVV3	2531	3473	4.00%	1.327%
11	12.190	3380	3390	3407	rBV4	22284	43217	49.73%	16.515%
12	13.849	3899	3906	3911	rBV3	690	1002	1.15%	0.383%
13	14.013	3949	3957	3965	rVB4	6847	8976	10.33%	3.430%
14	14.090	3970	3981	3999	rBV2	7844	14325	16.48%	5.474%
15	14.325	4044	4054	4069	rBV2	15820	26112	30.05%	9.978%
16	16.177	4624	4630	4639	rVB4	582	1011	1.16%	0.386%




Sum of corrected areas: 261686

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
Data File : VU063540.D
Acq On : 18 Jul 2025 16:55
Operator : MD/SY
Sample : VIBLK
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

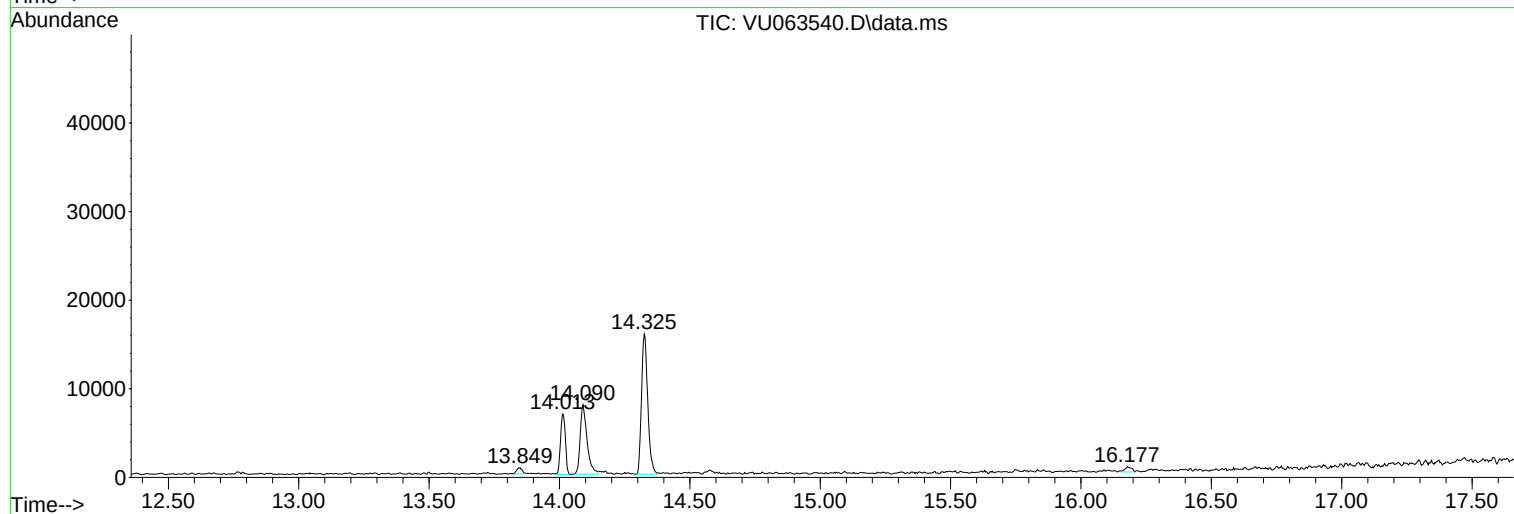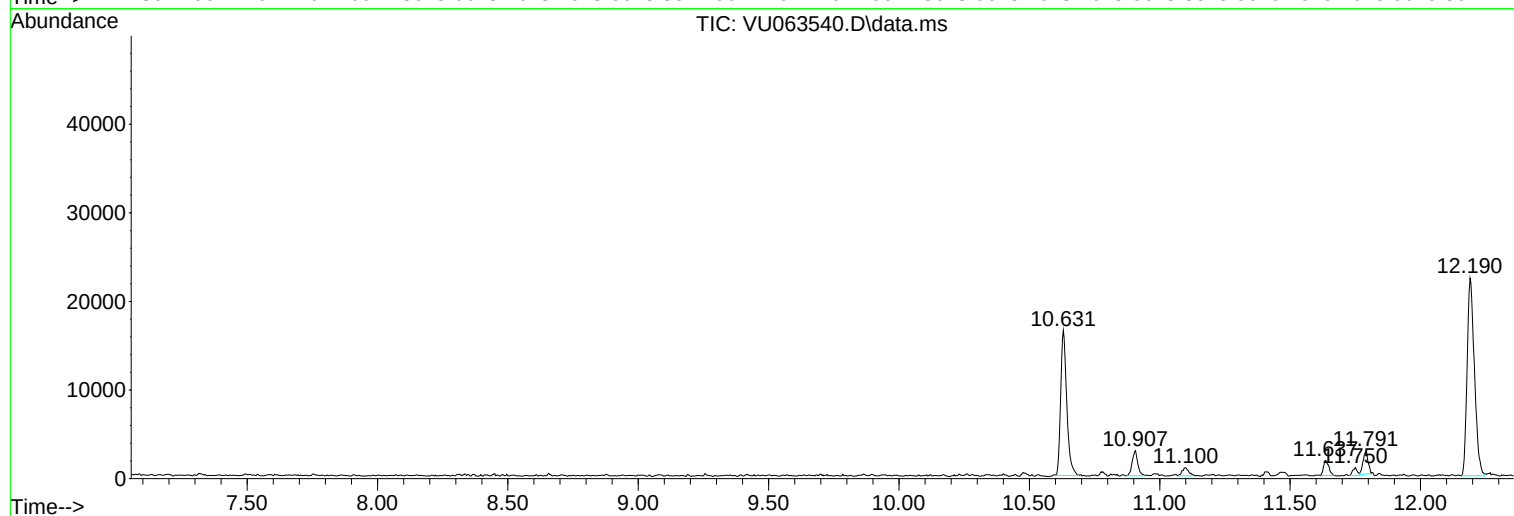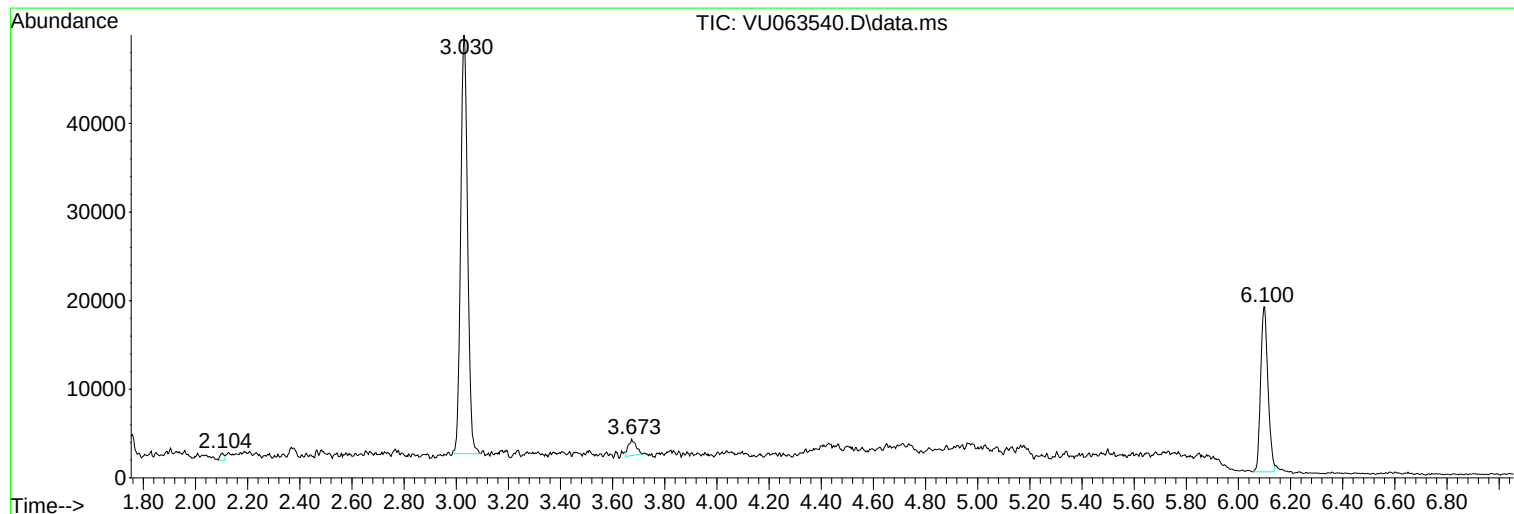

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
Data File : VU063540.D
Acq On : 18 Jul 2025 16:55
Operator : MD/SY
Sample : VIBLK
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
Data File : VU063540.D
Acq On : 18 Jul 2025 16:55
Operator : MD/SY
Sample : VIBLK
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------